

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
 Data File : BF130553.D
 Acq On : 06 Oct 2022 16:27
 Operator : CG\JU
 Sample : N4998-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 506D-2

Quant Time: Oct 07 02:10:57 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 07 02:06:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.616	152	76184	20.000	ng	0.00
21) Naphthalene-d8	7.898	136	298500	20.000	ng	# 0.00
39) Acenaphthene-d10	9.645	164	147662	20.000	ng	0.00
64) Phenanthrene-d10	11.127	188	218390	20.000	ng	0.00
76) Chrysene-d12	13.757	240	120698	20.000	ng	0.00
86) Perylene-d12	15.139	264	141905	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.216	112	271029	61.705	ng	0.00
7) Phenol-d6	6.257	99	198303	36.082	ng	-0.01
23) Nitrobenzene-d5	7.187	82	518126	88.678	ng	0.00
42) 2,4,6-Tribromophenol	10.439	330	191095	135.061	ng	0.00
45) 2-Fluorobiphenyl	8.975	172	964588	95.124	ng	0.00
79) Terphenyl-d14	12.716	244	705998	96.893	ng	0.00
Target Compounds						
74) Di-n-butylphthalate	11.698	149	306953	23.837	ng	Qvalue 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130553.D
Acq On : 06 Oct 2022 16:27
Operator : CG\JU
Sample : N4998-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
506D-2

Quant Time: Oct 07 02:10:57 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 07 02:06:46 2022
Response via : Initial Calibration



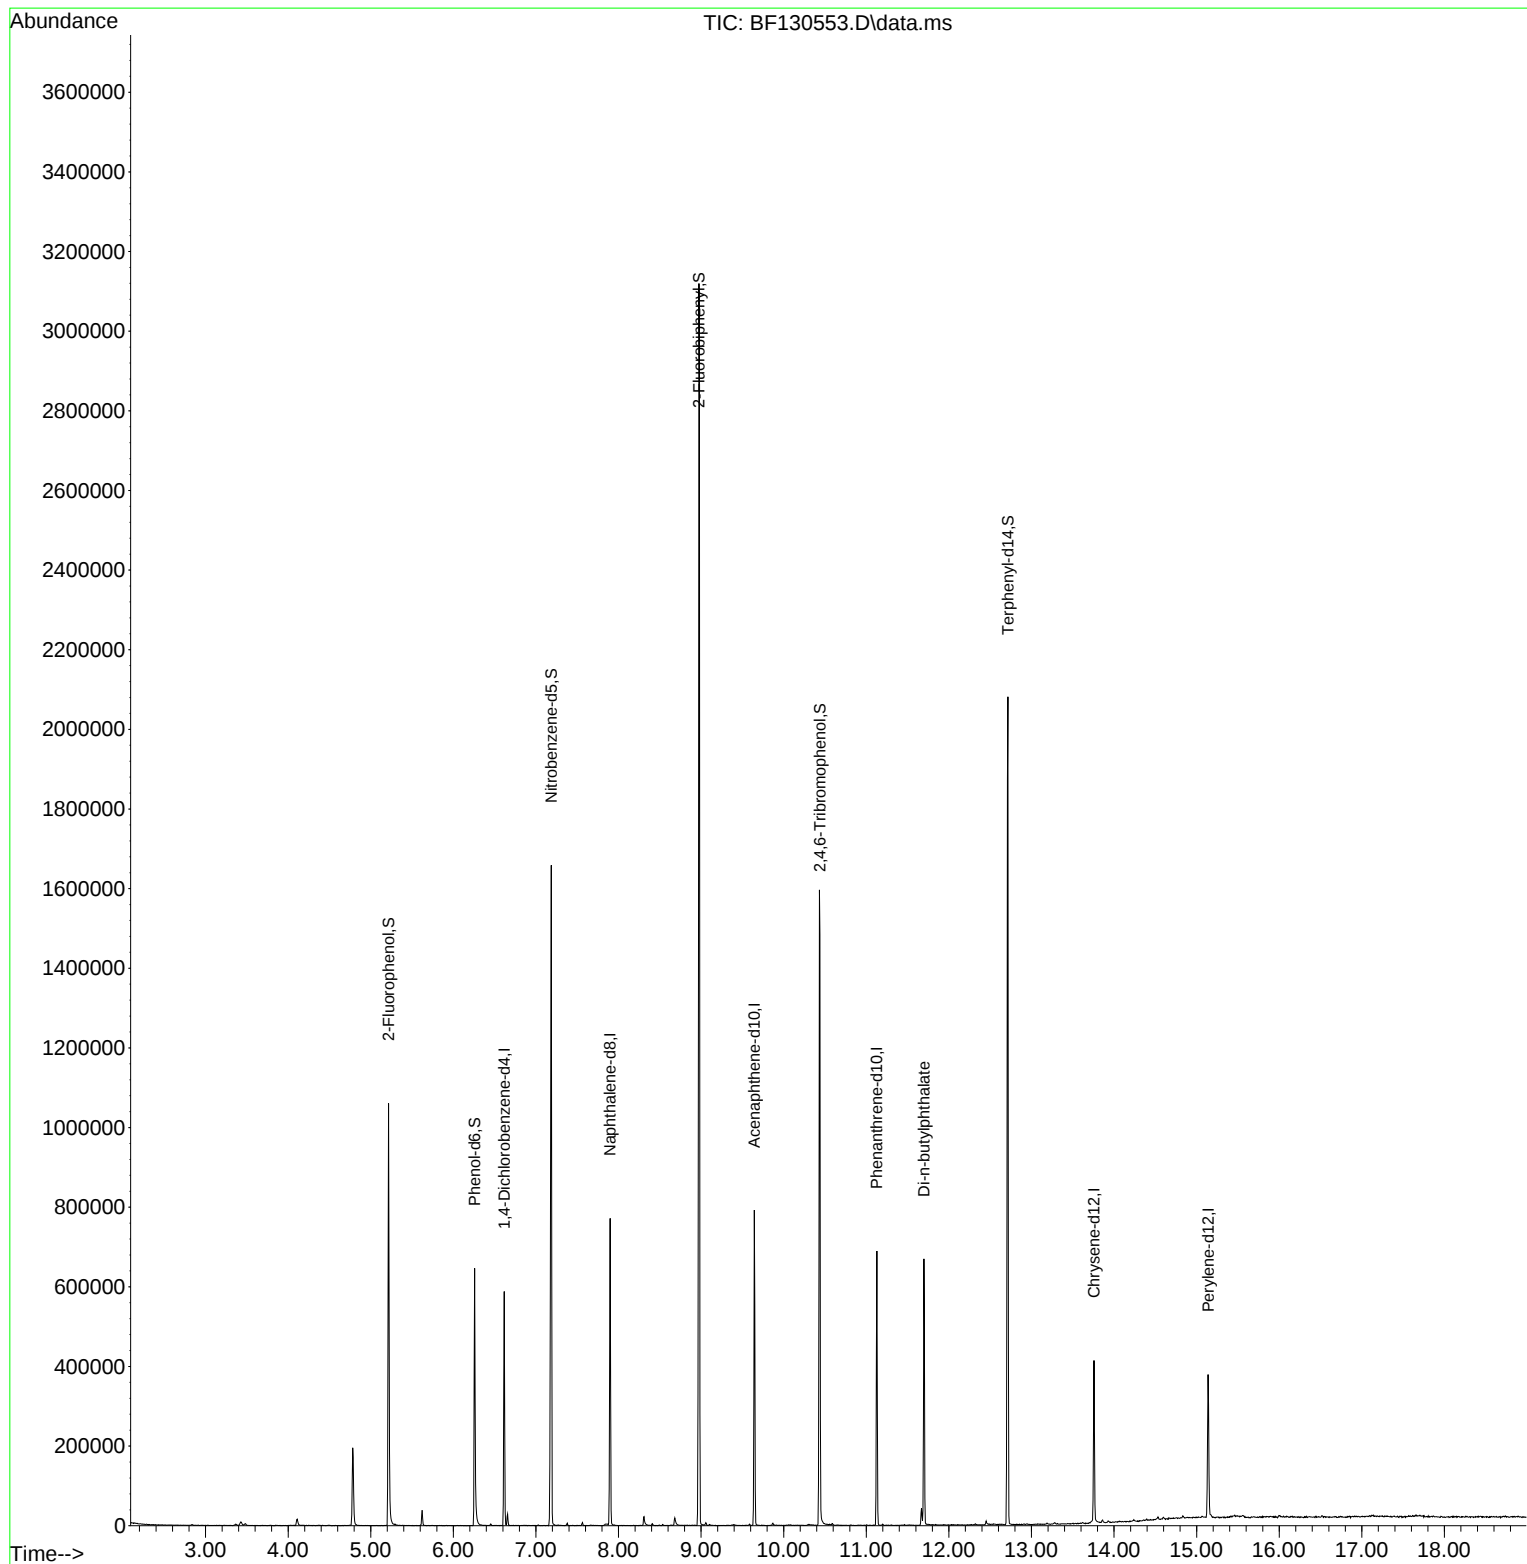




#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.616 min Scan# 71
 Delta R.T. -0.000 min
 Lab File: BF130553.D
 Acq: 06 Oct 2022 16:27




Instrument :
 BNA_F
 ClientSampleId :
 506D-2


Tgt Ion:152 Resp: 76184
 Ion Ratio Lower Upper
 152 100
 150 152.5 122.8 184.2
 115 65.8 53.8 80.8

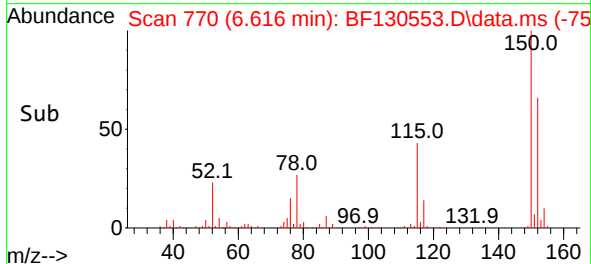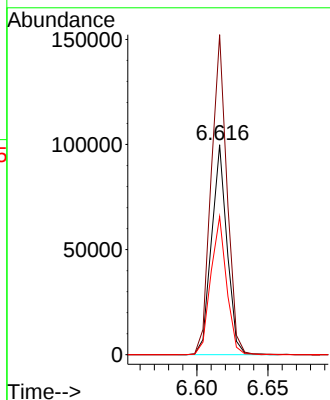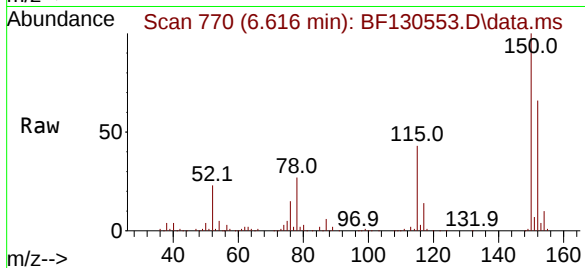

#5
 2-Fluorophenol
 Concen: 61.705 ng
 RT: 5.216 min Scan# 532
 Delta R.T. -0.000 min
 Lab File: BF130553.D
 Acq: 06 Oct 2022 16:27

Tgt Ion:112 Resp: 271029
 Ion Ratio Lower Upper
 112 100
 64 60.1 51.4 77.0
 63 32.6 28.8 43.2


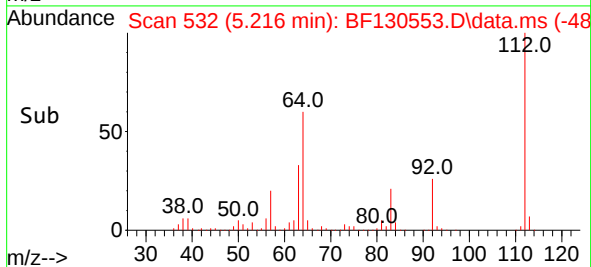
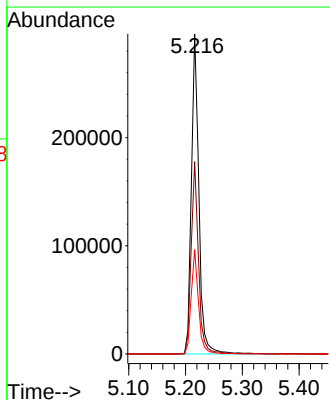
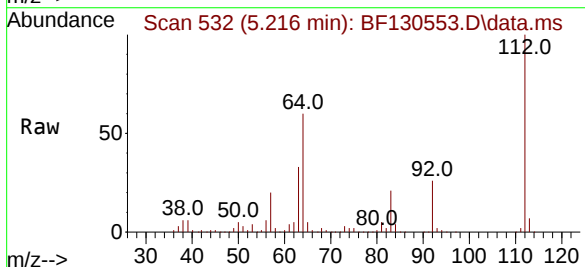


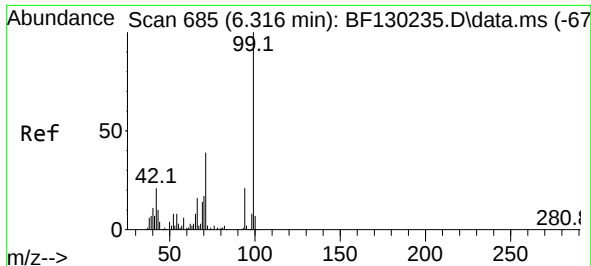

#7
Phenol-d6
Concen: 36.082 ng
RT: 6.257 min Scan# 709
Delta R.T. -0.012 min
Lab File: BF130553.D
Acq: 06 Oct 2022 16:27




Instrument :
BNA_F
ClientSampleId :
506D-2


Tgt Ion: 99 Resp: 198303
Ion Ratio Lower Upper
99 100
42 18.5 17.0 25.6
71 36.8 32.3 48.5

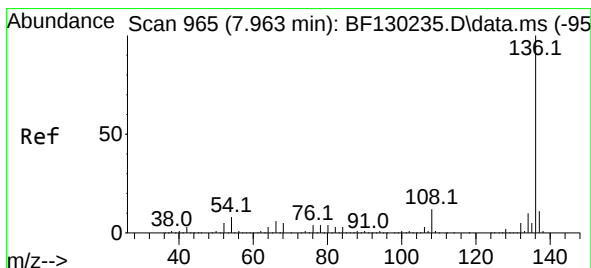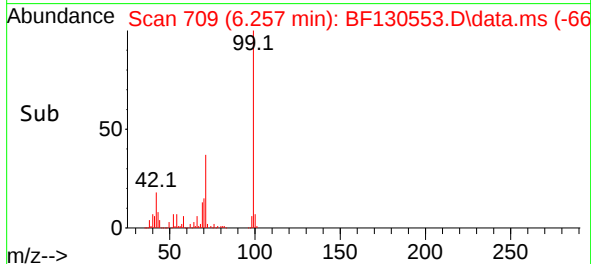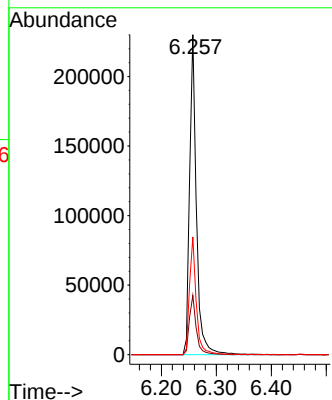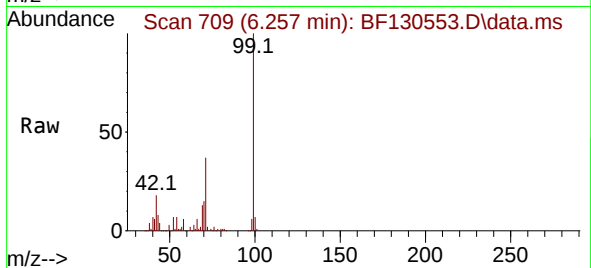

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.898 min Scan# 988
Delta R.T. -0.006 min
Lab File: BF130553.D
Acq: 06 Oct 2022 16:27

Tgt Ion: 136 Resp: 298500
Ion Ratio Lower Upper
136 100
137 10.7 9.1 13.7
54 6.9 7.1 10.7#
68 5.1 4.5 6.7

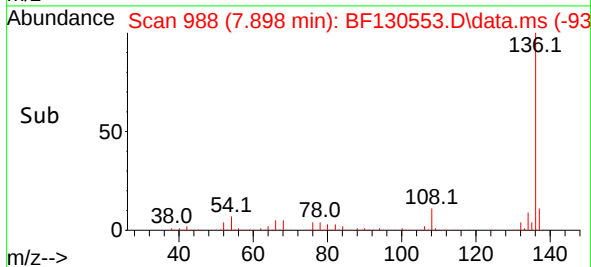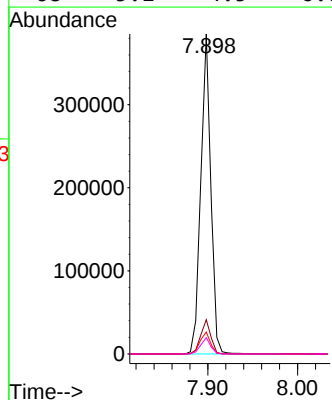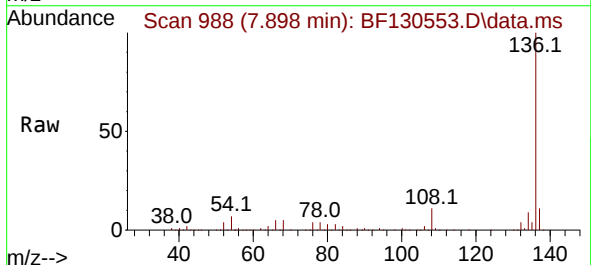

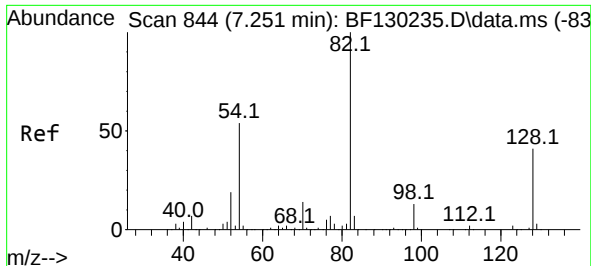

#23

Nitrobenzene-d5

Concen: 88.678 ng

RT: 7.187 min Scan# 8

Delta R.T. -0.006 min

Lab File: BF130553.D

Acq: 06 Oct 2022 16:27

Instrument :

BNA_F

ClientSampleId :

506D-2





Tgt Ion: 82 Resp: 518126

Ion Ratio Lower Upper

82 100

128 43.6 32.6 49.0

54 50.2 43.8 65.6

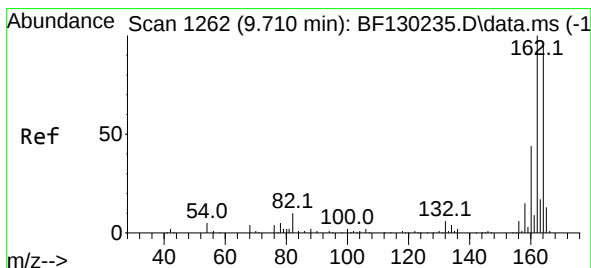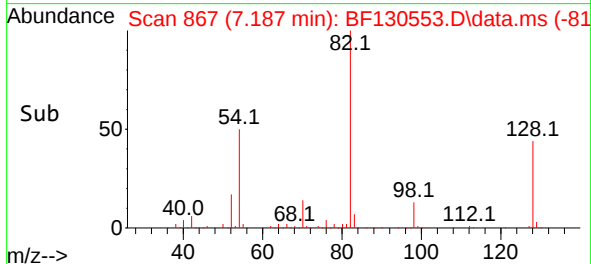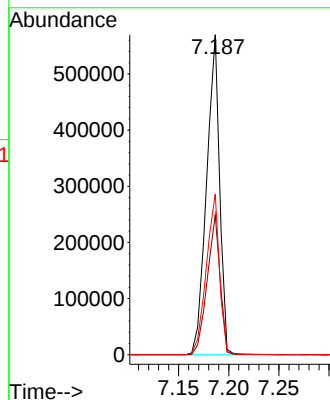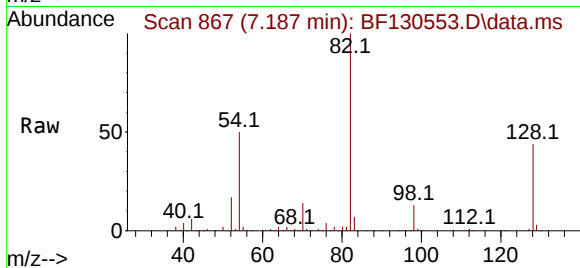

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.645 min Scan# 1285

Delta R.T. -0.006 min

Lab File: BF130553.D

Acq: 06 Oct 2022 16:27




Tgt Ion:164 Resp: 147662


Ion Ratio Lower Upper

164 100

162 103.3 81.4 122.0

160 45.4 36.2 54.4


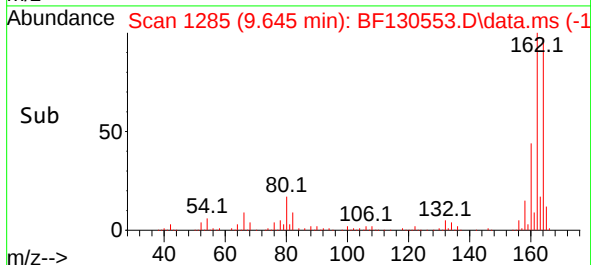
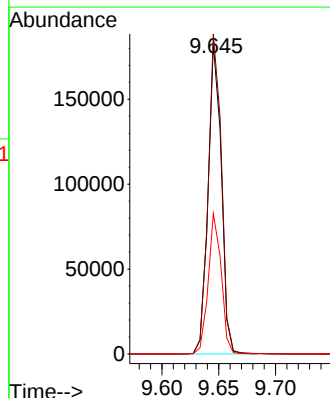
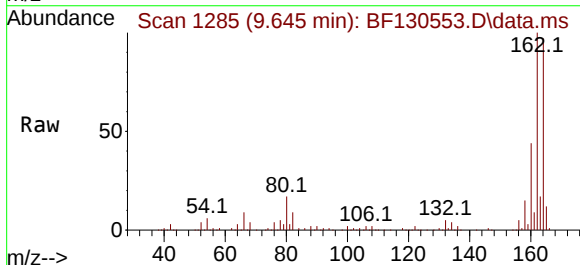


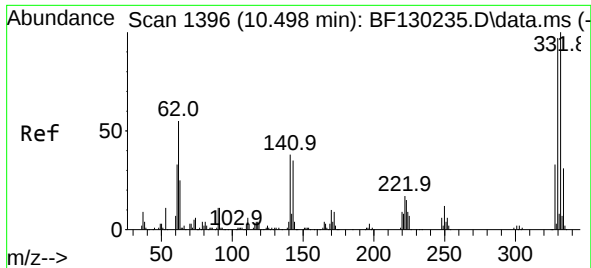

#42
2,4,6-Tribromophenol
Concen: 135.061 ng
RT: 10.439 min Scan# 14
Delta R.T. -0.000 min
Lab File: BF130553.D
Acq: 06 Oct 2022 16:27




Instrument :
BNA_F
ClientSampleId :
506D-2


Tgt Ion:330 Resp: 191095
Ion Ratio Lower Upper
330 100
332 103.6 83.4 125.2
141 35.9 34.0 51.0

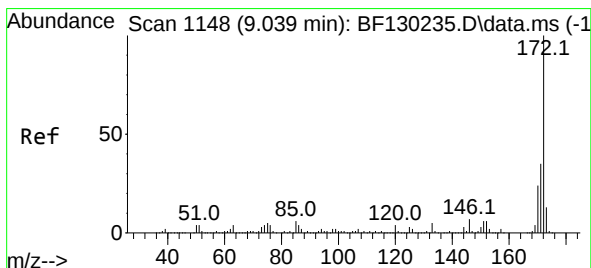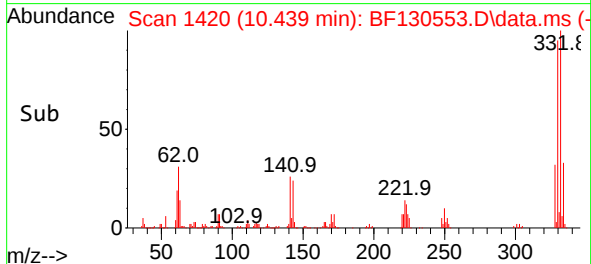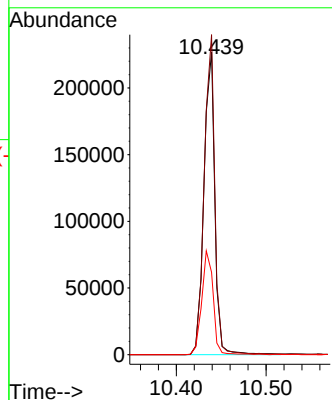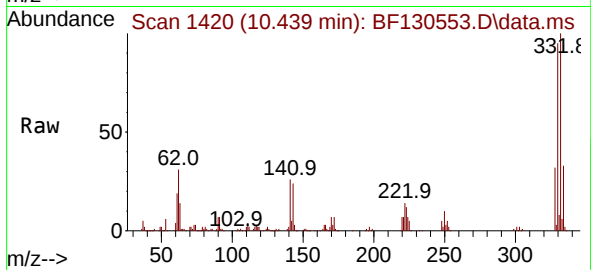

#45
2-Fluorobiphenyl
Concen: 95.124 ng
RT: 8.975 min Scan# 1171
Delta R.T. -0.006 min
Lab File: BF130553.D
Acq: 06 Oct 2022 16:27

Tgt Ion:172 Resp: 964588
Ion Ratio Lower Upper
172 100
171 35.0 28.3 42.5
170 22.9 18.7 28.1


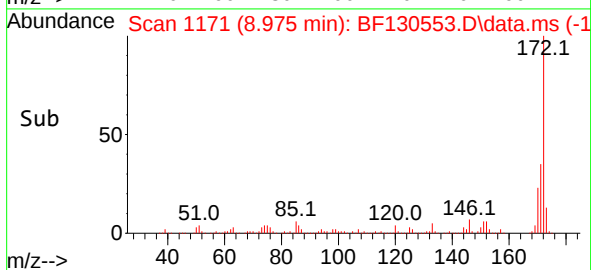
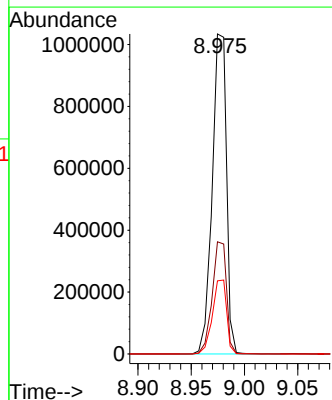
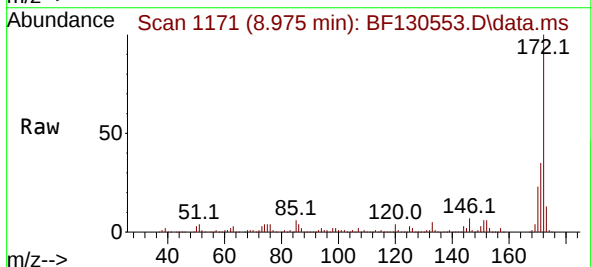


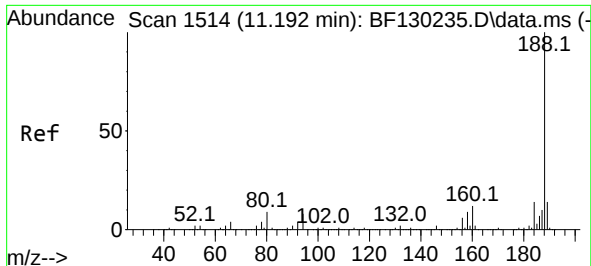

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.127 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF130553.D
Acq: 06 Oct 2022 16:27




Instrument :
BNA_F
ClientSampleId :
506D-2


Tgt Ion:188 Resp: 218390
Ion Ratio Lower Upper
188 100
94 8.9 7.4 11.2
80 9.0 7.9 11.9

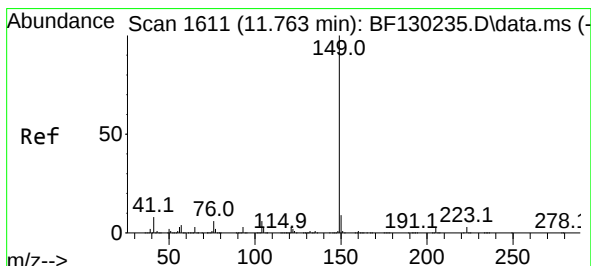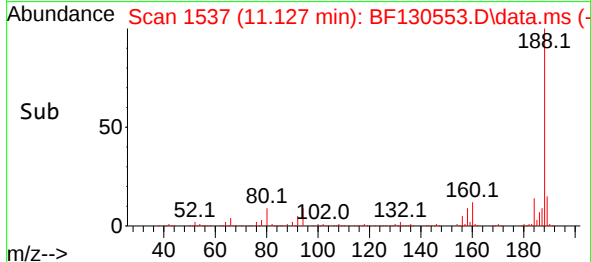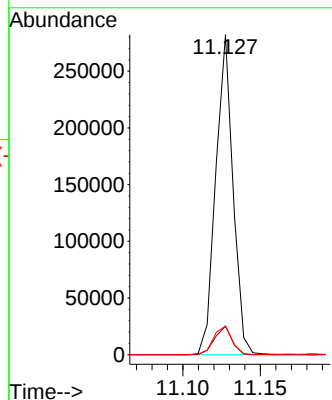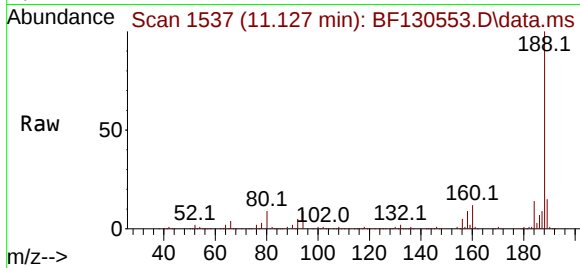

#74
Di-n-butylphthalate
Concen: 23.837 ng
RT: 11.698 min Scan# 1634
Delta R.T. -0.006 min
Lab File: BF130553.D
Acq: 06 Oct 2022 16:27

Tgt Ion:149 Resp: 306953
Ion Ratio Lower Upper
149 100
150 9.1 7.4 11.2
104 5.4 4.8 7.2


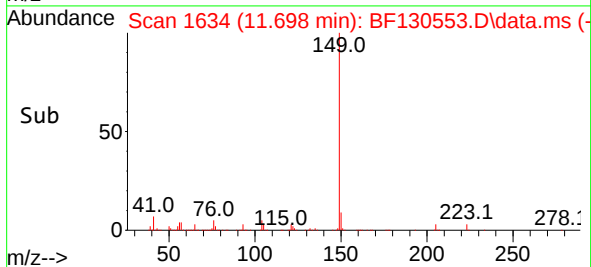
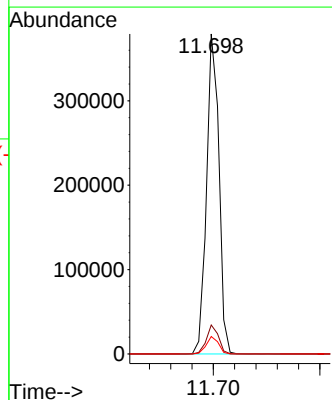
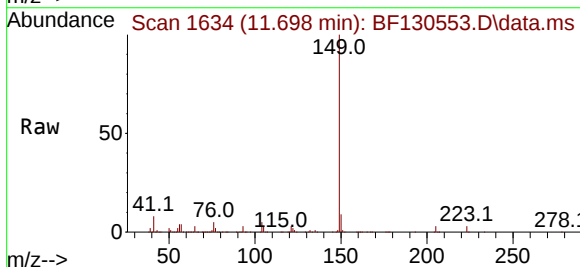


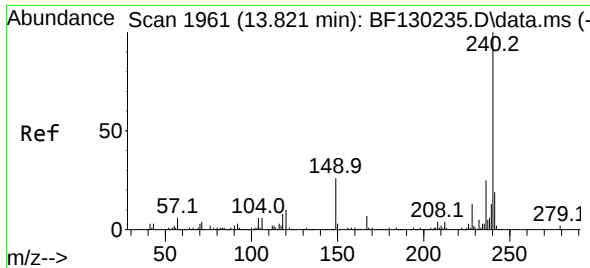

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.757 min Scan# 1807
Delta R.T. -0.006 min
Lab File: BF130553.D
Acq: 06 Oct 2022 16:27




Instrument :
BNA_F
ClientSampleId :
506D-2


Tgt Ion:240 Resp: 120698
Ion Ratio Lower Upper
240 100
120 10.3 8.7 13.1
236 26.1 20.9 31.3

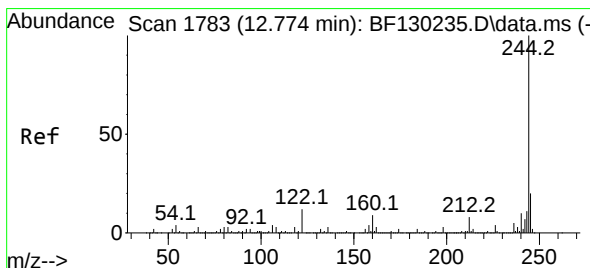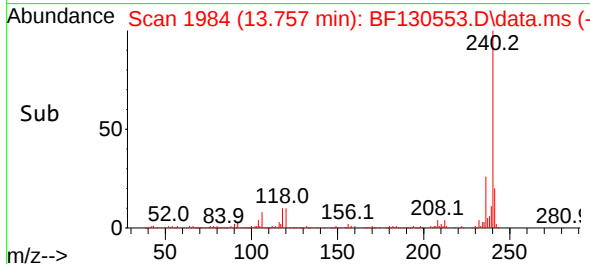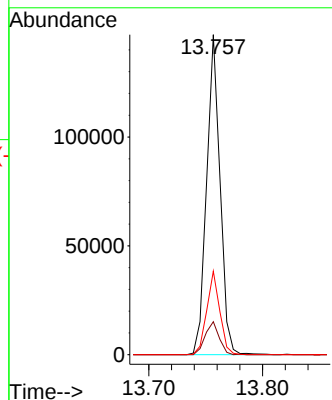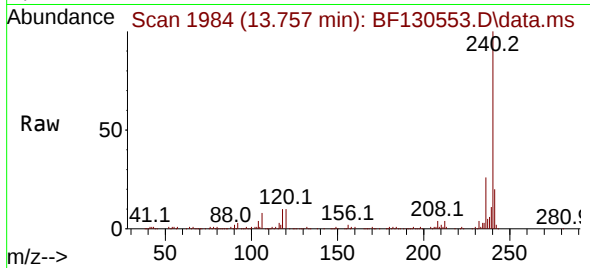

#79
Terphenyl-d14
Concen: 96.893 ng
RT: 12.716 min Scan# 1807
Delta R.T. -0.000 min
Lab File: BF130553.D
Acq: 06 Oct 2022 16:27


Tgt Ion:244 Resp: 705998
Ion Ratio Lower Upper
244 100
212 6.8 5.9 8.9
122 9.6 8.5 12.7

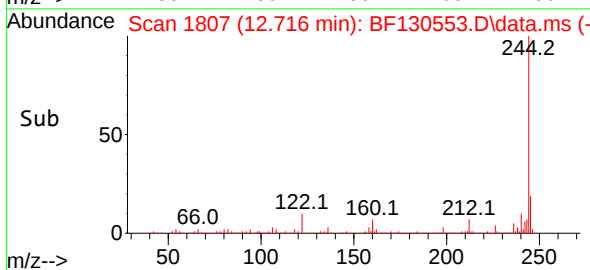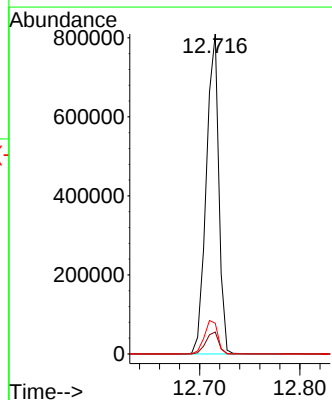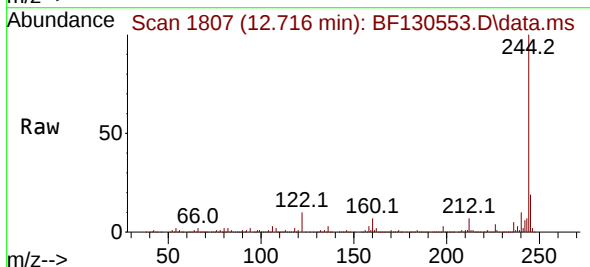

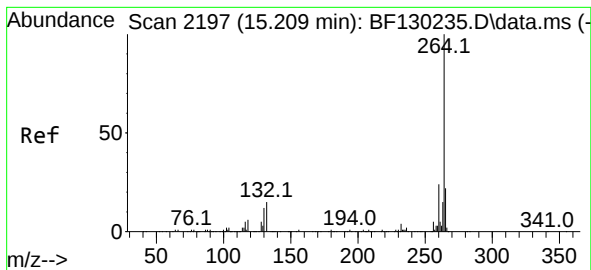

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.139 min Scan# 2197
 Delta R.T. -0.006 min
 Lab File: BF130553.D
 Acq: 06 Oct 2022 16:27

Instrument :
 BNA_F
 ClientSampleId :
 506D-2

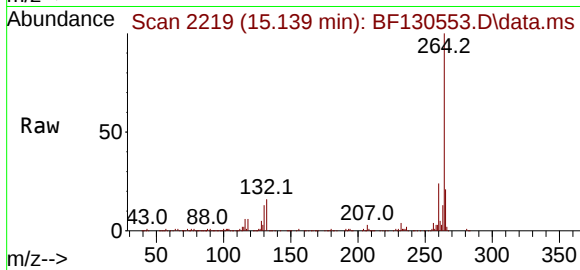

Tgt Ion:264 Resp: 141905
 Ion Ratio Lower Upper
 264 100
 260 23.7 19.3 28.9
 265 20.8 17.0 25.4

