

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
 Data File : BF130554.D
 Acq On : 06 Oct 2022 17:00
 Operator : CG\JU
 Sample : N5000-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 5486-4

Quant Time: Oct 07 02:11:08 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Oct 07 02:06:46 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.616	152	75758	20.000	ng	0.00
21) Naphthalene-d8	7.898	136	301507	20.000	ng	# 0.00
39) Acenaphthene-d10	9.645	164	151665	20.000	ng	0.00
64) Phenanthrene-d10	11.127	188	227876	20.000	ng	0.00
76) Chrysene-d12	13.757	240	129538	20.000	ng	0.00
86) Perylene-d12	15.139	264	146012	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.216	112	291106	66.648	ng	0.00
7) Phenol-d6	6.257	99	209774	38.384	ng	-0.01
23) Nitrobenzene-d5	7.186	82	534429	90.556	ng	0.00
42) 2,4,6-Tribromophenol	10.439	330	186089	128.051	ng	0.00
45) 2-Fluorobiphenyl	8.975	172	990980	95.148	ng	0.00
79) Terphenyl-d14	12.716	244	709265	90.699	ng	0.00
Target Compounds						
74) Di-n-butylphthalate	11.710	149	2267074	168.725	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130554.D
Acq On : 06 Oct 2022 17:00
Operator : CG\JU
Sample : N5000-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
5486-4

Quant Time: Oct 07 02:11:08 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 07 02:06:46 2022
Response via : Initial Calibration




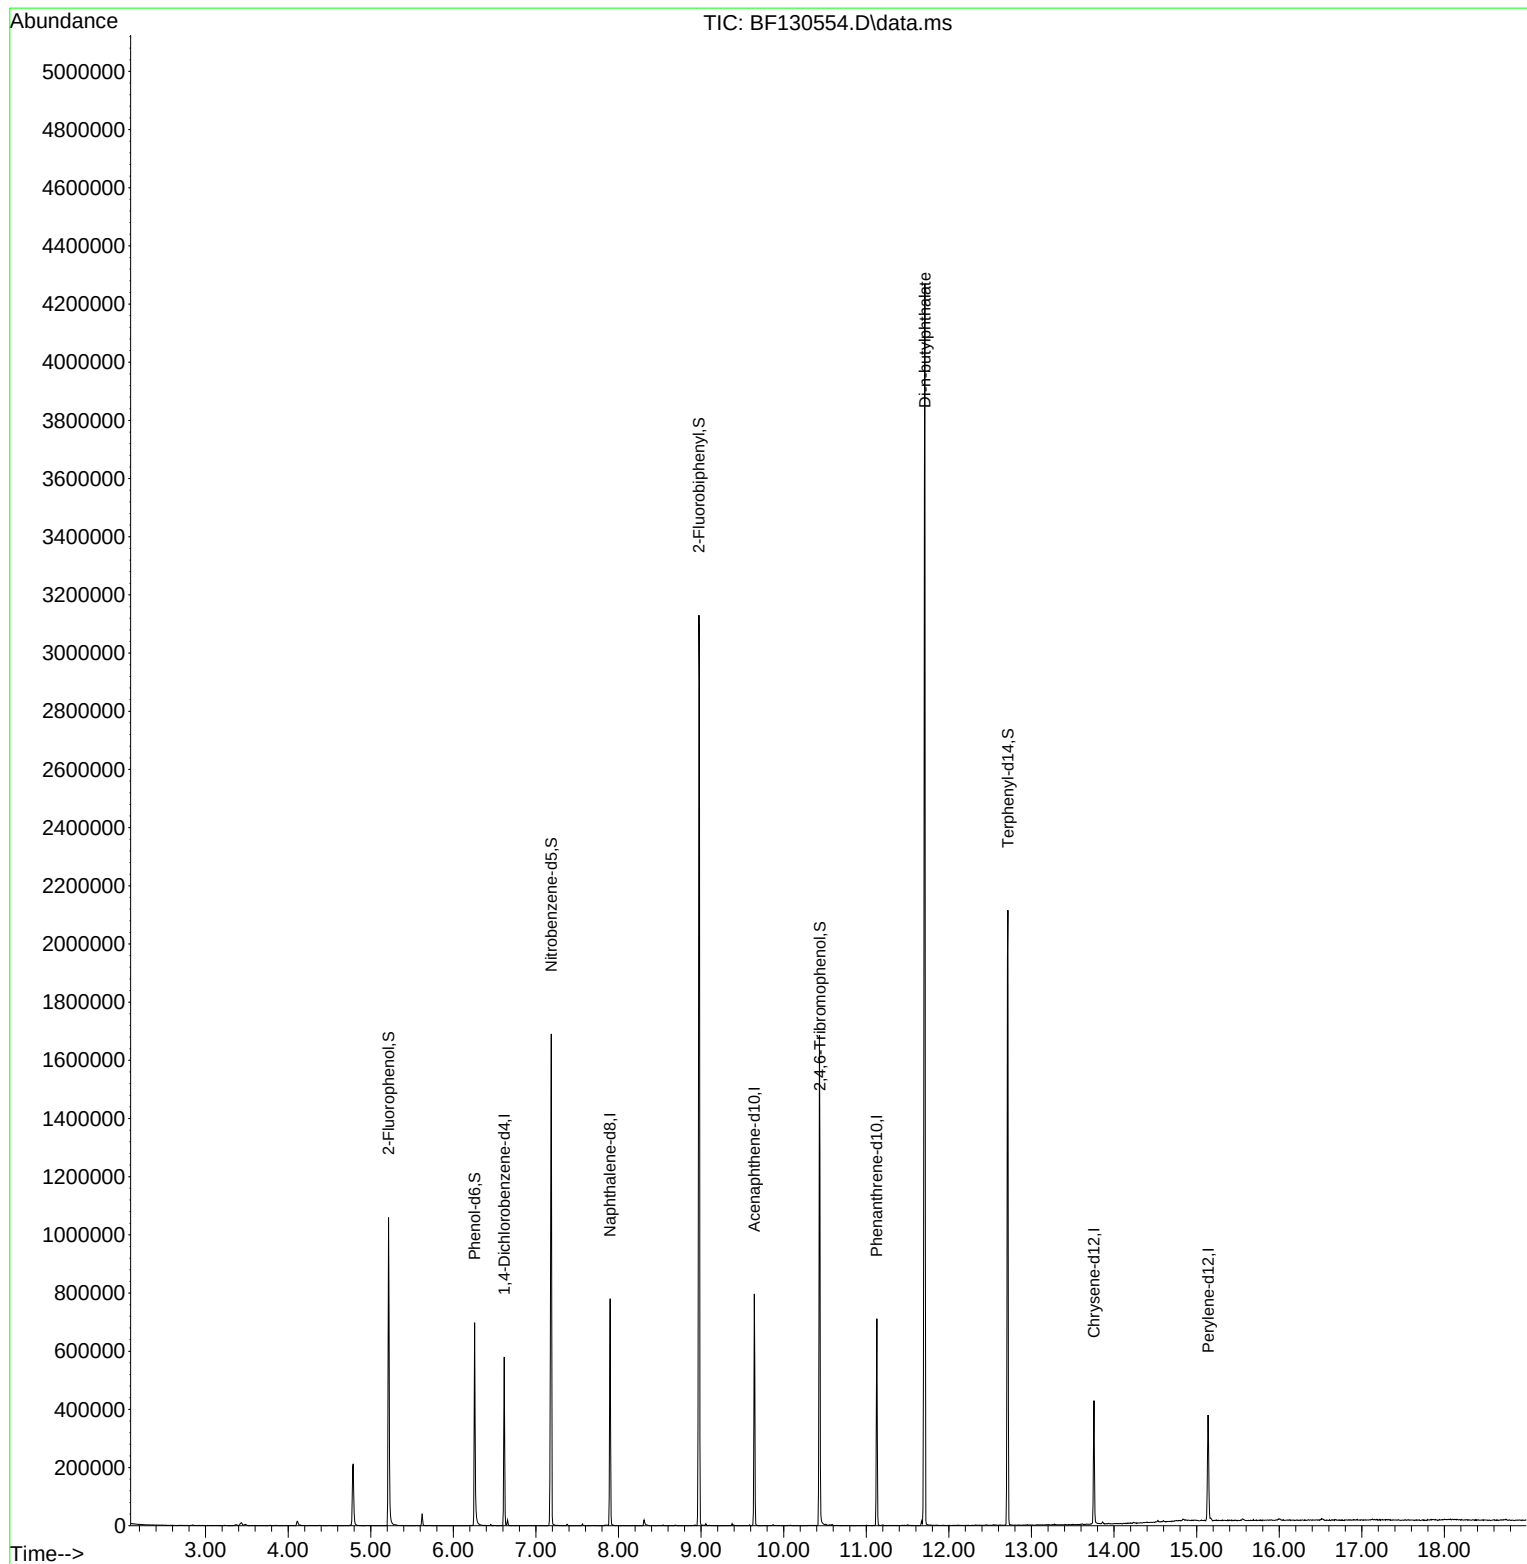


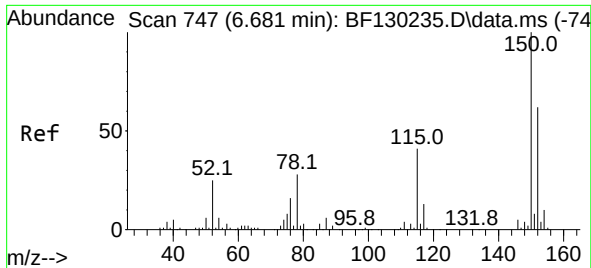

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.616 min Scan# 71
Delta R.T. -0.000 min
Lab File: BF130554.D
Acq: 06 Oct 2022 17:00




Instrument :
BNA_F
ClientSampleId :
5486-4


Tgt Ion:152 Resp: 75758
Ion Ratio Lower Upper
152 100
150 153.7 122.8 184.2
115 64.9 53.8 80.8

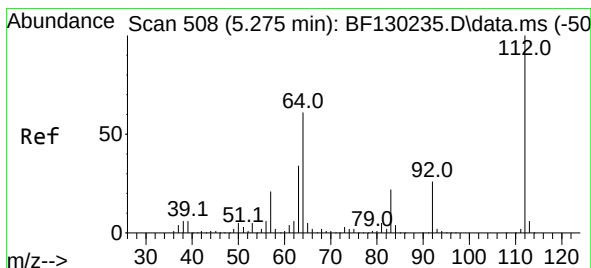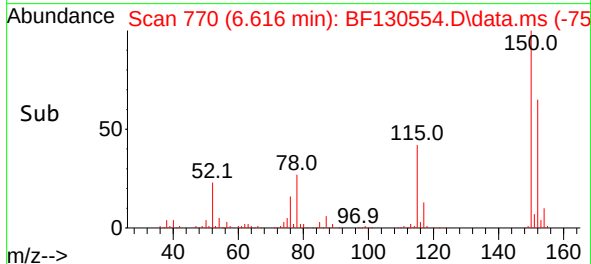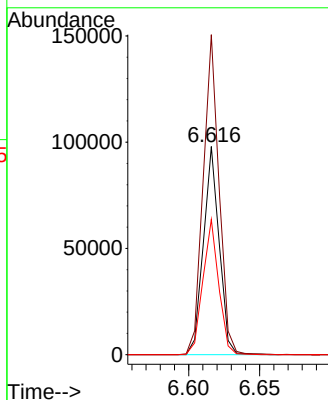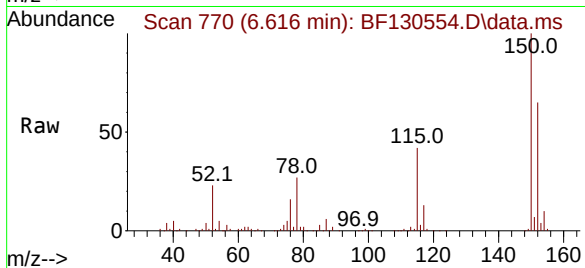

#5
2-Fluorophenol
Concen: 66.648 ng
RT: 5.216 min Scan# 532
Delta R.T. -0.000 min
Lab File: BF130554.D
Acq: 06 Oct 2022 17:00

Tgt Ion:112 Resp: 291106
Ion Ratio Lower Upper
112 100
64 60.7 51.4 77.0
63 32.7 28.8 43.2


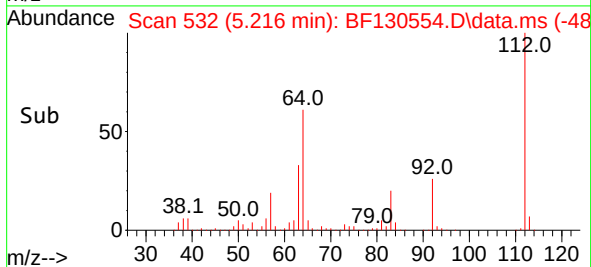
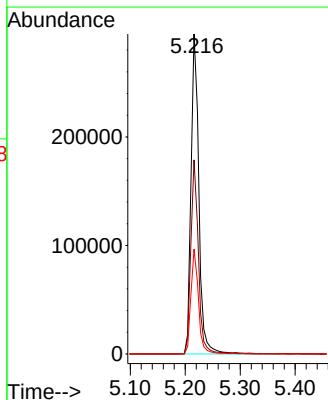
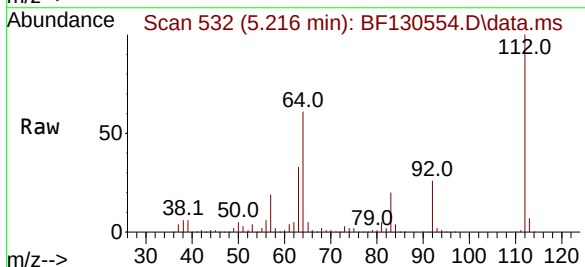


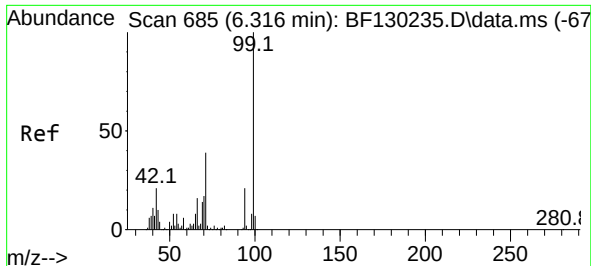

#7
Phenol-d6
Concen: 38.384 ng
RT: 6.257 min Scan# 709
Delta R.T. -0.012 min
Lab File: BF130554.D
Acq: 06 Oct 2022 17:00




Instrument :
BNA_F
ClientSampleId :
5486-4


Tgt Ion: 99 Resp: 209774
Ion Ratio Lower Upper
99 100
42 18.3 17.0 25.6
71 38.2 32.3 48.5

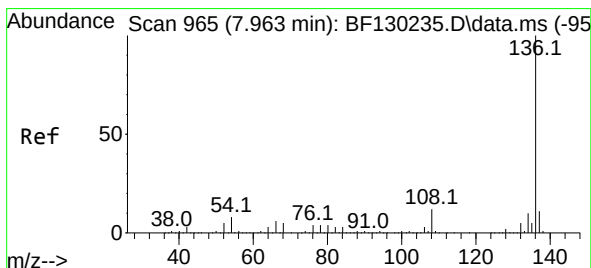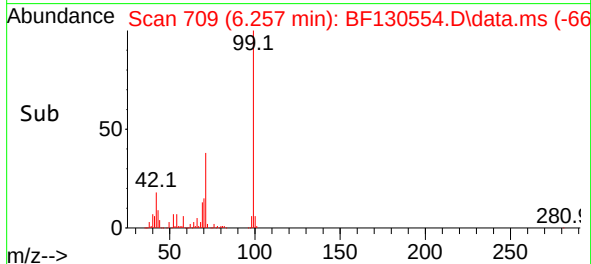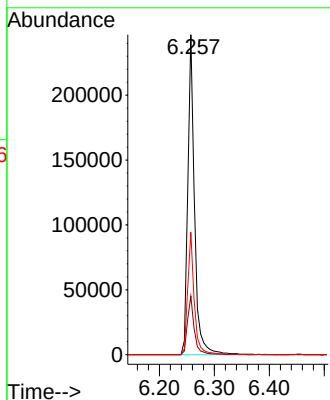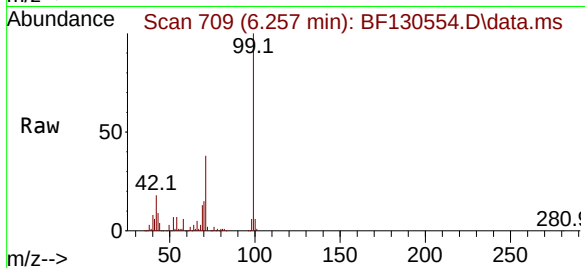

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.898 min Scan# 988
Delta R.T. -0.006 min
Lab File: BF130554.D
Acq: 06 Oct 2022 17:00

Tgt Ion: 136 Resp: 301507
Ion Ratio Lower Upper
136 100
137 10.7 9.1 13.7
54 6.9 7.1 10.7#
68 4.7 4.5 6.7

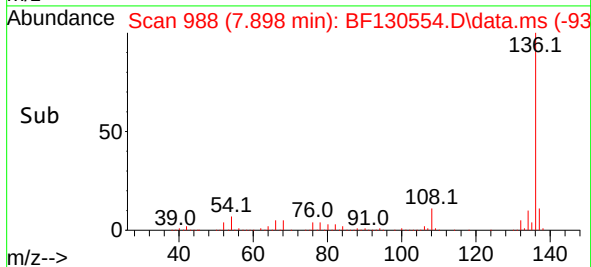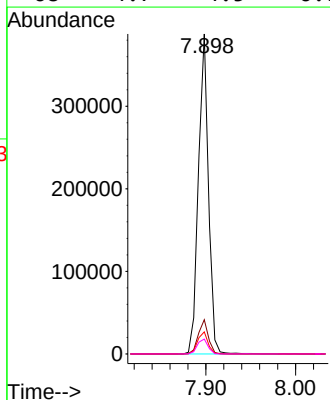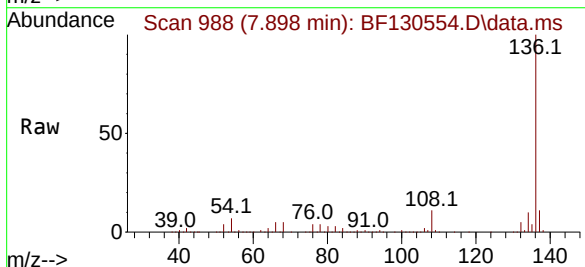

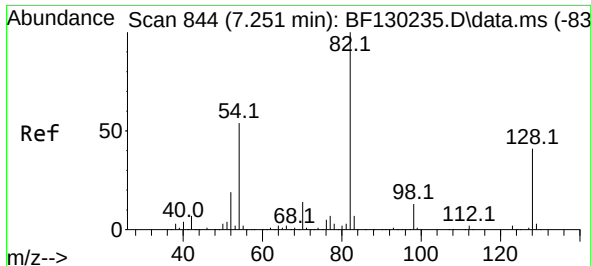

#23

Nitrobenzene-d5

Concen: 90.556 ng

RT: 7.186 min Scan# 81

Delta R.T. -0.006 min

Lab File: BF130554.D

Acq: 06 Oct 2022 17:00

Instrument :

BNA_F

ClientSampleId :

5486-4





Tgt Ion: 82 Resp: 534429

Ion Ratio Lower Upper

82 100

128 43.5 32.6 49.0

54 51.7 43.8 65.6

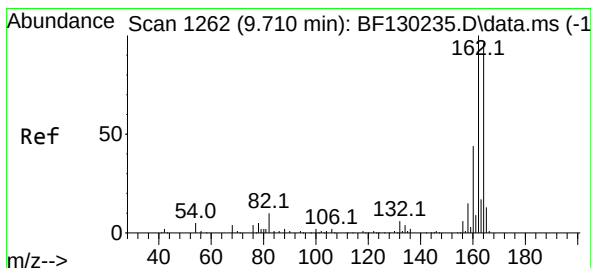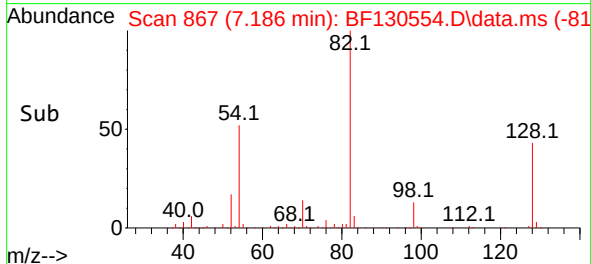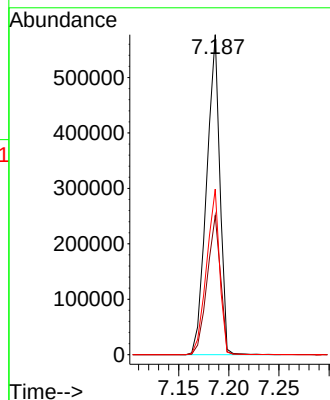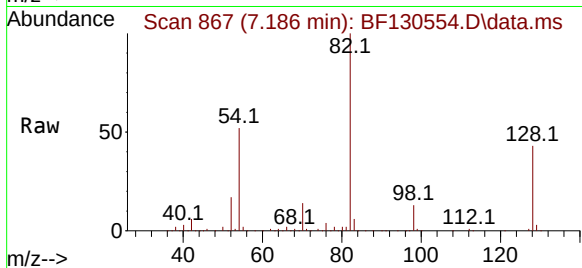

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.645 min Scan# 1285

Delta R.T. -0.006 min

Lab File: BF130554.D

Acq: 06 Oct 2022 17:00




Tgt Ion:164 Resp: 151665


Ion Ratio Lower Upper

164 100

162 100.9 81.4 122.0

160 43.8 36.2 54.4


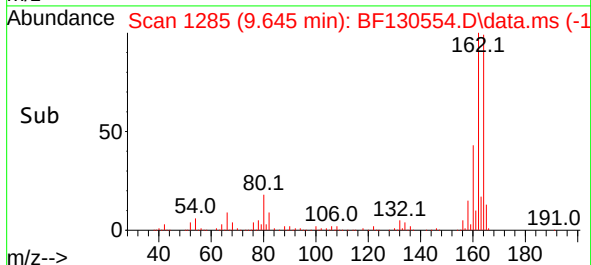
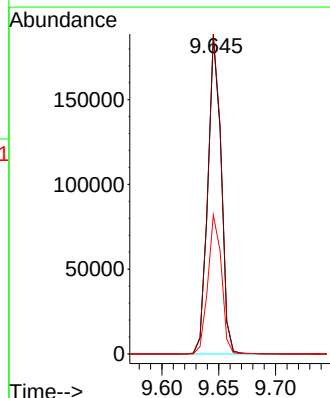
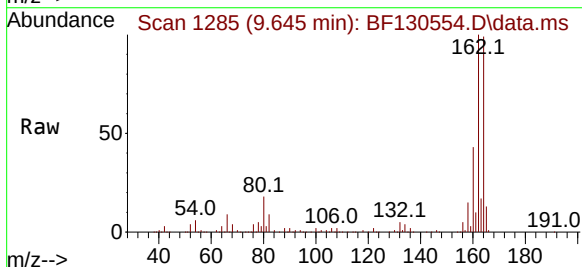


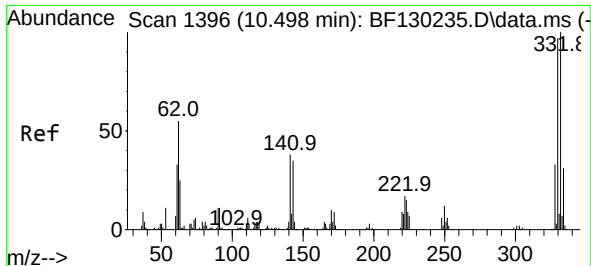

#42
2,4,6-Tribromophenol
Concen: 128.051 ng
RT: 10.439 min Scan# 1420
Delta R.T. -0.000 min
Lab File: BF130554.D
Acq: 06 Oct 2022 17:00




Instrument :
BNA_F
ClientSampleId :
5486-4


Tgt Ion:330 Resp: 186089
Ion Ratio Lower Upper
330 100
332 105.9 83.4 125.2
141 35.4 34.0 51.0

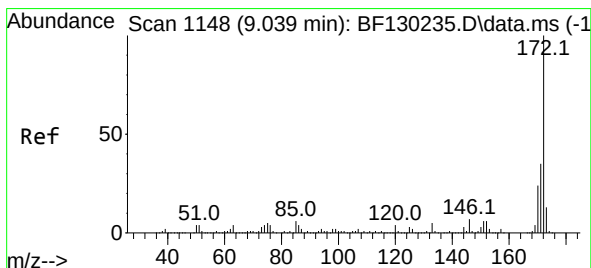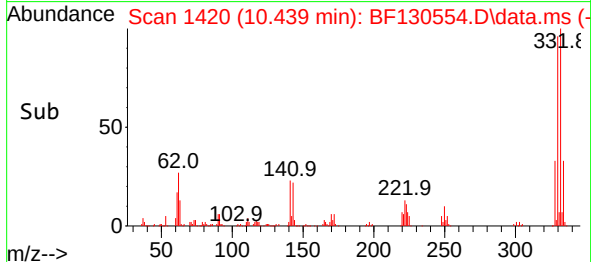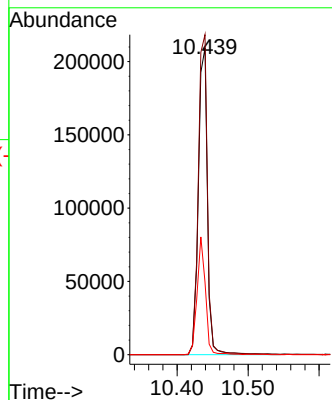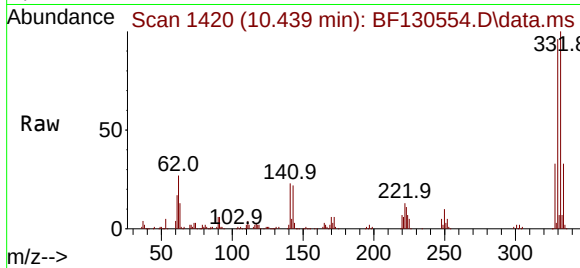

#45
2-Fluorobiphenyl
Concen: 95.148 ng
RT: 8.975 min Scan# 1171
Delta R.T. -0.006 min
Lab File: BF130554.D
Acq: 06 Oct 2022 17:00

Tgt Ion:172 Resp: 990980
Ion Ratio Lower Upper
172 100
171 34.8 28.3 42.5
170 23.2 18.7 28.1

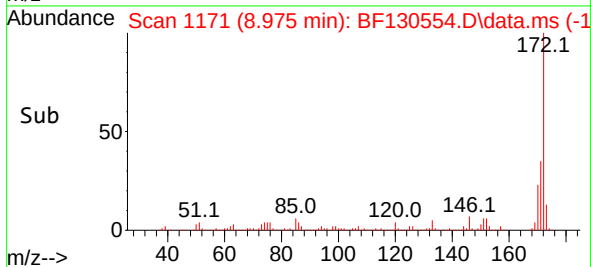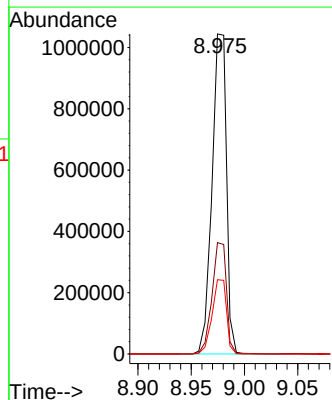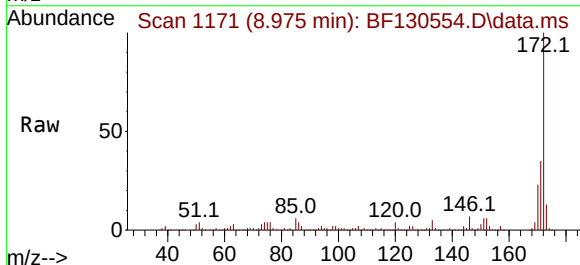

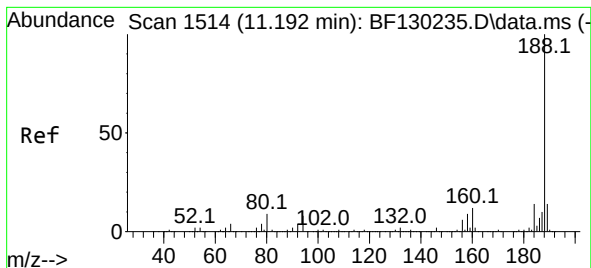

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.127 min Scan# 1

Delta R.T. -0.006 min

Lab File: BF130554.D

Acq: 06 Oct 2022 17:00

Instrument :

BNA_F

ClientSampleId :

5486-4





Tgt Ion:188 Resp: 227876

Ion Ratio Lower Upper

188 100

94 8.2 7.4 11.2

80 9.6 7.9 11.9

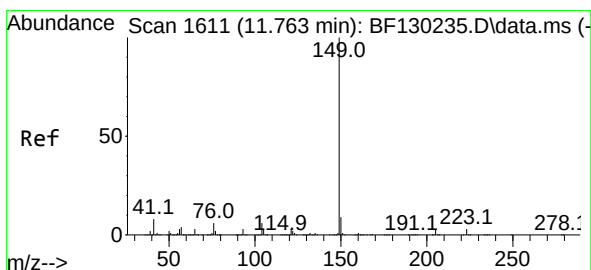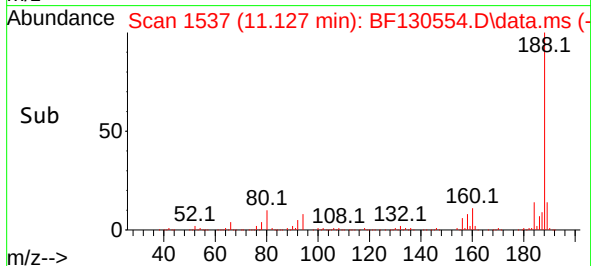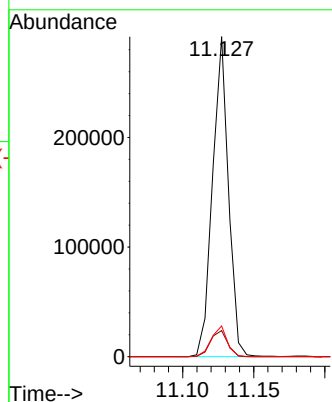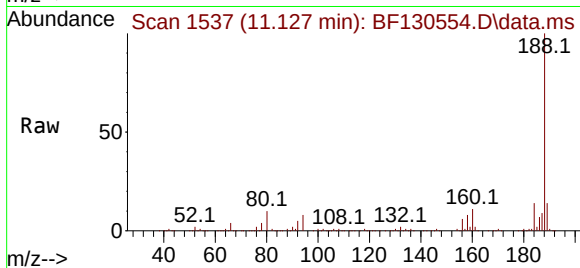

#74

Di-n-butylphthalate

Concen: 168.725 ng

RT: 11.710 min Scan# 1636

Delta R.T. 0.006 min

Lab File: BF130554.D

Acq: 06 Oct 2022 17:00




Tgt Ion:149 Resp: 2267074


Ion Ratio Lower Upper

149 100

150 9.8 7.4 11.2

104 5.4 4.8 7.2

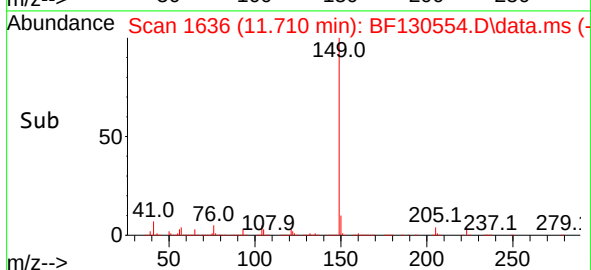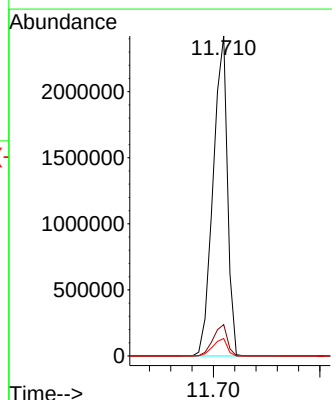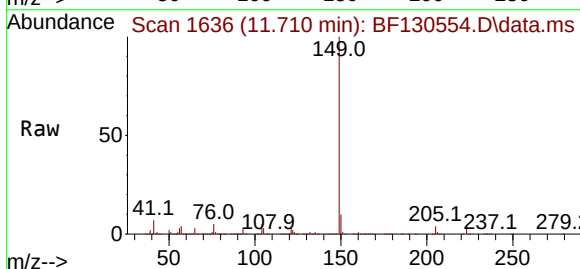

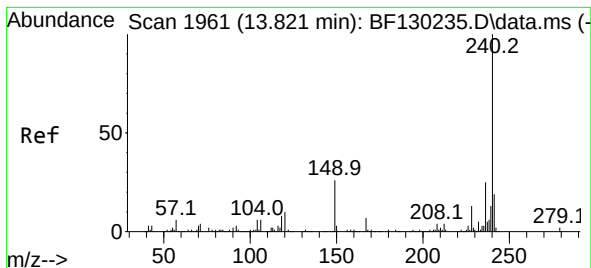

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.757 min Scan# 1961

Delta R.T. -0.006 min

Lab File: BF130554.D

Acq: 06 Oct 2022 17:00

Instrument :

BNA_F

ClientSampleId :

5486-4





Tgt Ion:240 Resp: 129538

Ion Ratio Lower Upper

240 100

120 10.1 8.7 13.1

236 24.9 20.9 31.3

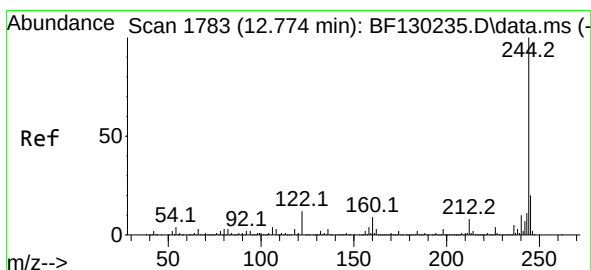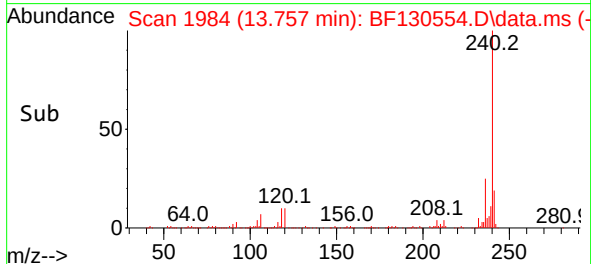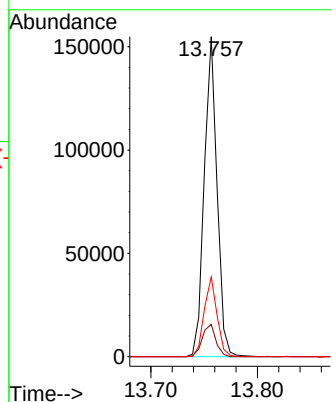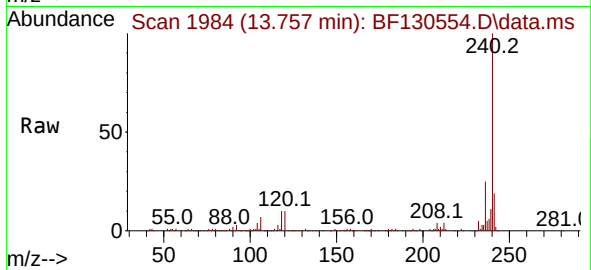

#79

Terphenyl-d14

Concen: 90.699 ng

RT: 12.716 min Scan# 1807

Delta R.T. -0.000 min

Lab File: BF130554.D

Acq: 06 Oct 2022 17:00




Tgt Ion:244 Resp: 709265


Ion Ratio Lower Upper

244 100

212 6.8 5.9 8.9


122 9.4 8.5 12.7

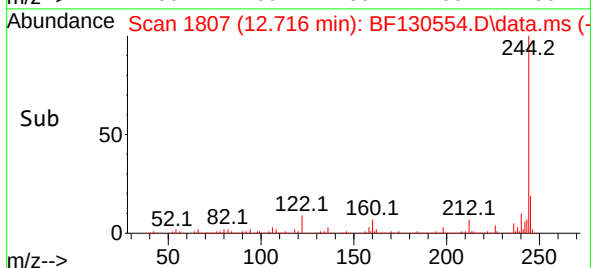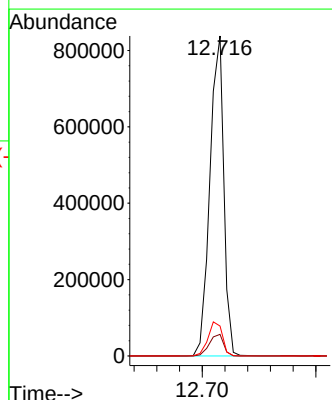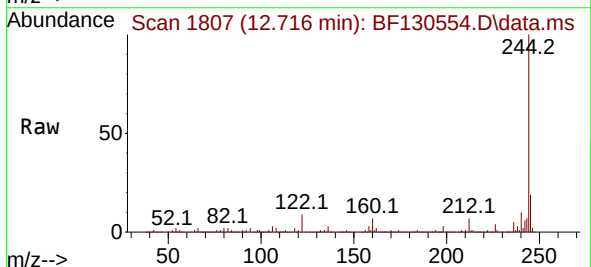

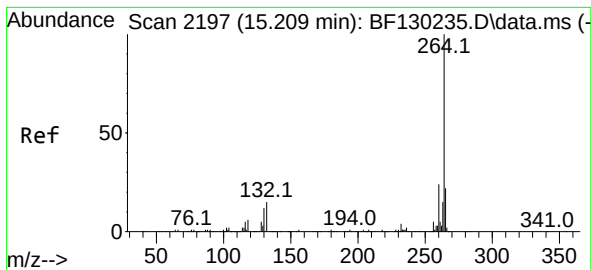

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.139 min Scan# 21
 Delta R.T. -0.006 min
 Lab File: BF130554.D
 Acq: 06 Oct 2022 17:00

Instrument :
 BNA_F
 ClientSampleId :
 5486-4

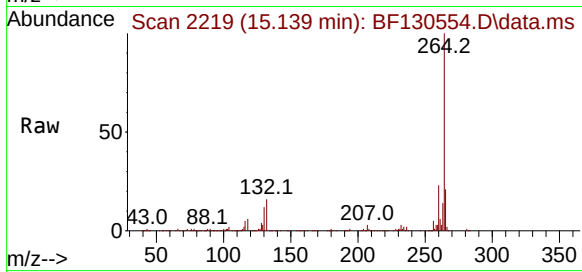

Tgt Ion:264 Resp: 146012
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.3 28.9
 265 21.3 17.0 25.4

