

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
 Data File : BF130547.D
 Acq On : 06 Oct 2022 12:50
 Operator : CG\JU
 Sample : PB148116BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB148116BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130547.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.822	461	465	475	rBV	30018	43576	1.41%	0.241%
2	5.228	529	534	537	rBV	2499571	2351323	76.19%	12.980%
3	6.263	705	710	713	rBV	2232273	2391402	77.48%	13.201%
4	6.616	766	770	773	rBV	735437	572410	18.55%	3.160%
5	7.187	862	867	870	rBV	1628990	1566883	50.77%	8.649%
6	7.898	983	988	991	rBV	925006	776043	25.14%	4.284%
7	8.981	1166	1172	1175	rBV	3505805	3086279	100.00%	17.037%
8	9.645	1281	1285	1289	rBV	1037658	880252	28.52%	4.859%
9	10.439	1415	1420	1423	rBV	2219553	1851924	60.01%	10.223%
10	11.127	1533	1537	1540	rBV	1110906	857624	27.79%	4.734%
11	12.716	1803	1807	1810	rBV	3261295	2767490	89.67%	15.277%
12	13.757	1980	1984	1988	rBV	616870	519175	16.82%	2.866%
13	15.145	2215	2220	2223	rBV	363387	417535	13.53%	2.305%
14	15.762	2319	2325	2334	rVB5	11129	33747	1.09%	0.186%




Sum of corrected areas: 18115663

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130547.D
Acq On : 06 Oct 2022 12:50
Operator : CG\JU
Sample : PB148116BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148116BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

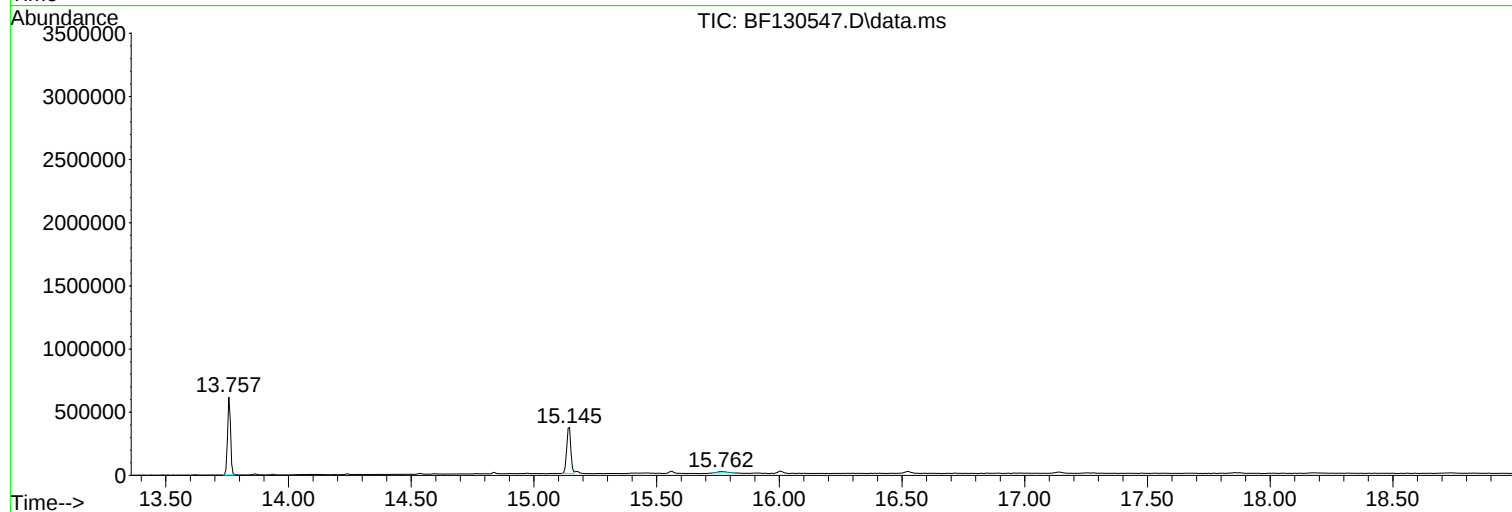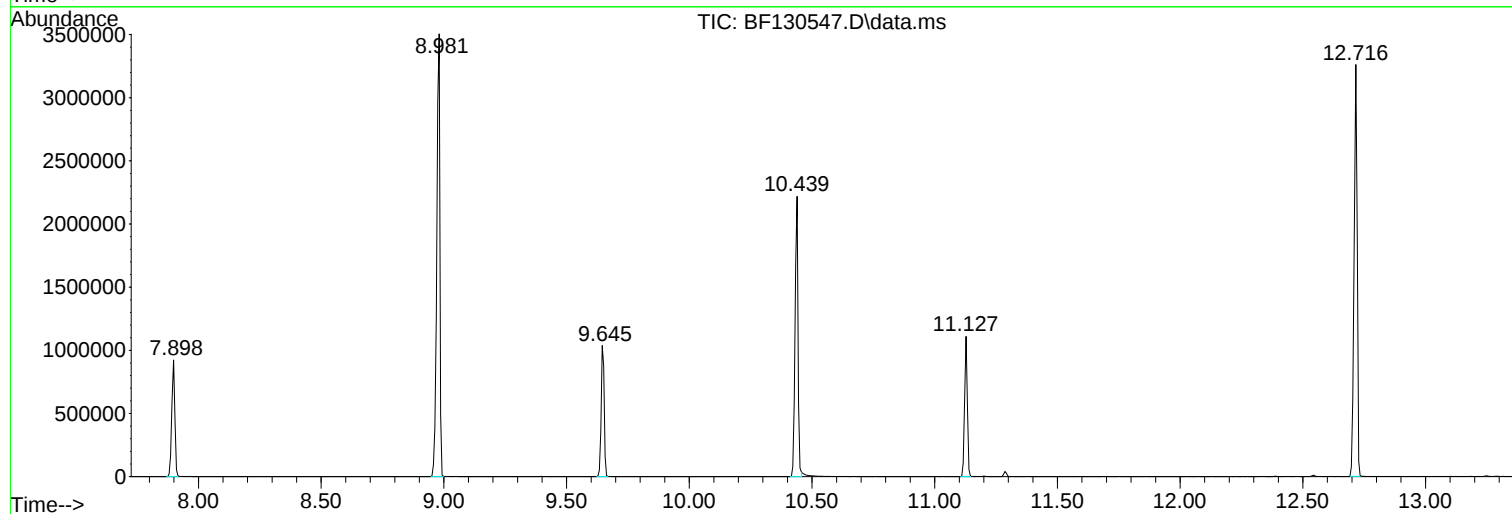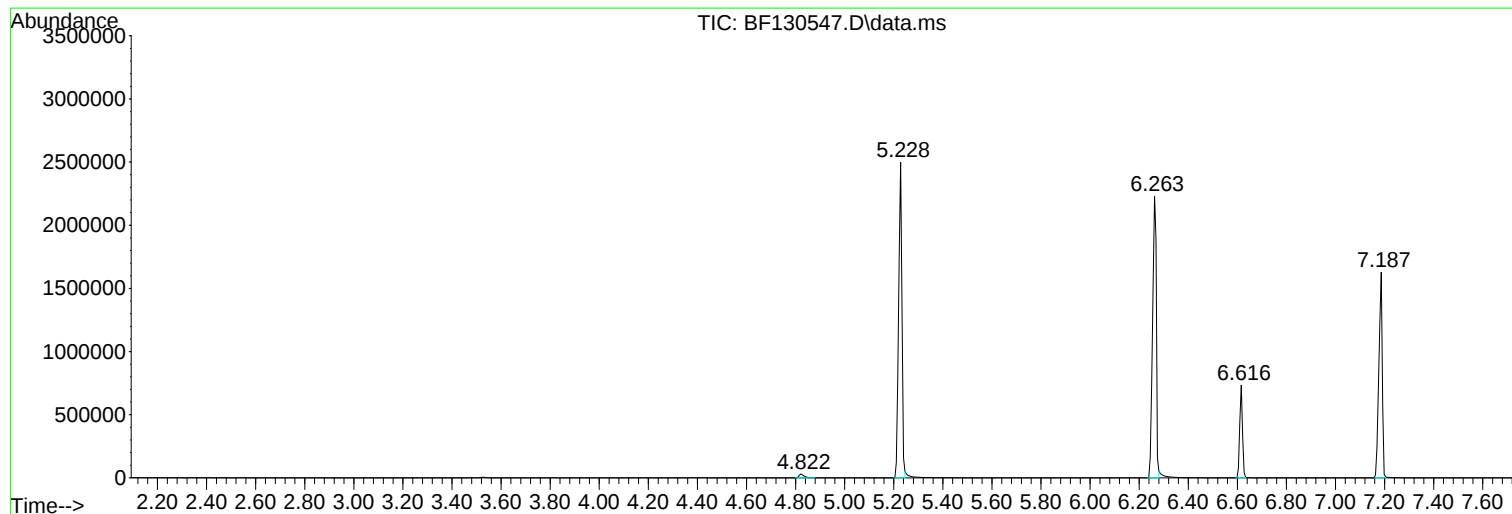

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130547.D
Acq On : 06 Oct 2022 12:50
Operator : CG\JU
Sample : PB148116BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148116BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130547.D
Acq On : 06 Oct 2022 12:50
Operator : CG\JU
Sample : PB148116BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148116BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------