

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
 Data File : BF130553.D
 Acq On : 06 Oct 2022 16:27
 Operator : CG\JU
 Sample : N4998-01
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 506D-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130553.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.781	454	458	468	rVB	194905	225958	7.98%	1.737%
2	5.216	528	532	544	rBV	1059446	951438	33.61%	7.312%
3	5.622	598	601	605	rBV	38328	32121	1.13%	0.247%
4	6.257	706	709	726	rBV	645882	574116	20.28%	4.412%
5	6.616	766	770	774	rBV	587748	458406	16.19%	3.523%
6	7.187	862	867	870	rBV	1655481	1503381	53.11%	11.554%
7	7.898	984	988	991	rBV	769151	598774	21.15%	4.602%
8	8.975	1167	1171	1174	rBV	3118567	2830780	100.00%	21.755%
9	9.645	1281	1285	1289	rBV	791771	633321	22.37%	4.867%
10	10.433	1415	1419	1423	rBV	1595629	1466187	51.79%	11.268%
11	11.127	1533	1537	1540	rBV	689077	539890	19.07%	4.149%
12	11.669	1626	1629	1631	rBV	42784	40462	1.43%	0.311%
13	11.698	1631	1634	1638	rVB	666445	534356	18.88%	4.107%
14	12.716	1802	1807	1810	rBV	2079105	1899014	67.08%	14.594%
15	13.757	1980	1984	1988	rBV	402736	337049	11.91%	2.590%
16	15.139	2215	2219	2224	rBV	358897	386905	13.67%	2.973%




Sum of corrected areas: 13012158

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130553.D
Acq On : 06 Oct 2022 16:27
Operator : CG\JU
Sample : N4998-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
506D-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

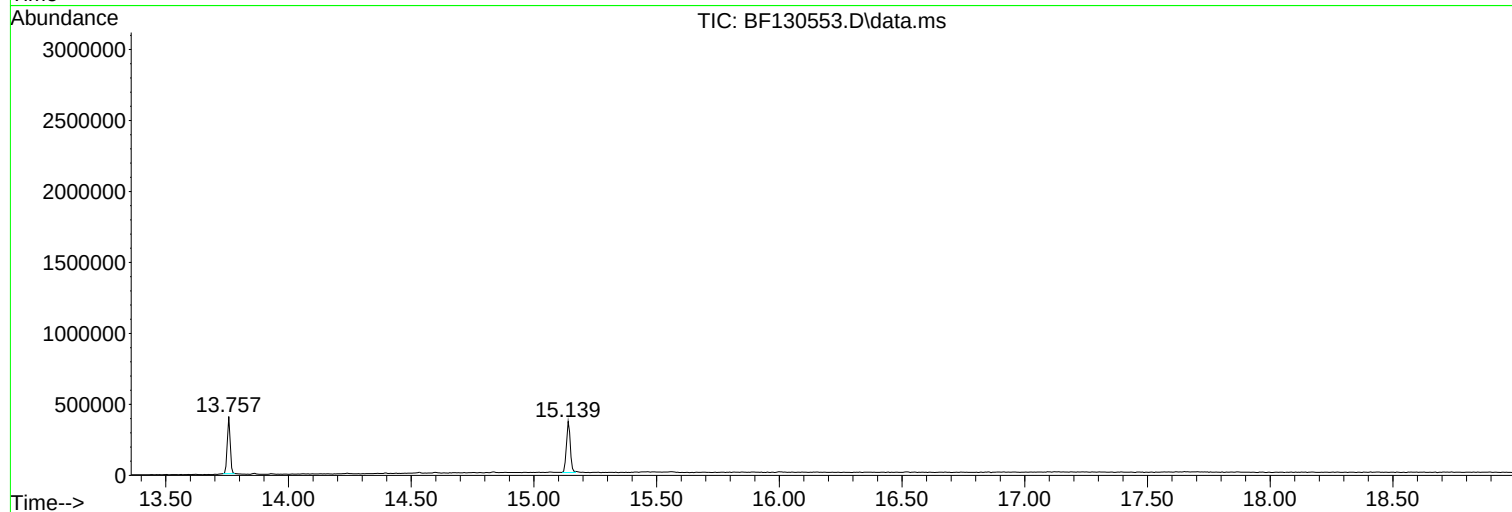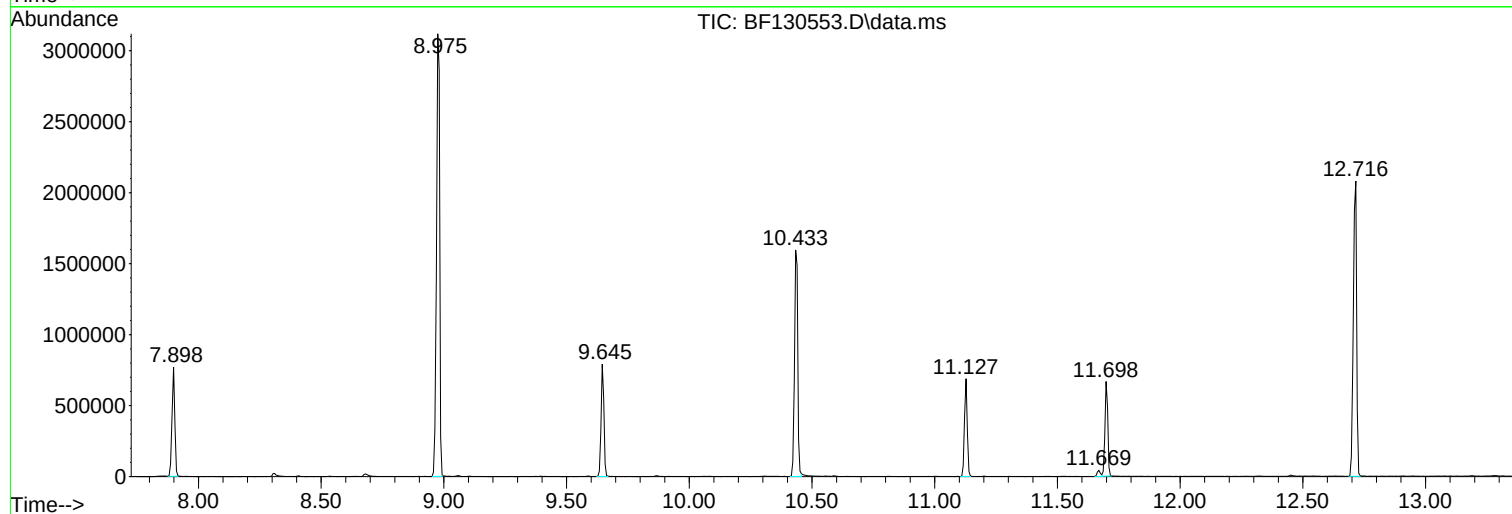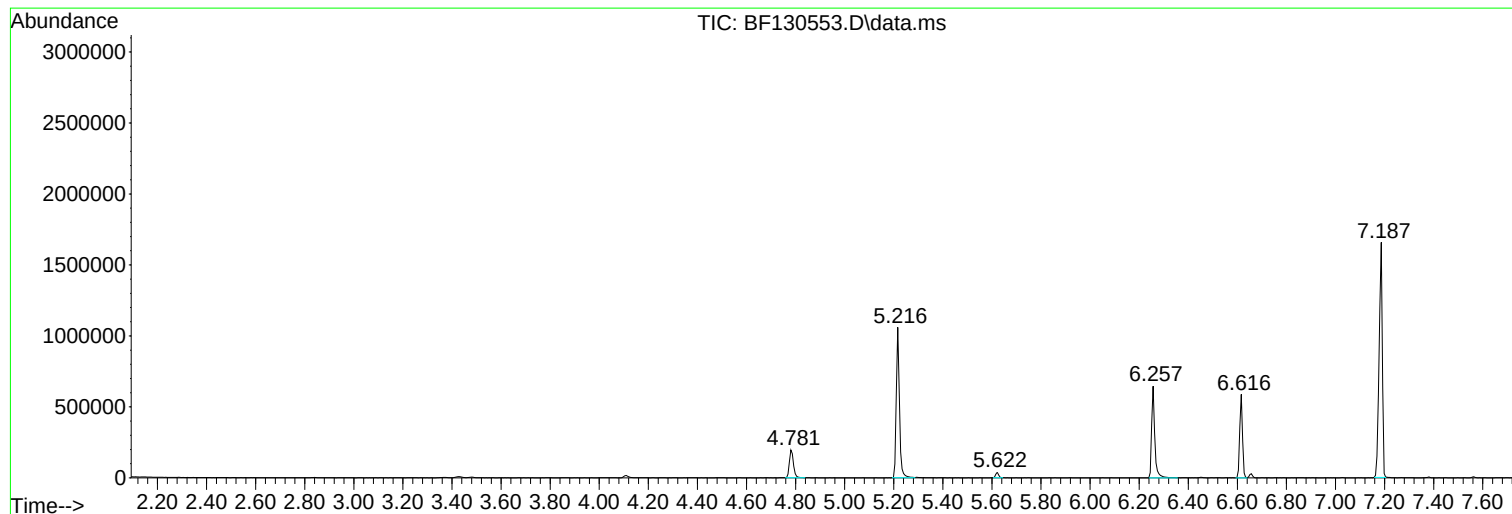

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130553.D
Acq On : 06 Oct 2022 16:27
Operator : CG\JU
Sample : N4998-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
506D-2









Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.781	9.86 ng	225958	1,4-Dichlorobenzene-d4	6.616

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	53		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	Morpholine, 4-methyl-	101	C5H11NO	000109-02-4	9		

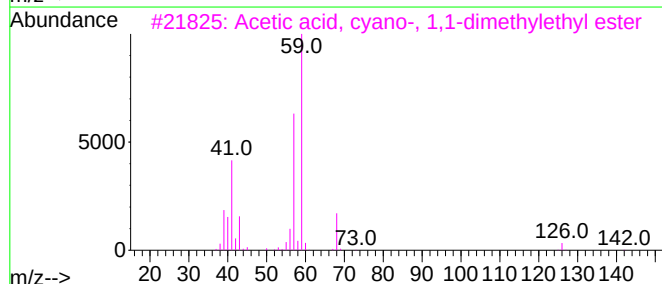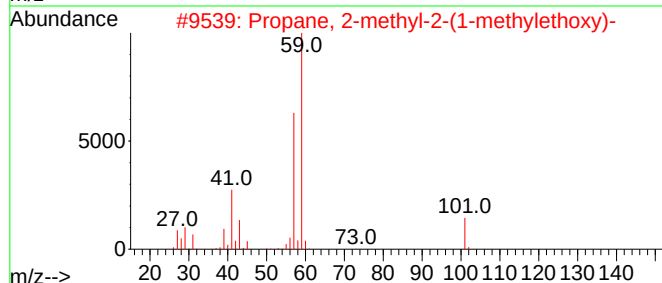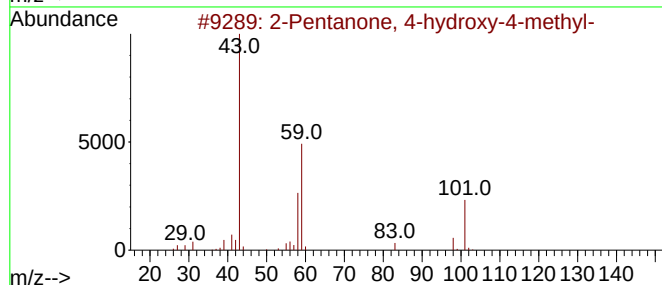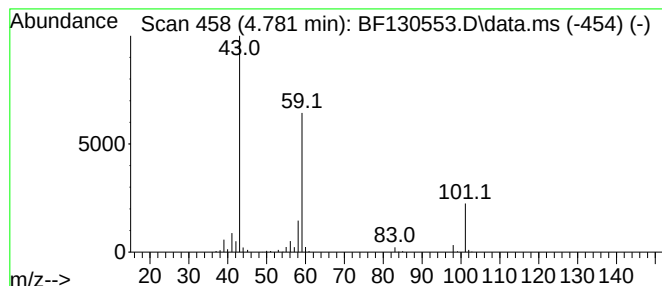

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130553.D
Acq On : 06 Oct 2022 16:27
Operator : CG\JU
Sample : N4998-01
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
506D-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.781	9.9	ng	225958	1	6.616	458406	20.0