

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
 Data File : BF130555.D
 Acq On : 06 Oct 2022 17:34
 Operator : CG\JU
 Sample : N5014-13
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-01-0-2.0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130555.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.787	455	459	476	rVB	326087	423651	24.62%	3.853%
2	5.222	529	533	555	rBV	1508303	1492792	86.75%	13.577%
3	5.622	598	601	606	rVB	28037	24441	1.42%	0.222%
4	6.263	705	710	728	rBV	1586991	1482728	86.16%	13.486%
5	6.616	767	770	774	rBV	597481	455370	26.46%	4.142%
6	7.181	862	866	870	rBV	1026559	973718	56.58%	8.856%
7	7.898	984	988	991	rBV	755131	590123	34.29%	5.367%
8	8.975	1167	1171	1174	rBV	2243980	1720844	100.00%	15.651%
9	9.645	1282	1285	1289	rBV	776918	613828	35.67%	5.583%
10	10.433	1415	1419	1427	rBV	1042154	826695	48.04%	7.519%
11	11.127	1533	1537	1540	rBV	632410	521594	30.31%	4.744%
12	12.710	1802	1806	1810	rBV	1299973	1044685	60.71%	9.502%
13	13.757	1980	1984	1987	rBV	413975	365289	21.23%	3.322%
14	14.757	2151	2154	2157	rBV	18387	22432	1.30%	0.204%
15	15.139	2214	2219	2223	rBV	397106	436635	25.37%	3.971%




Sum of corrected areas: 10994825

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130555.D
Acq On : 06 Oct 2022 17:34
Operator : CG\JU
Sample : N5014-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-01-0-2.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

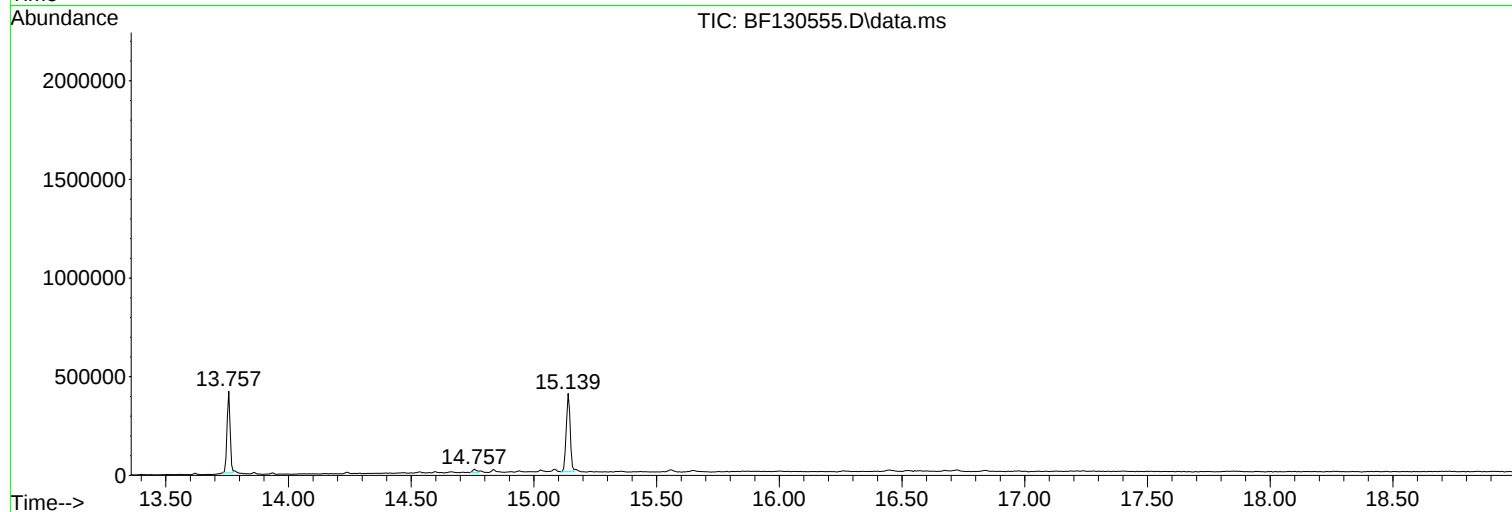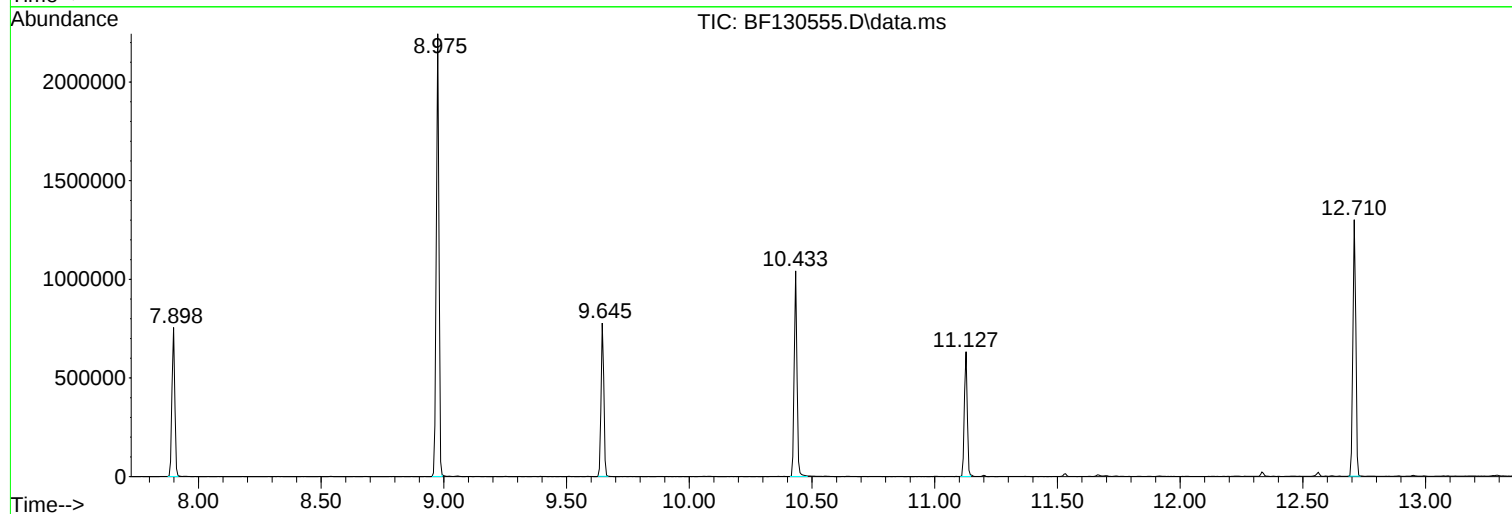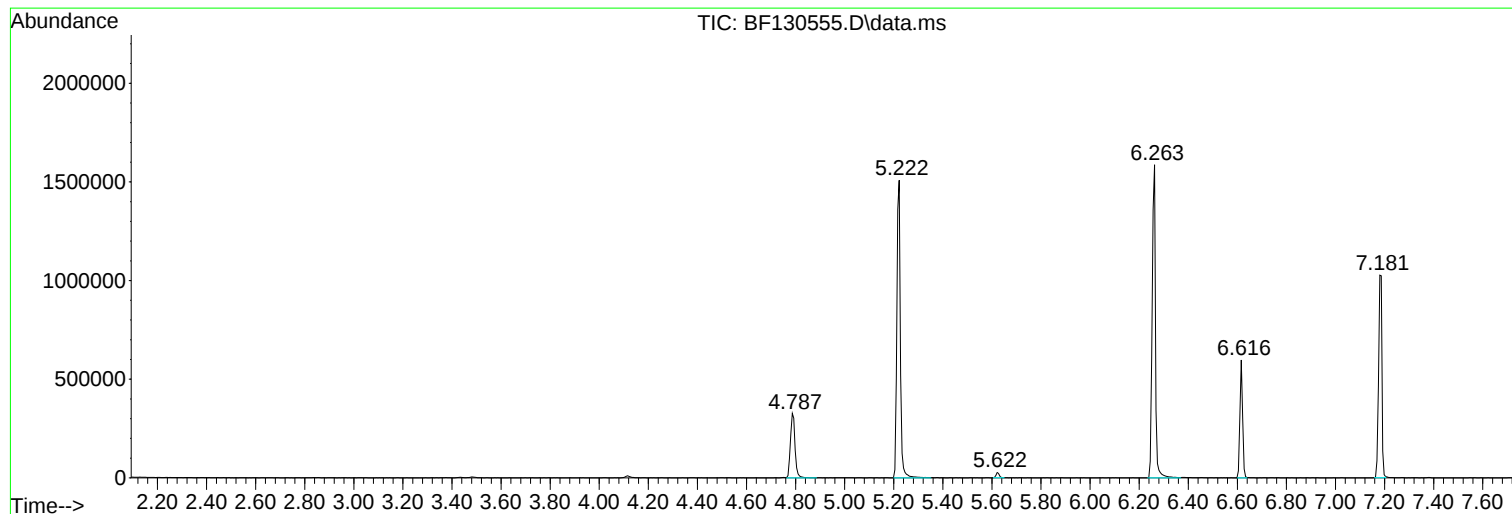

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130555.D
Acq On : 06 Oct 2022 17:34
Operator : CG\JU
Sample : N5014-13
Misc :
ALS Vial : 11 Sample Multiplier: 1









Instrument :
BNA_F
ClientSampleId :
SB-01-0-2.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
4.787	18.61 ng	423651	1,4-Dichlorobenzene-d4	6.616	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	72
2	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9

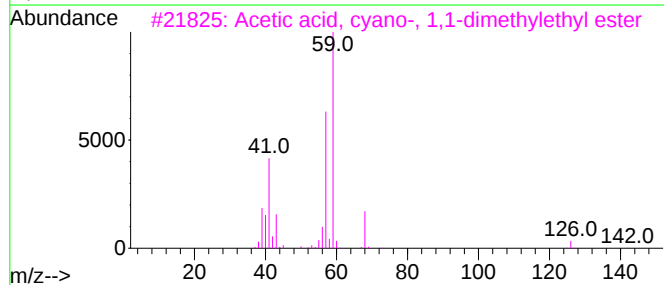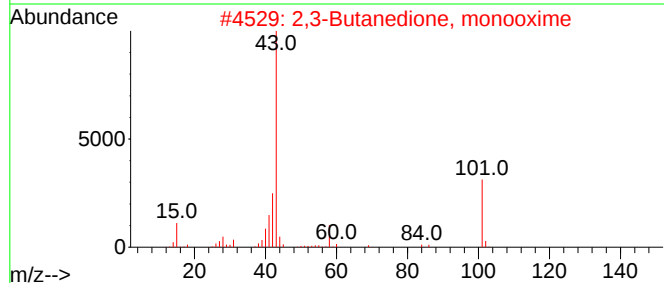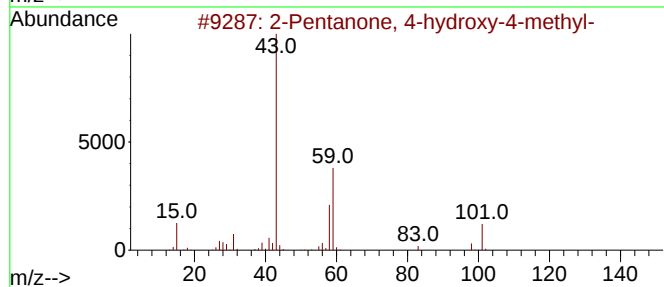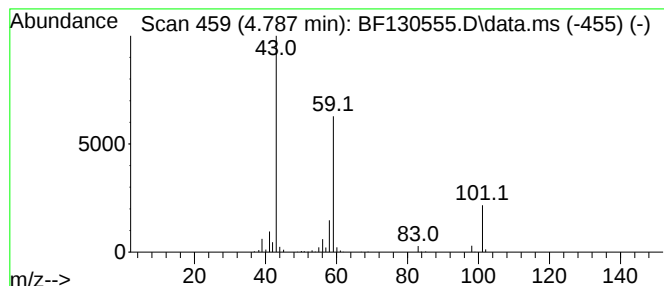

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130555.D
Acq On : 06 Oct 2022 17:34
Operator : CG\JU
Sample : N5014-13
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-01-0-2.0

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.787	18.6	ng	423651	1	6.616	455370	20.0