


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
 Data File : BF130545.D
 Acq On : 06 Oct 2022 11:45
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 07 02:06:46 2022

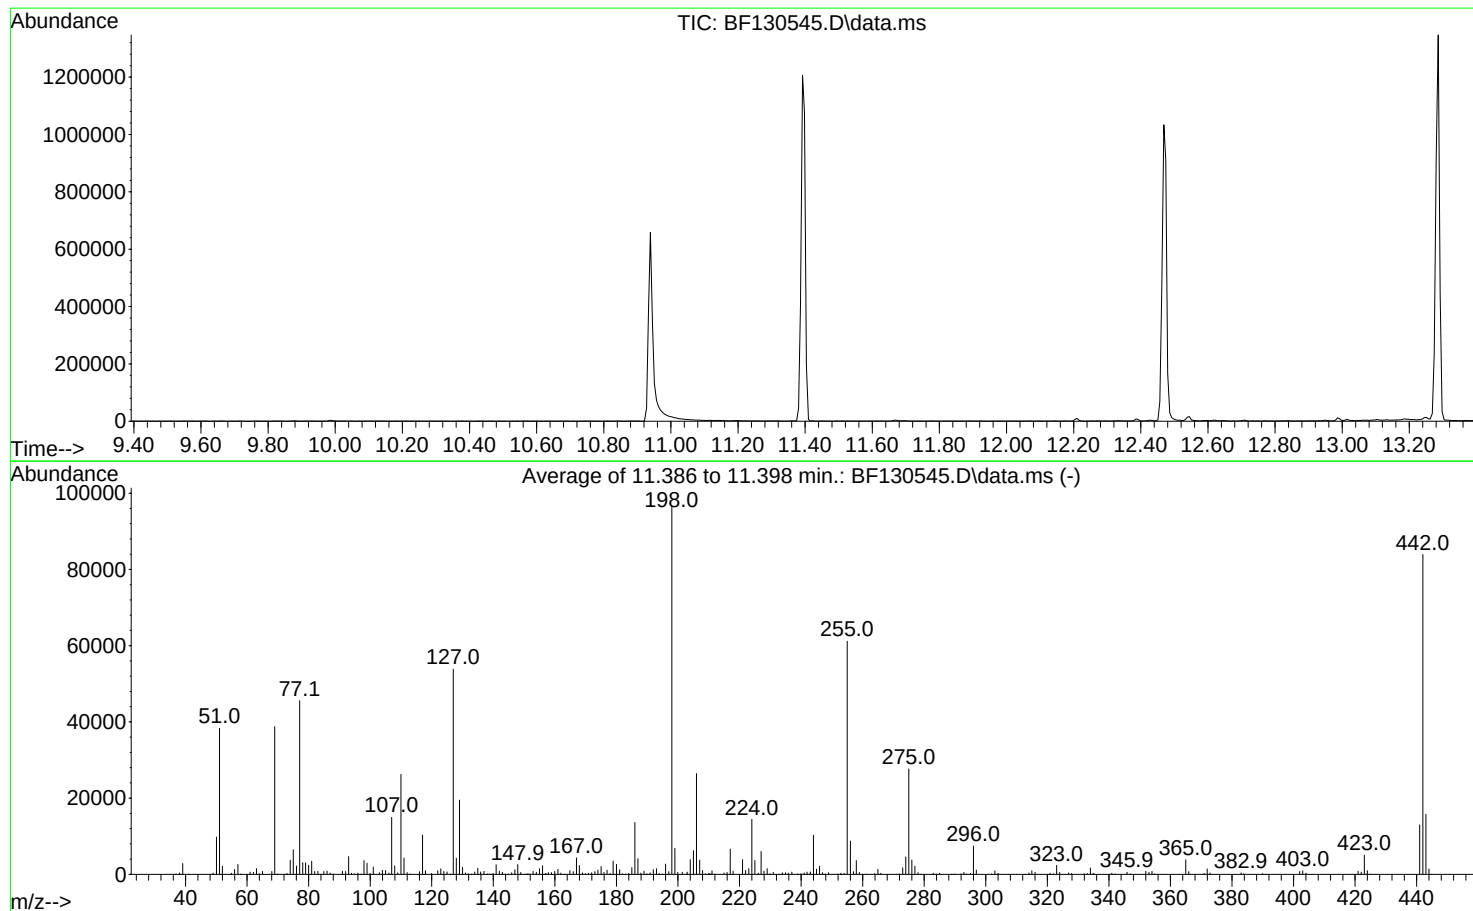




AutoFind: Scans 1581, 1582, 1583; Background Corrected with Scan 1577

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.7	38309	PASS
68	69	0.00	2	1.9	748	PASS
69	198	0.00	100	40.1	38736	PASS
70	69	0.00	2	0.4	144	PASS
127	198	10	80	55.8	53813	PASS
197	198	0.00	2	0.8	735	PASS
198	198	100	100	100.0	96512	PASS
199	198	5	9	7.1	6845	PASS
275	198	10	60	28.7	27654	PASS
365	198	1	100	3.9	3808	PASS
441	198	0.01	100	13.4	12954	PASS
442	442	50	100	100.0	83899	PASS
443	442	15	24	18.8	15779	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130545.D
Acq On : 06 Oct 2022 11:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 07 05:20:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 07 02:06:46 2022
Response via : Initial Calibration

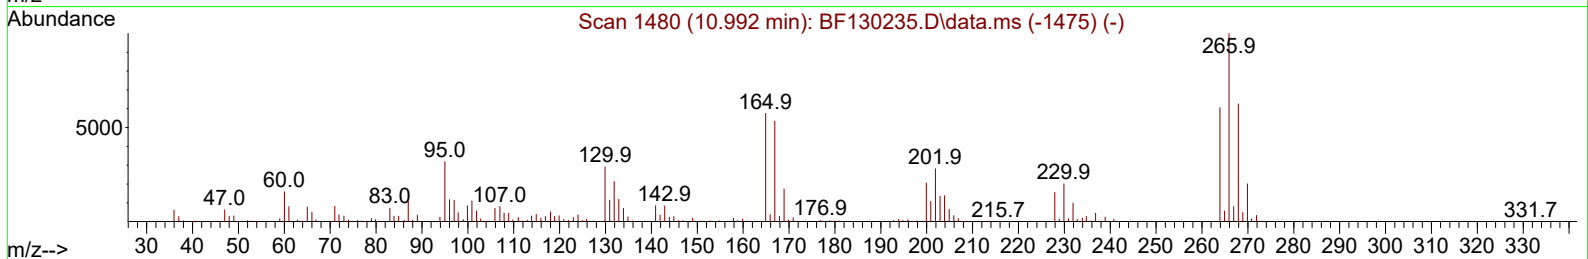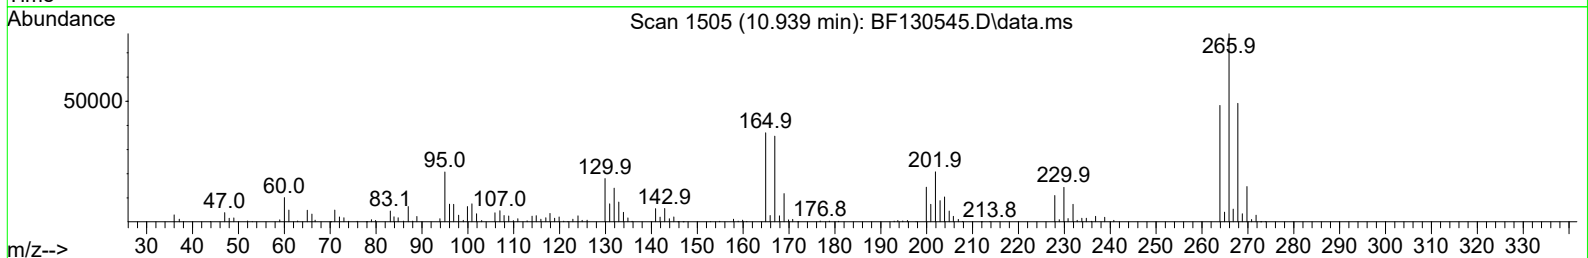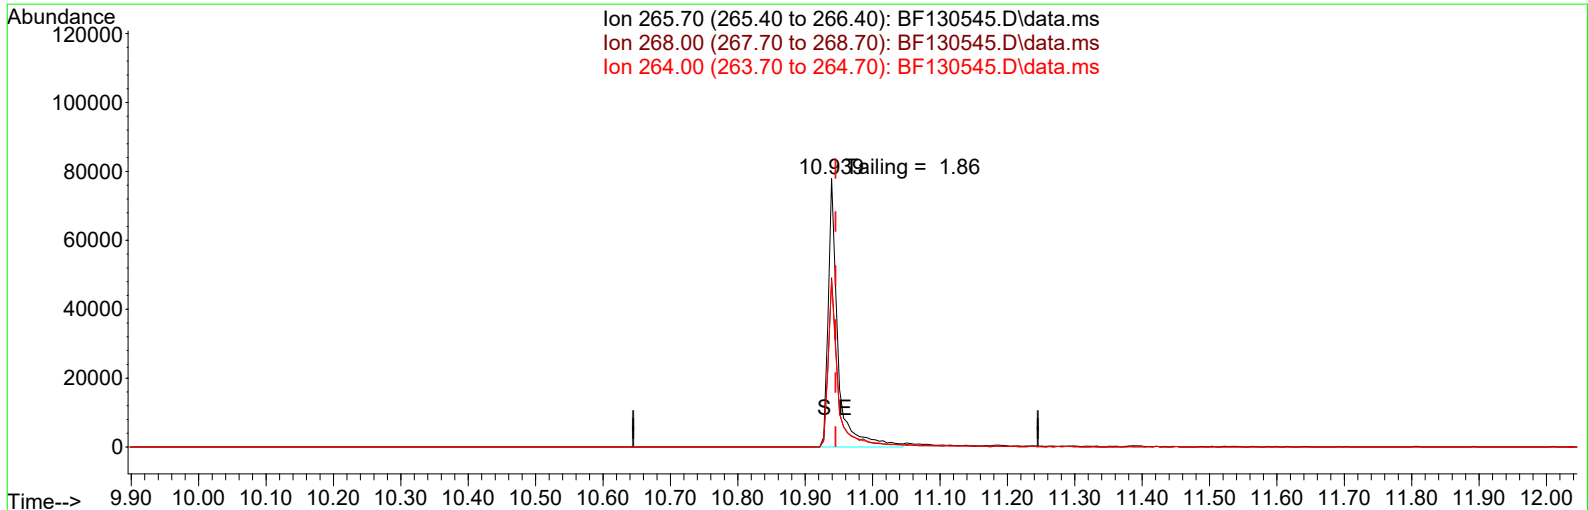

TIC: BF130545.D\data.ms

(70) Pentachlorophenol (C)

10.939min (-0.006) 31233.59 ng




response 79236

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.04
264.00	63.10	61.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100622\
Data File : BF130545.D
Acq On : 06 Oct 2022 11:45
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 07 05:20:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 07 02:06:46 2022
Response via : Initial Calibration

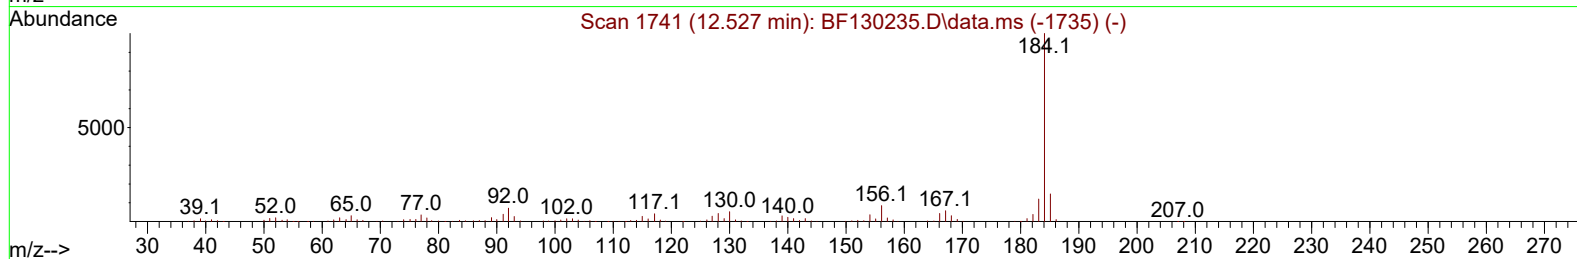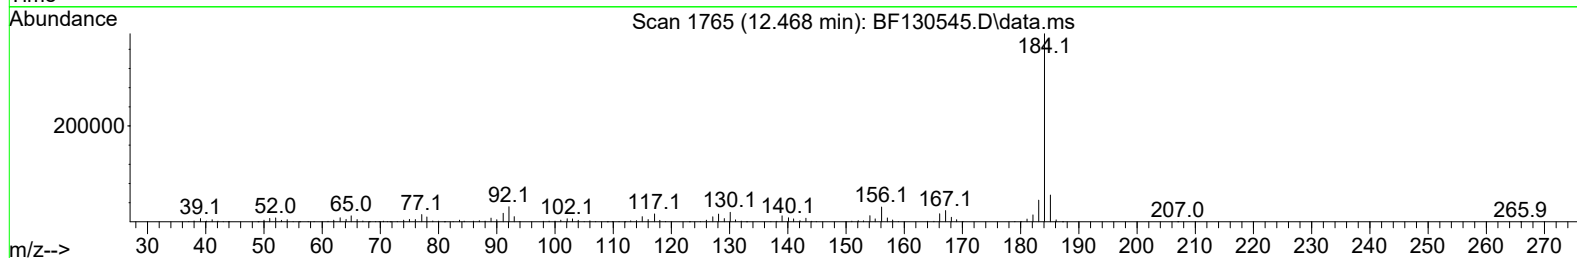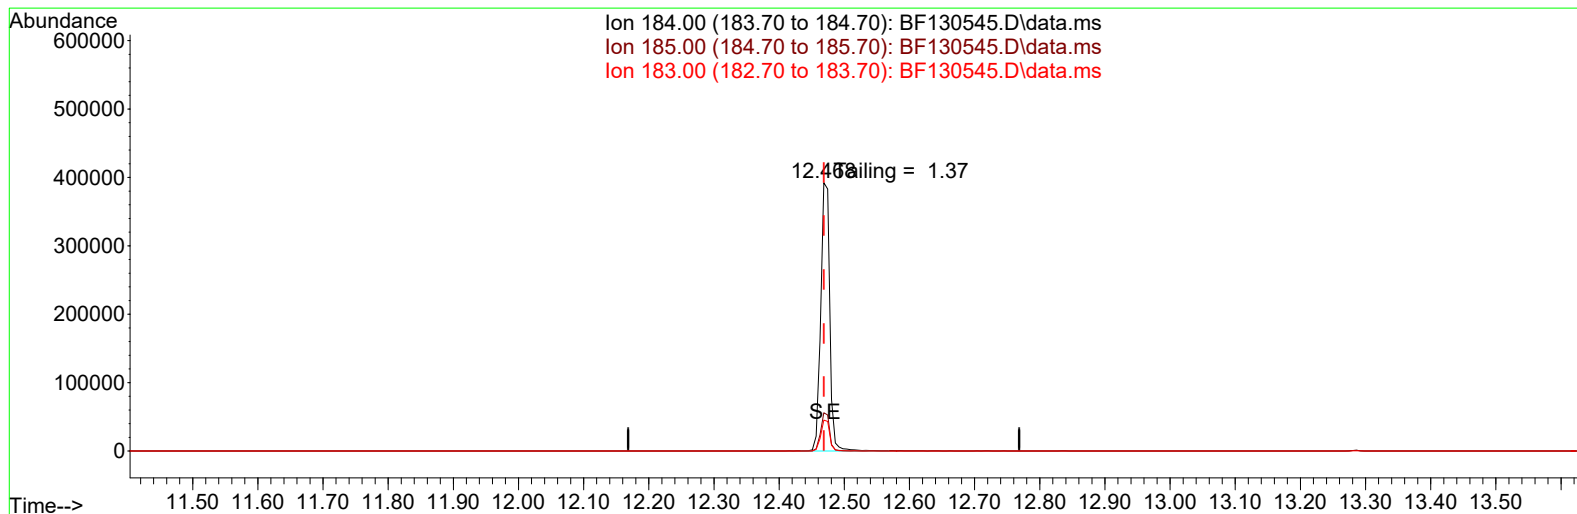

TIC: BF130545.D\data.ms

(77) Benzidine

12.468min (-0.000) 0.00 ng

response 379647

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.29
183.00	11.40	11.50
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/6/2022	BNA_F	<u>BF130545.D</u>
Compound Name	Response	Retention Time
DDT	197143	13.286
DDD	3141	12.986
DDE	139	12.657
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3280	200423	1.64

Instrument :
BNA_F
ClientSampleId :
DFTPP