


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100920\
 Data File : BF121900.D
 Acq On : 9 Oct 2020 10:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091020.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 01 14:29:14 2020

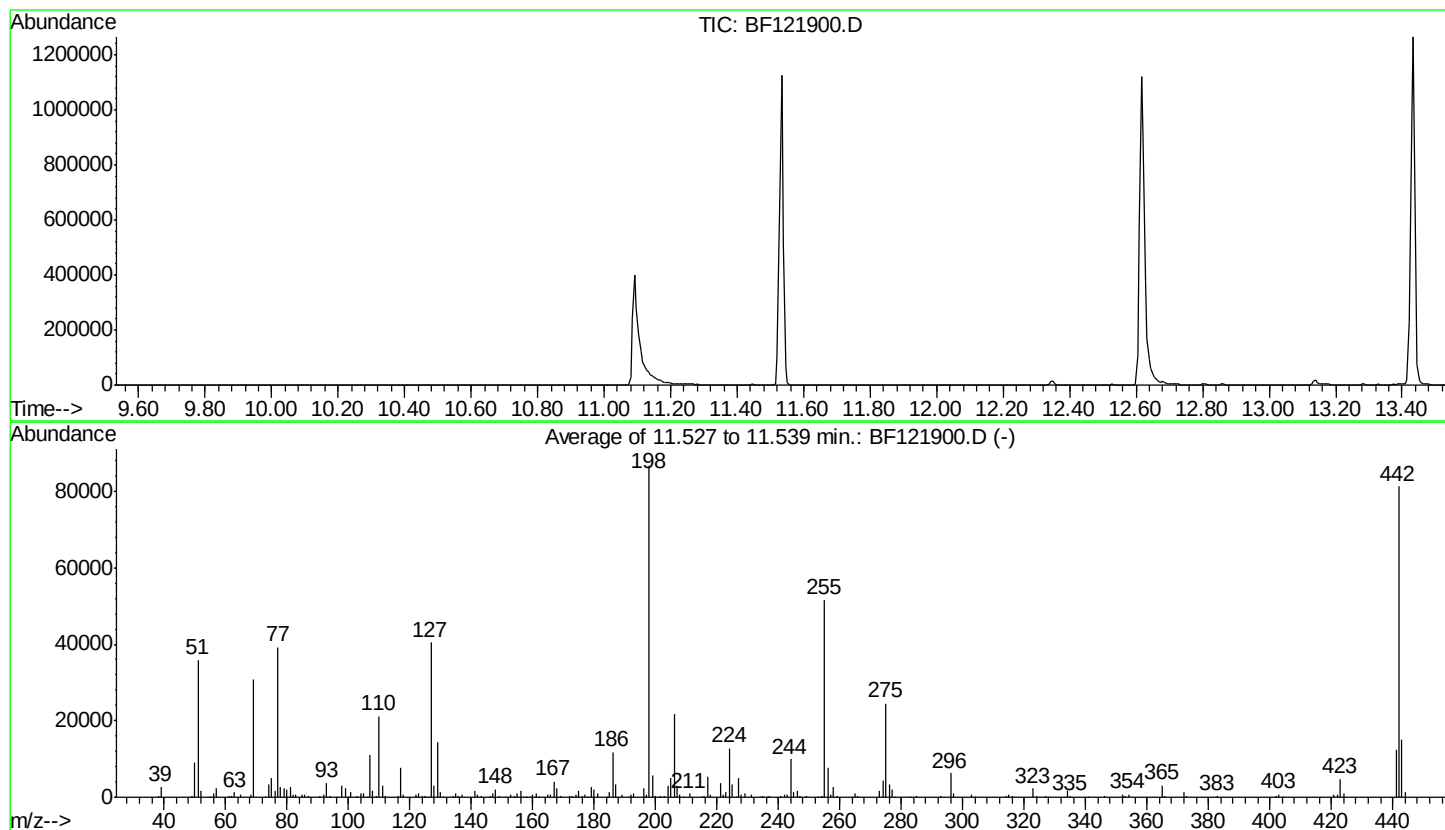

AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.4	35896	PASS
68	69	0.00	2	1.7	530	PASS
69	198	0.00	100	35.6	30876	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.6	40368	PASS
197	198	0.00	2	0.8	728	PASS
198	198	100	100	100.0	86690	PASS
199	198	5	9	6.5	5646	PASS
275	198	10	60	28.2	24440	PASS
365	198	1	100	3.6	3151	PASS
441	198	0.01	100	14.5	12533	PASS
442	198	50	100	93.7	81218	PASS
443	442	15	24	18.6	15114	PASS