

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102022\
 Data File : BF130736.D
 Acq On : 20 Oct 2022 20:17
 Operator : CG\JU
 Sample : PB148413BL
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB148413BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130736.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.757	484	488	507	rBV	138376	246765	7.02%	1.289%
2	5.175	556	559	578	rBV	2220030	2516338	71.55%	13.147%
3	6.222	733	737	766	rBV	2177514	2445594	69.53%	12.777%
4	6.563	792	795	809	rBV	543740	513283	14.59%	2.682%
5	7.134	888	892	910	rBV	1536745	1655331	47.07%	8.649%
6	7.845	1009	1013	1032	rBV	651606	680248	19.34%	3.554%
7	8.922	1191	1196	1199	rBV	3108387	2882501	81.96%	15.060%
8	9.592	1306	1310	1324	rVB	728673	699795	19.90%	3.656%
9	10.380	1440	1444	1471	rBV	1975612	1938243	55.11%	10.127%
10	11.069	1558	1561	1579	rBV	902372	763846	21.72%	3.991%
11	12.657	1826	1831	1834	rBV	3889556	3517104	100.00%	18.376%
12	13.704	2005	2009	2025	rVB	650390	670625	19.07%	3.504%
13	15.074	2239	2242	2260	rVB	398851	572671	16.28%	2.992%
14	15.880	2374	2379	2390	rVB3	20923	37708	1.07%	0.197%




Sum of corrected areas: 19140052

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102022\
Data File : BF130736.D
Acq On : 20 Oct 2022 20:17
Operator : CG\JU
Sample : PB148413BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148413BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

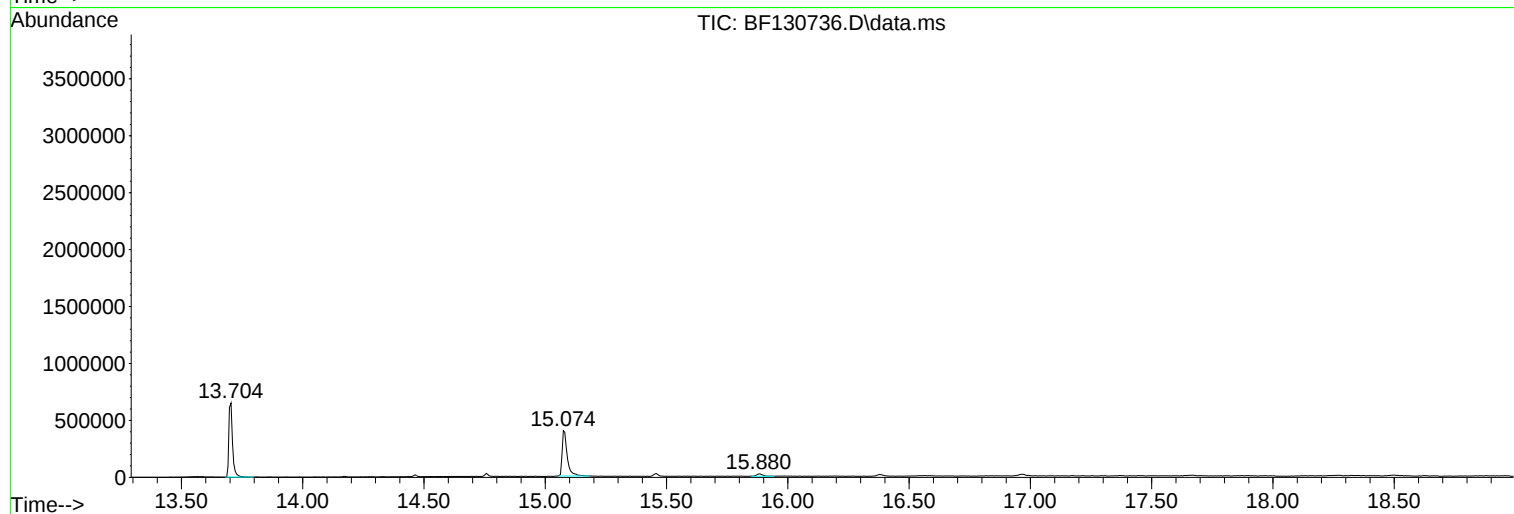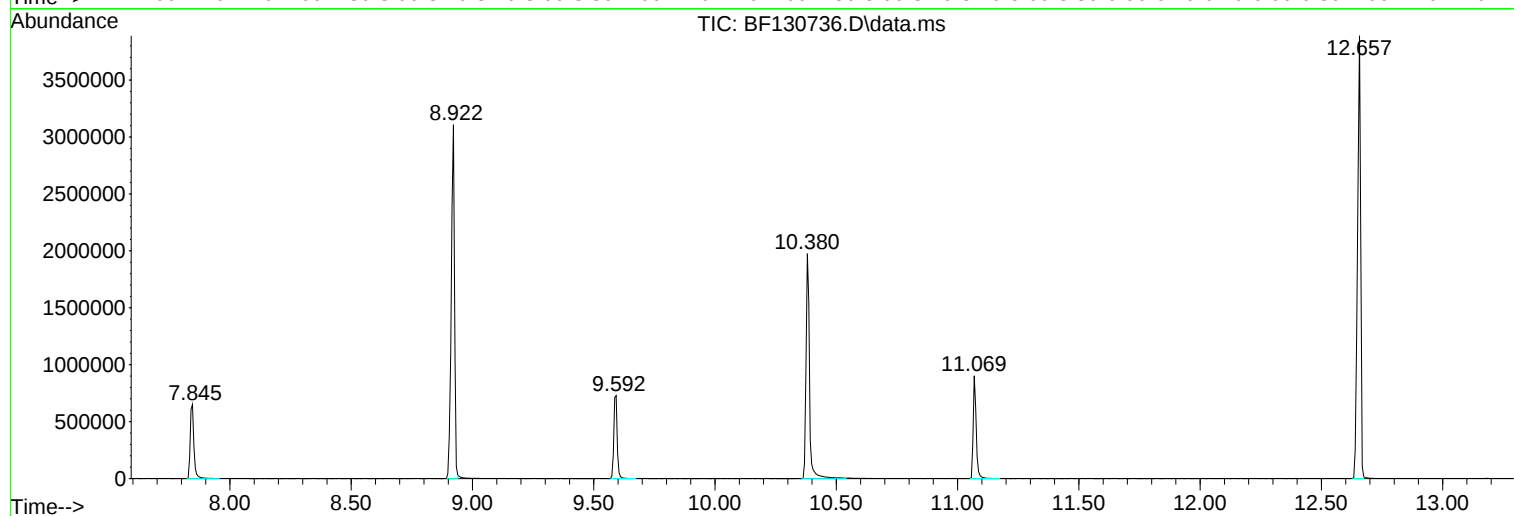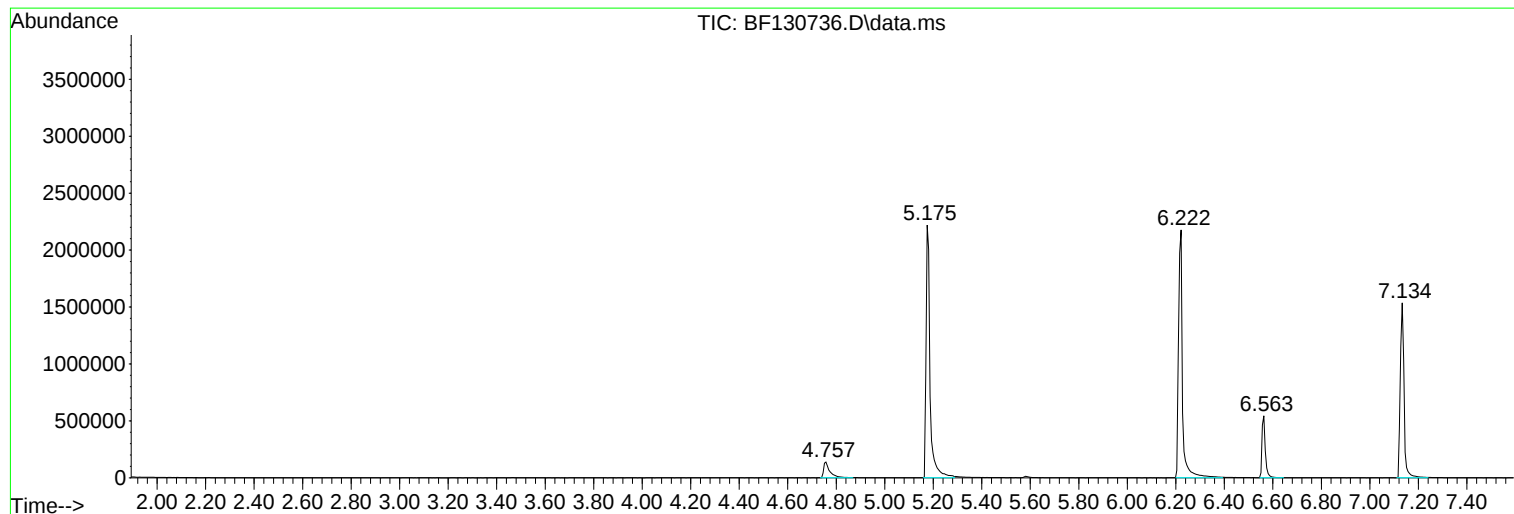

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102022\
Data File : BF130736.D
Acq On : 20 Oct 2022 20:17
Operator : CG\JU
Sample : PB148413BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148413BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.757	9.62 ng	246765	1,4-Dichlorobenzene-d4	6.563

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	(+)-4-Amino-4,5-dihydro-2(3H)-f...	101	C4H7NO2	016504-58-8	9		
5	Butane, 1-ethoxy-	102	C6H14O	000628-81-9	9		

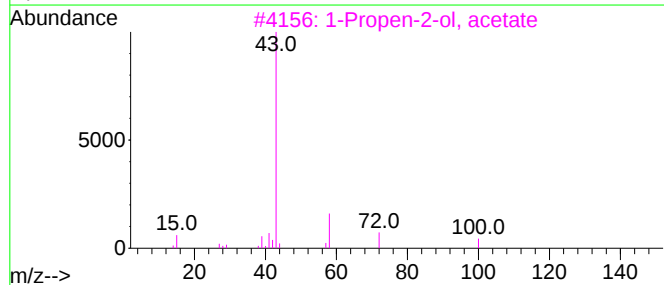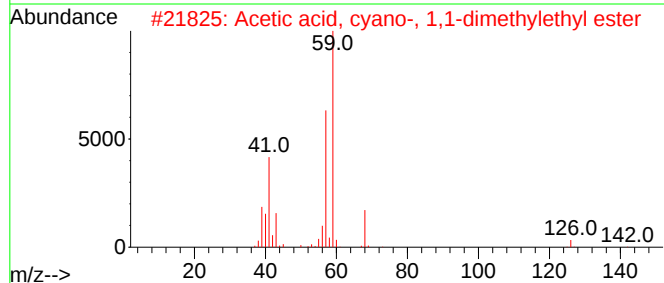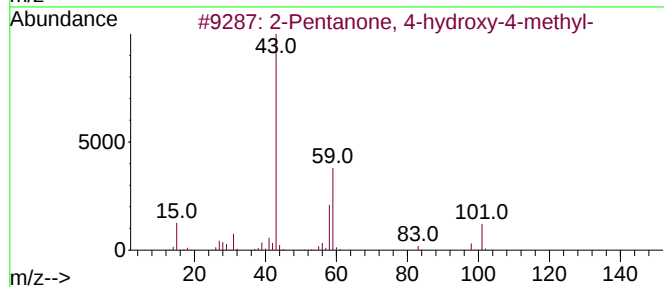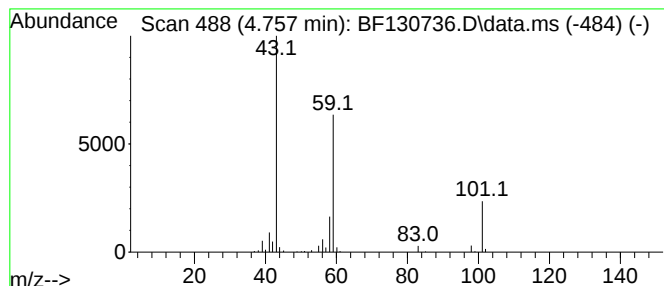

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102022\
Data File : BF130736.D
Acq On : 20 Oct 2022 20:17
Operator : CG\JU
Sample : PB148413BL
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148413BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.757	9.6	ng	246765	1	6.563	513283	20.0