


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102022\
 Data File : BF130724.D
 Acq On : 20 Oct 2022 10:46
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 21 06:12:36 2022

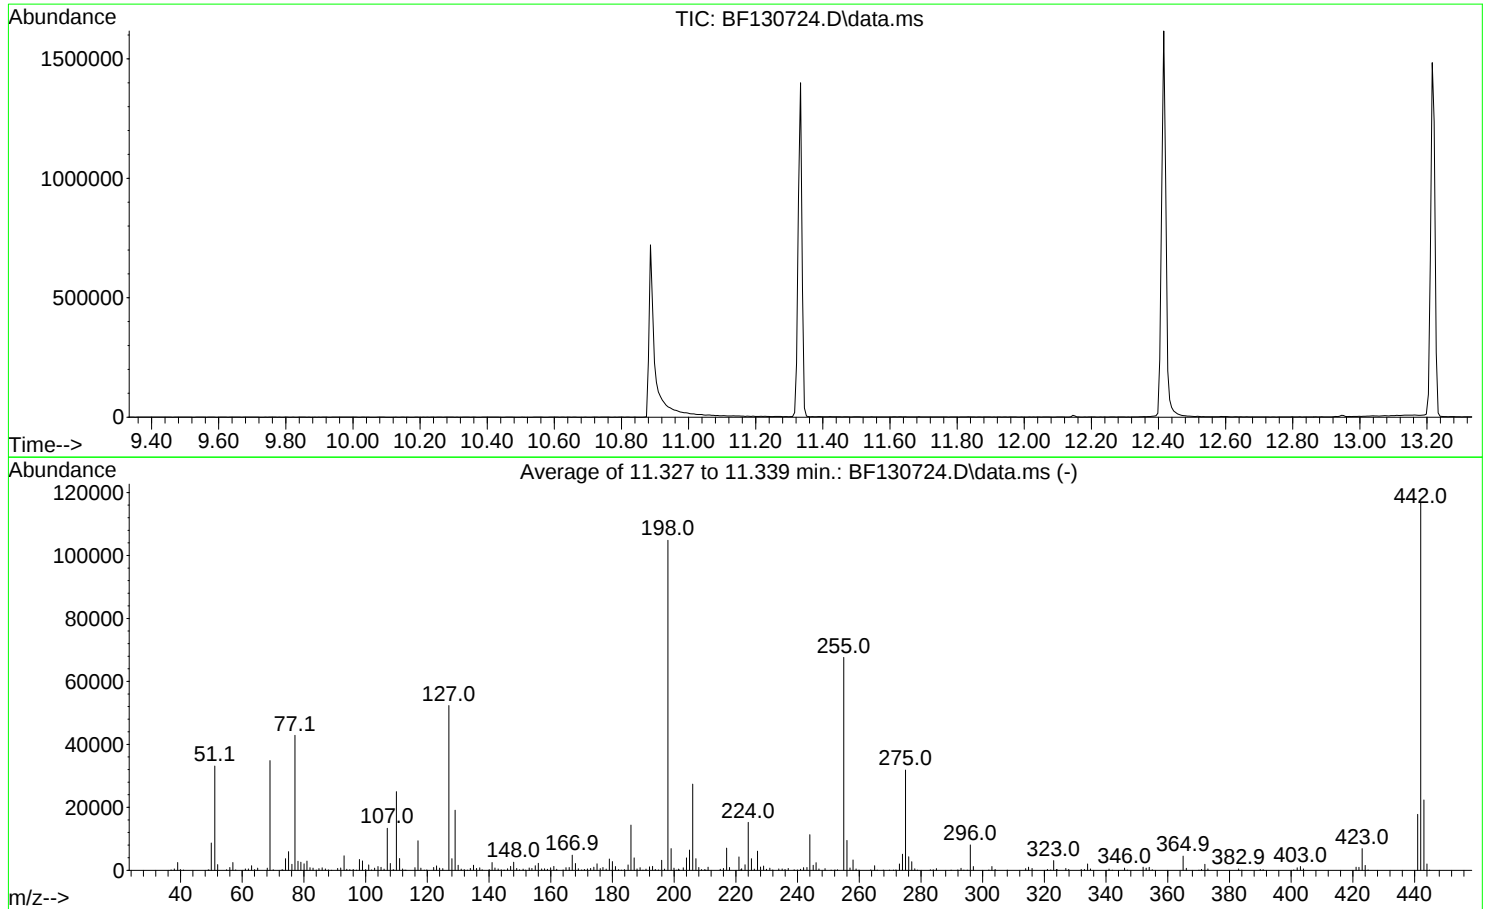




AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1600

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.6	33125	PASS
68	69	0.00	2	2.0	696	PASS
69	198	0.00	100	33.3	34859	PASS
70	69	0.00	2	0.6	198	PASS
127	198	10	80	49.9	52349	PASS
197	198	0.00	2	0.3	361	PASS
198	198	100	100	100.0	104816	PASS
199	198	5	9	6.6	6866	PASS
275	198	10	60	30.4	31848	PASS
365	198	1	100	4.3	4487	PASS
441	198	0.01	100	17.0	17768	PASS
442	442	50	100	100.0	116856	PASS
443	442	15	24	19.1	22316	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102022\  
Data File : BF130724.D  
Acq On    : 20 Oct 2022  10:46  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 21 09:22:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 06:12:36 2022
Response via : Initial Calibration

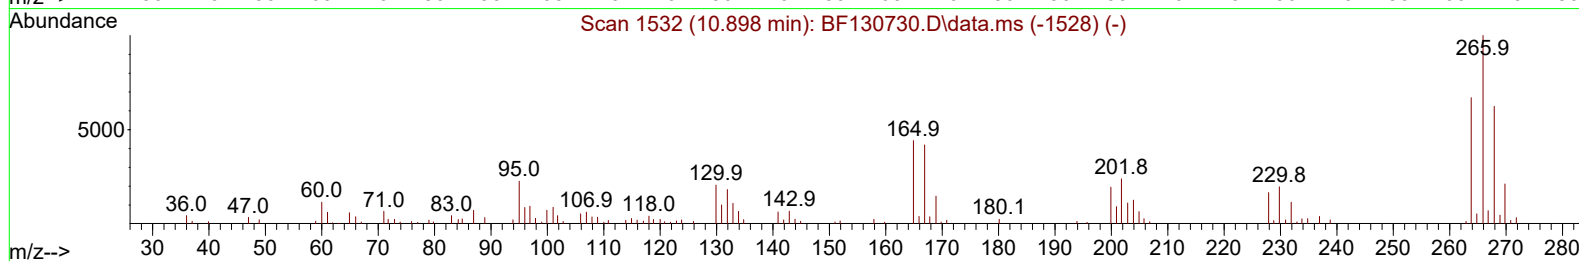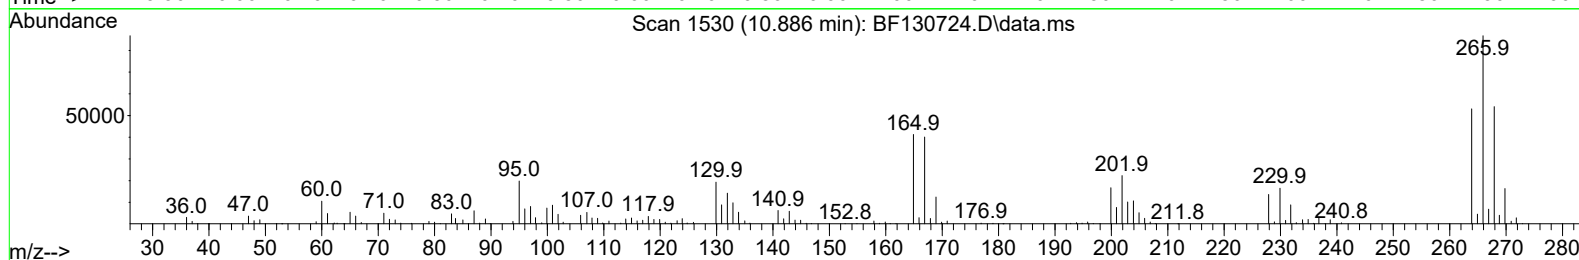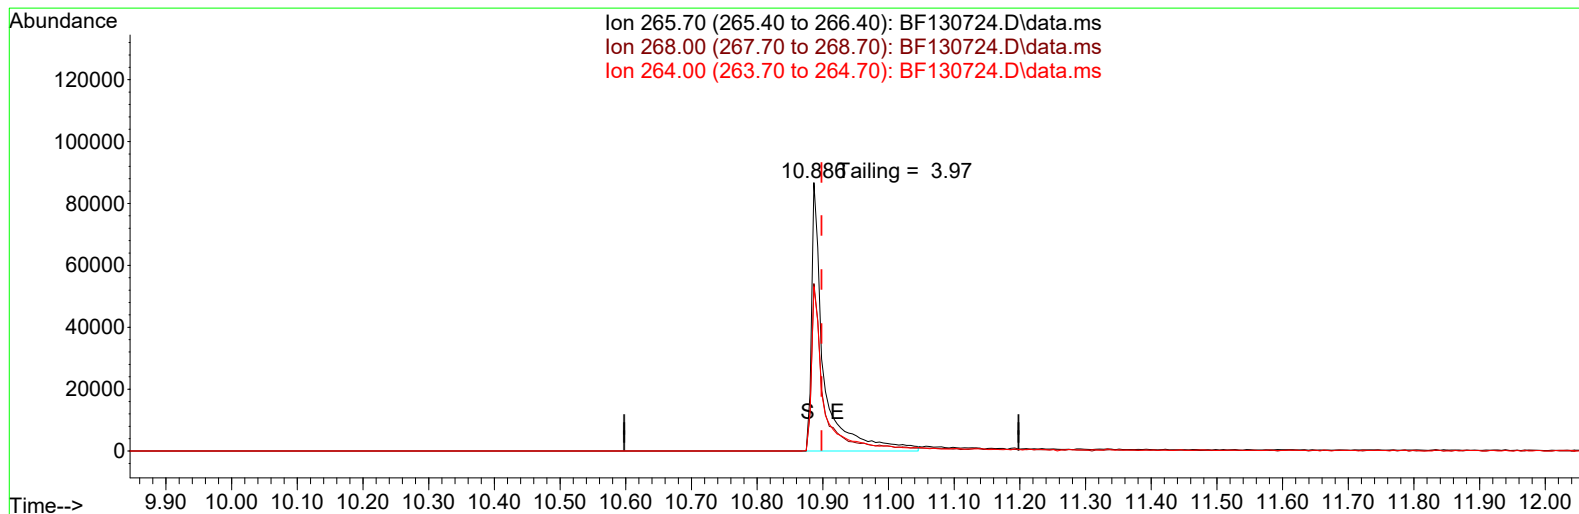

TIC: BF130724.D\data.ms

(70) Pentachlorophenol (C)

10.886min (-0.012) 4108.44 ng




response **114530**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.40	62.36
264.00	67.00	61.21
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102022\
Data File : BF130724.D
Acq On : 20 Oct 2022 10:46
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 21 09:22:45 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102022.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Oct 21 06:12:36 2022
Response via : Initial Calibration

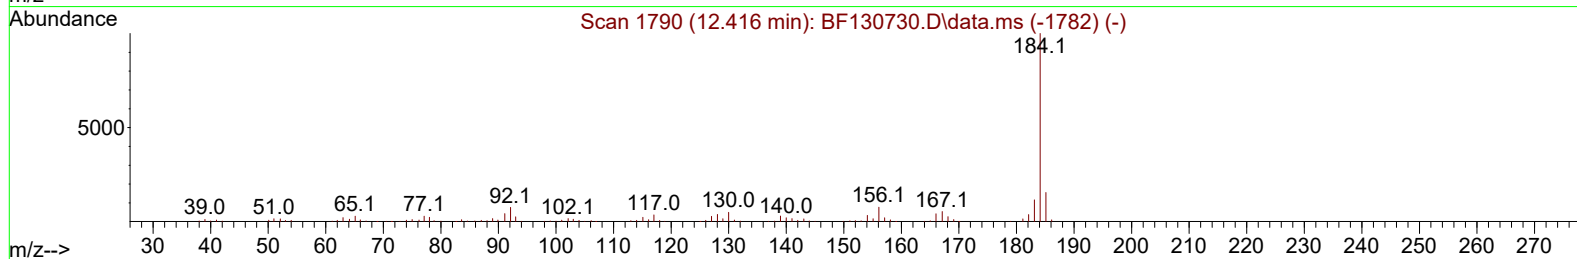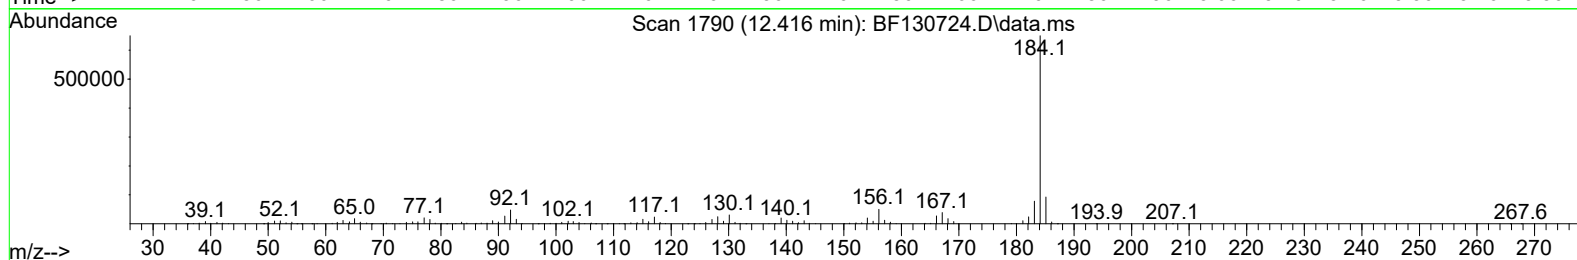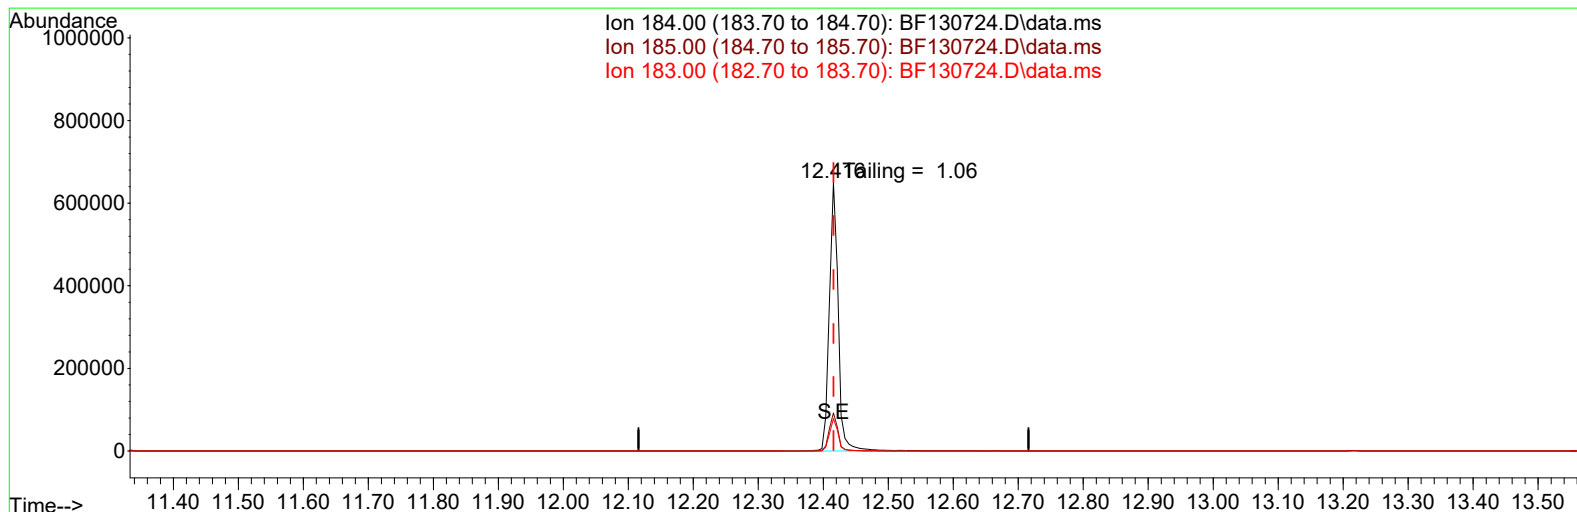

TIC: BF130724.D\data.ms

(77) Benzidine

12.416min (-0.000) 0.00 ng

response 619321

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.50	14.20
183.00	11.60	12.06
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/20/2022	BNA_F	<u>BF130724.D</u>
Compound Name	Response	Retention Time
DDT	262436	13.216
DDD	2614	12.945
DDE	738	12.592
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3352	265788	1.26

Instrument :
BNA_F
ClientSampleId :
DFTPP