
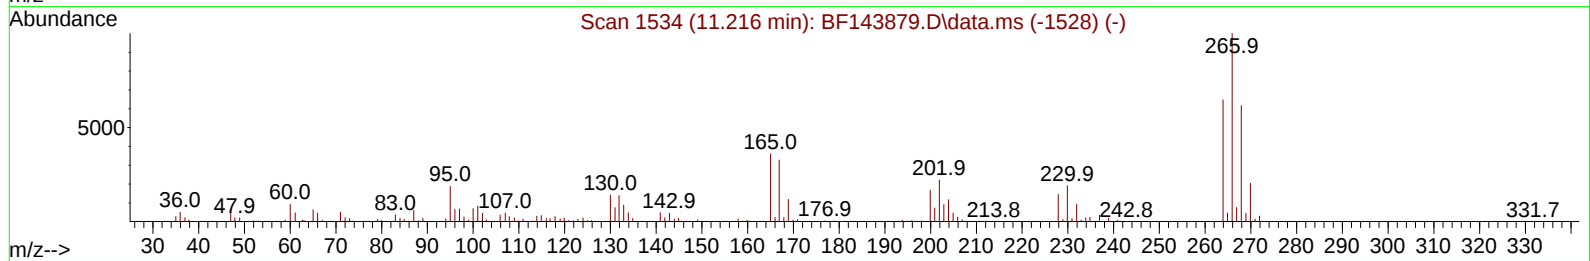
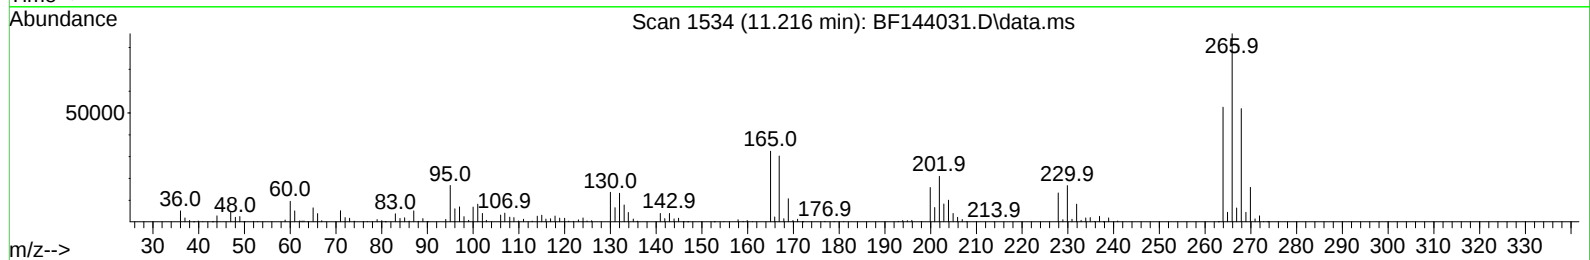


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102225\
Data File : BF144031.D
Acq On : 22 Oct 2025 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 12:25:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

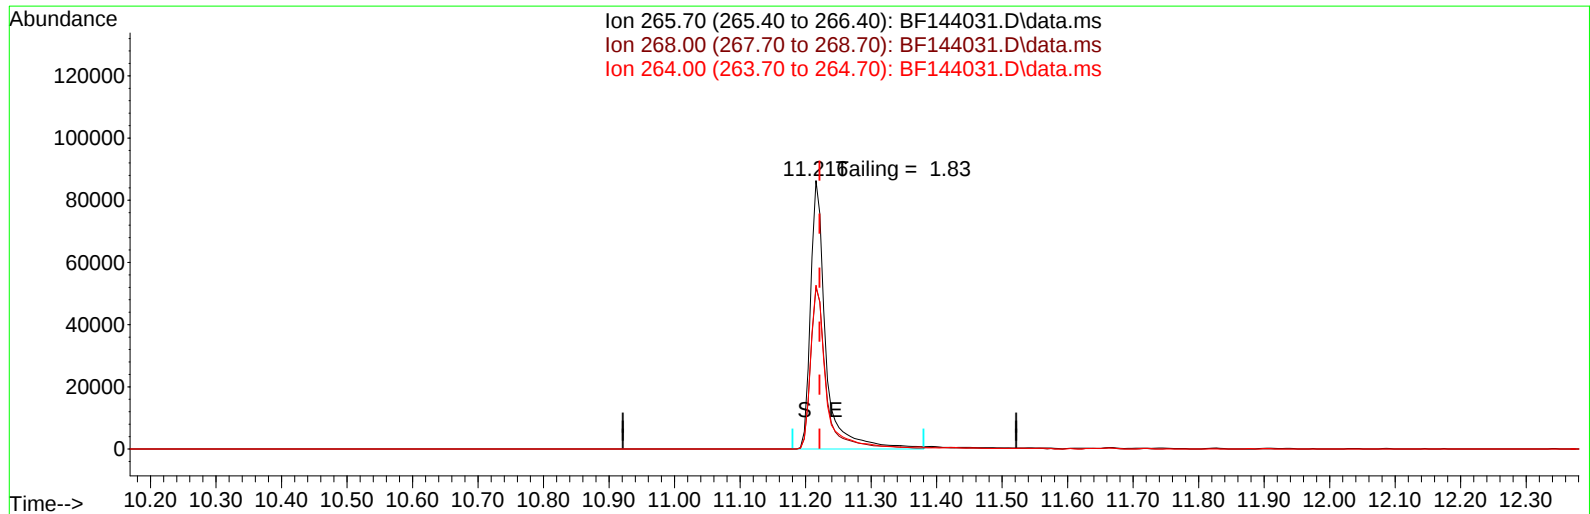

TIC: BF144031.D\data.ms

(70) Pentachlorophenol (C)




11.216min (-0.006) 25307.30 ng

response 139659

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	60.26
264.00	64.70	61.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102225\
Data File : BF144031.D
Acq On : 22 Oct 2025 09:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 22 12:25:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF100625.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

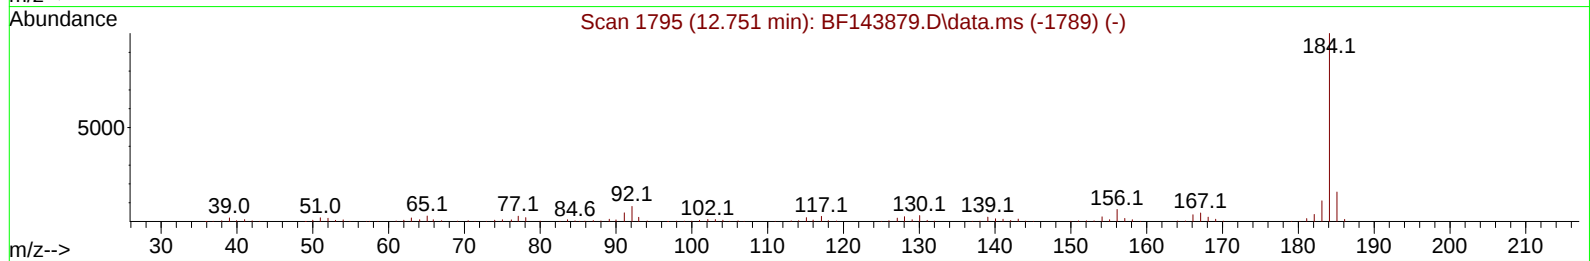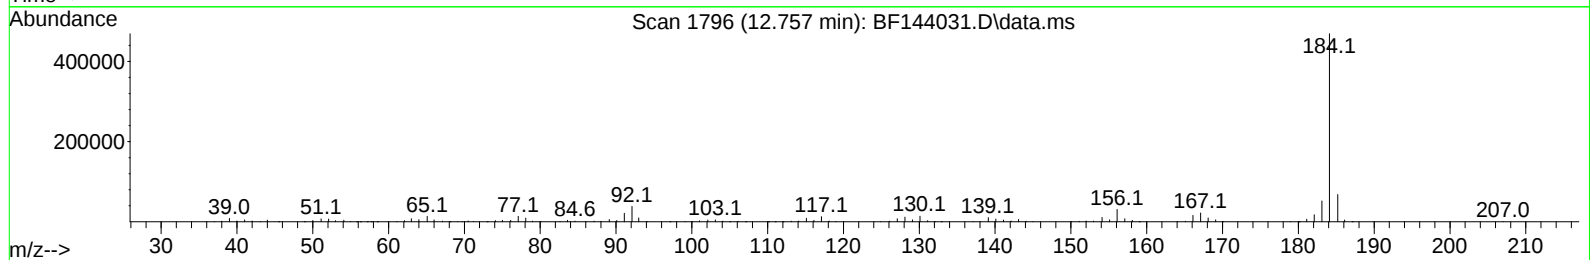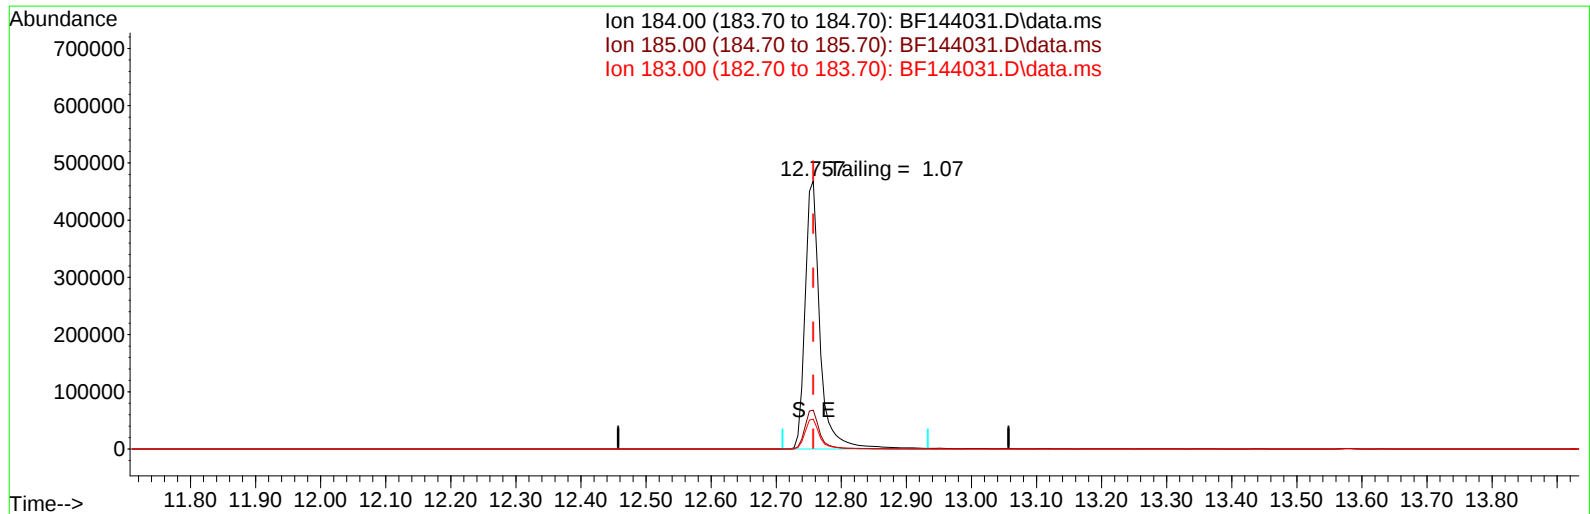

TIC: BF144031.D\data.ms

(77) Benzidine

12.757min (-0.000) 0.00 ng

response 749496

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.47
183.00	11.00	11.14
0.00	0.00	0.00