


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102425\
Data File : BF144055.D
Acq On : 24 Oct 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 10:43:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

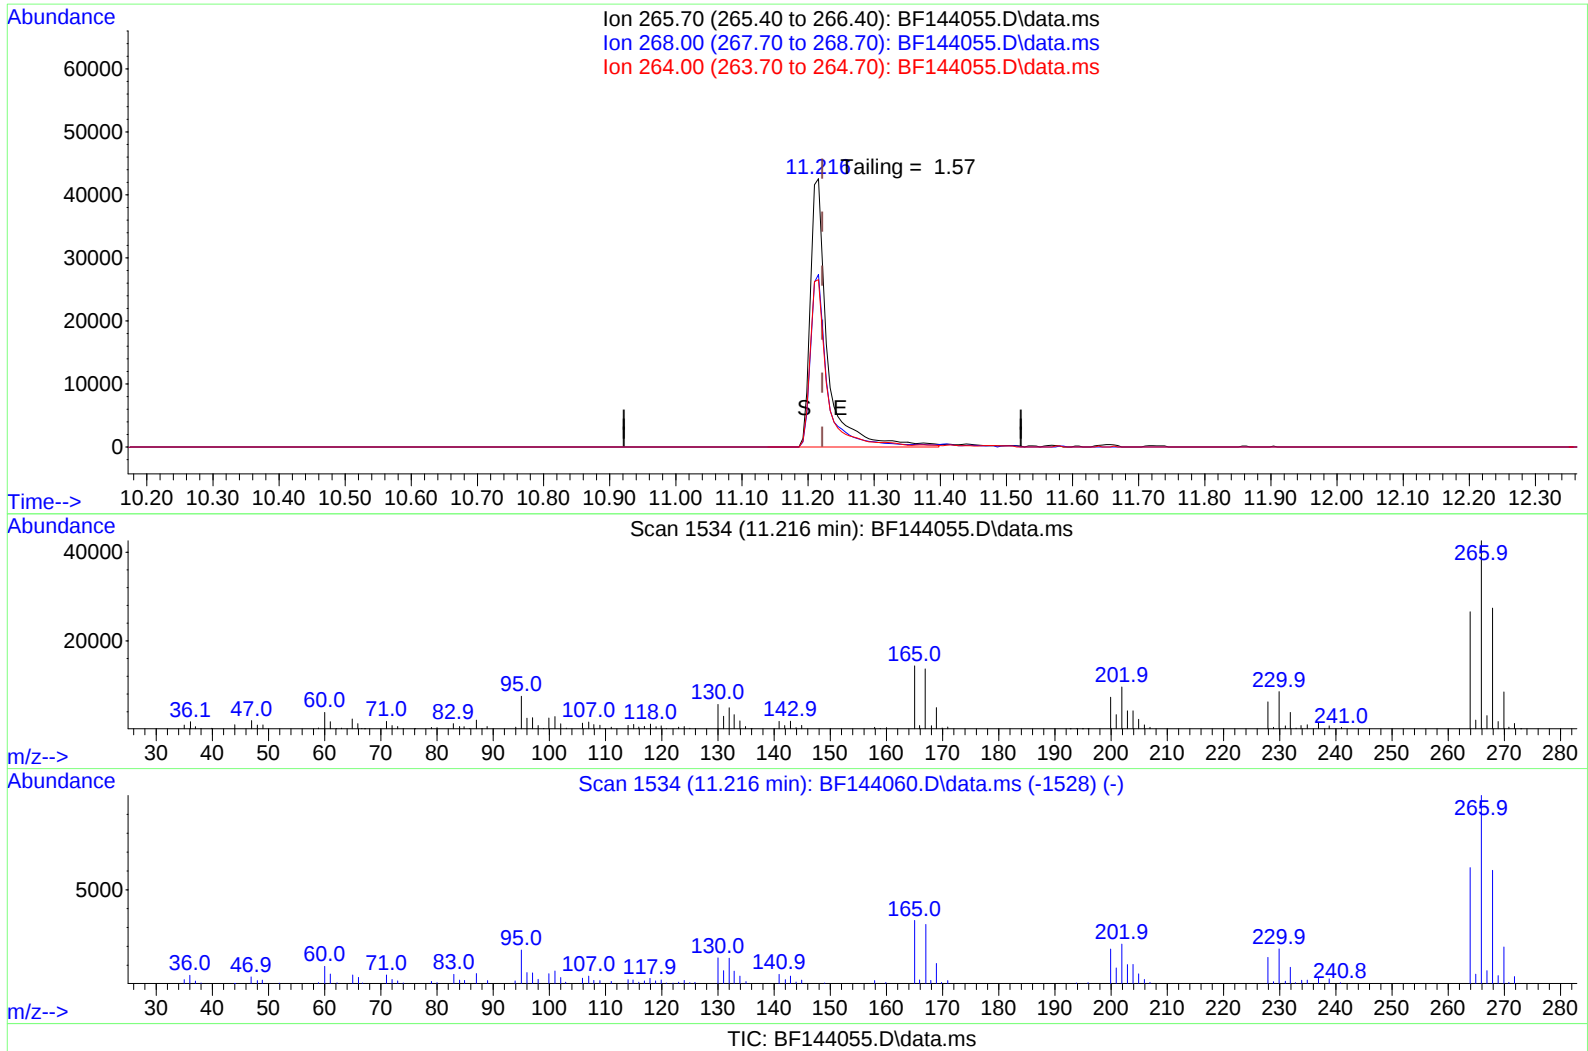

(70) Pentachlorophenol (C)




11.216min (-0.006) 43857.19 ng

response 76701

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.70	64.29
264.00	64.70	62.39
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102425\
Data File : BF144055.D
Acq On : 24 Oct 2025 09:45
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 24 10:43:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102425.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 06 15:29:47 2025
Response via : Initial Calibration

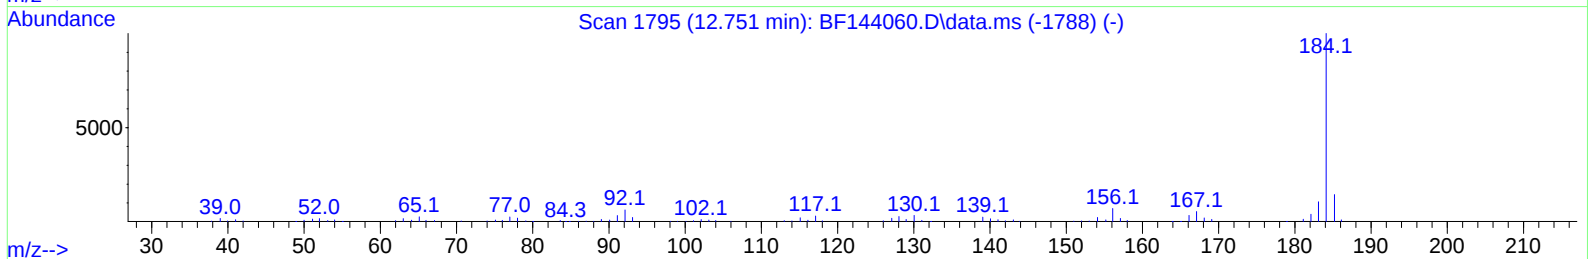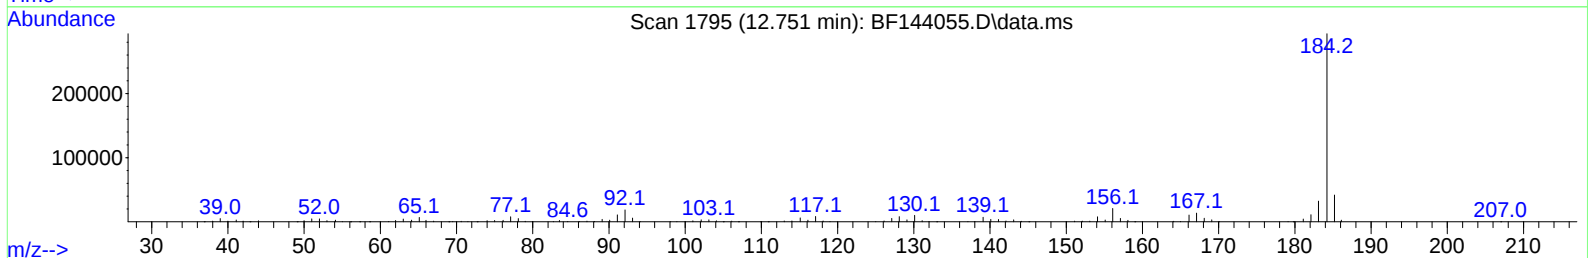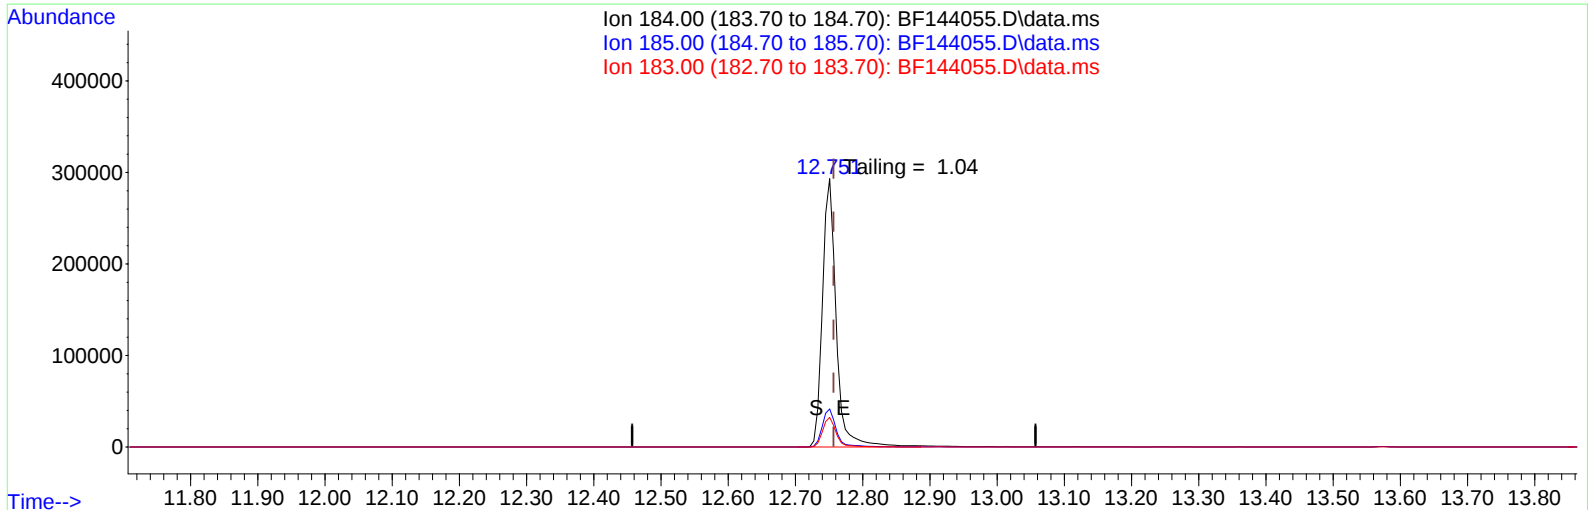

TIC: BF144055.D\data.ms

(77) Benzidine

12.751min (-0.006) 0.00 ng

response 416414

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.70	14.23
183.00	11.00	11.07
0.00	0.00	0.00