
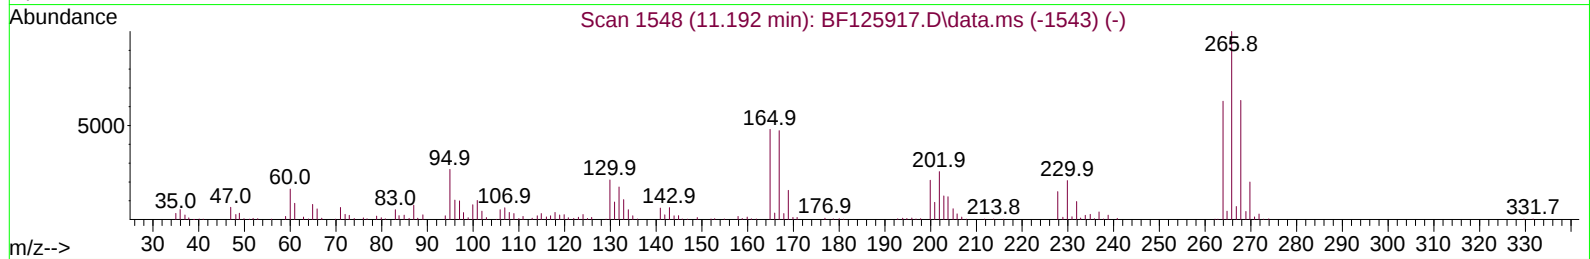
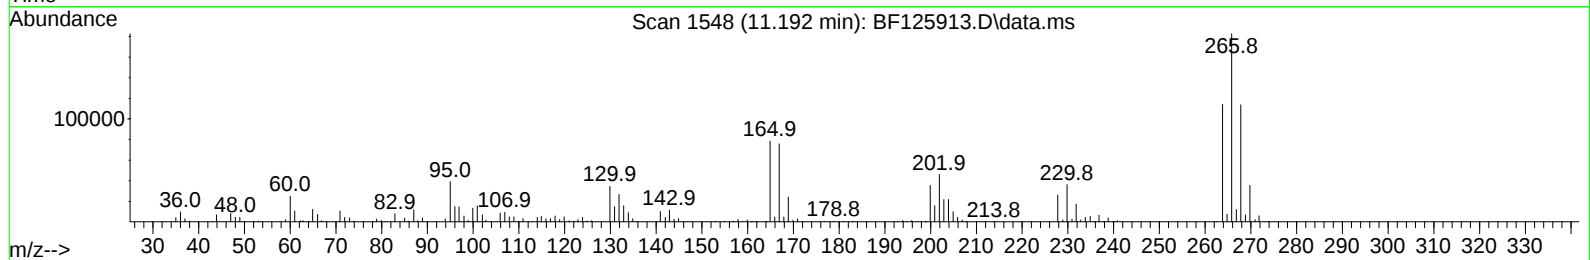


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF102521\  
Data File : BF125913.D  
Acq On : 25 Oct 2021 12:40  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 19:07:07 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF102521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Oct 25 18:49:16 2021  
Response via : Initial Calibration

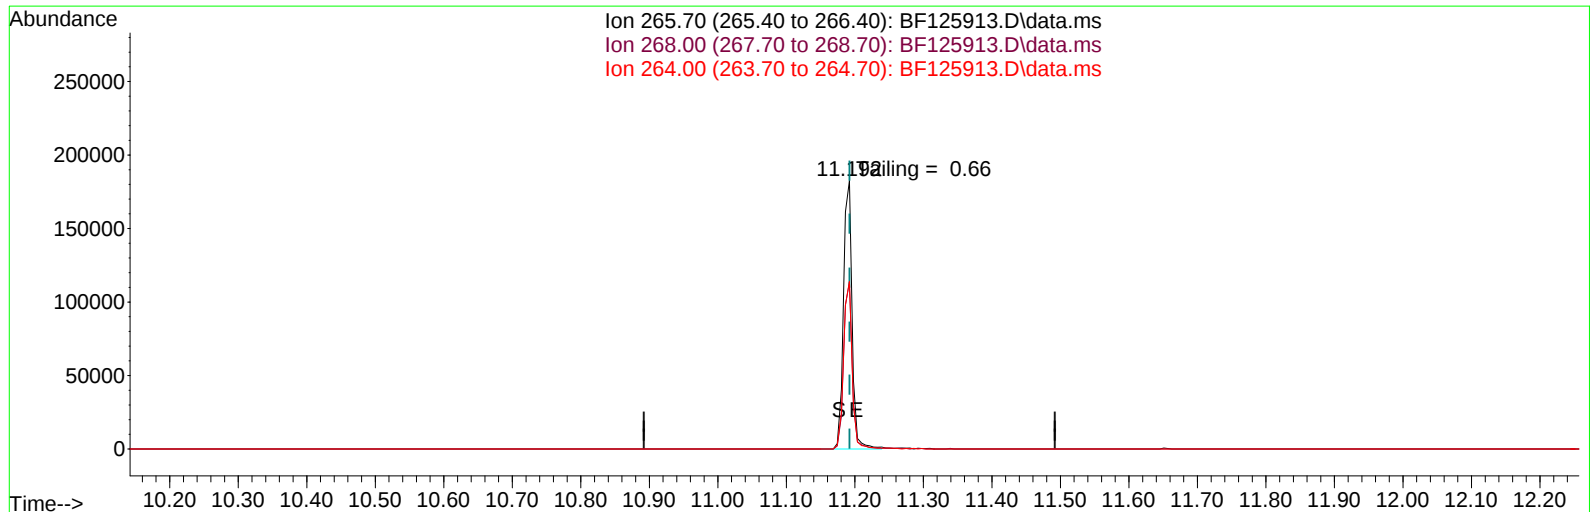

TIC: BF125913.D\data.ms

**(70) Pentachlorophenol (C)**




**11.192min (+ 0.000) 33273.01 ng**

**response 161200**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 61.10  | 62.25  |
| 264.00 | 69.90  | 62.44  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF102521\  
Data File : BF125913.D  
Acq On : 25 Oct 2021 12:40  
Operator : JU/CG  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 25 19:07:07 2021  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF102521.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Mon Oct 25 18:49:16 2021  
Response via : Initial Calibration

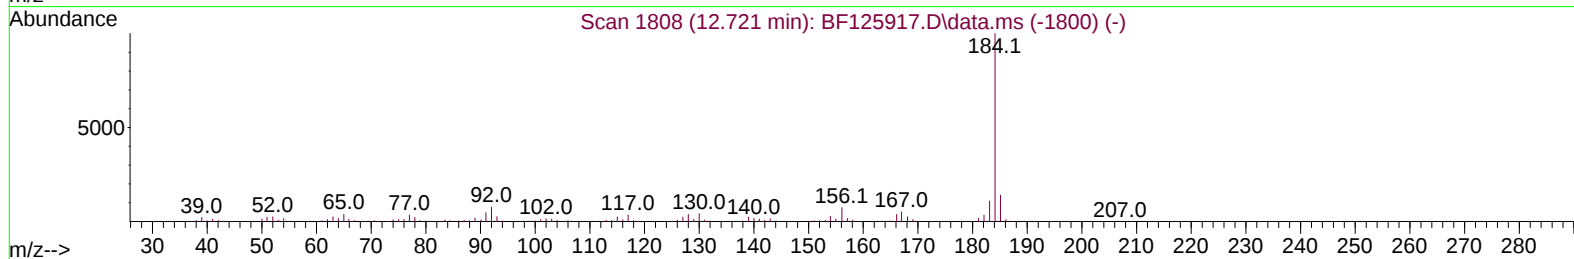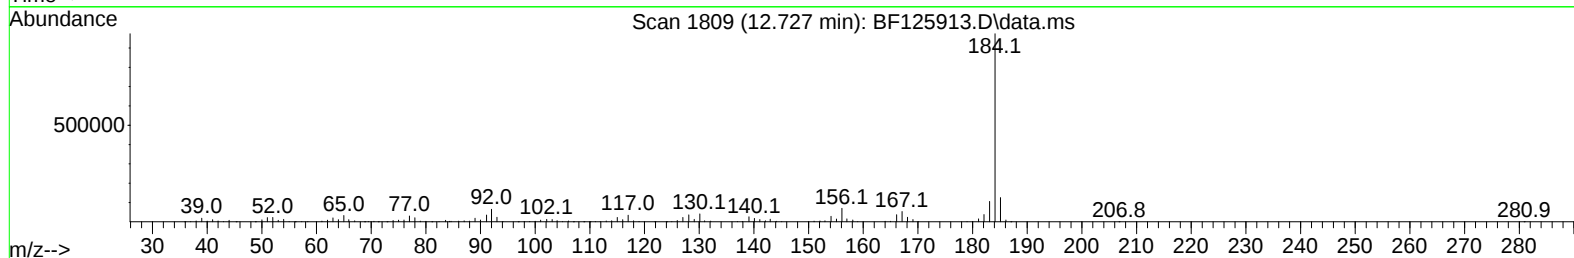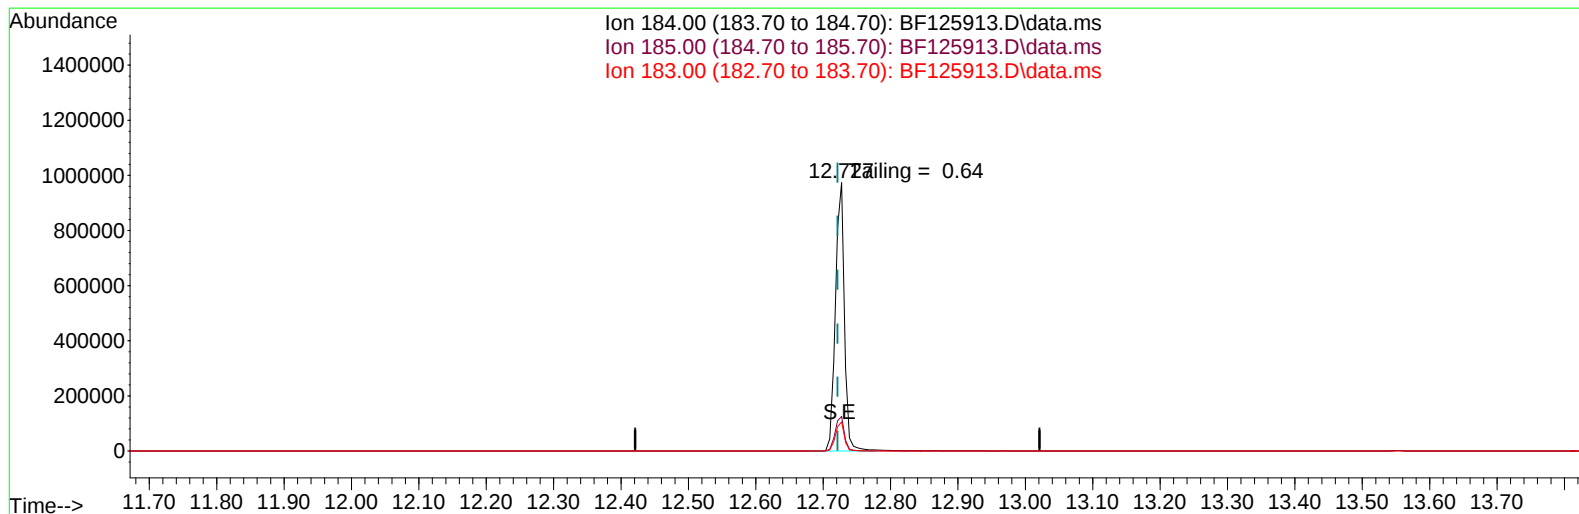

TIC: BF125913.D\data.ms

**(77) Benzidine**

12.727min (+ 0.006) 0.00 ng

response 906532

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 13.50  | 12.87  |
| 183.00 | 10.10  | 10.86  |
| 0.00   | 0.00   | 0.00   |