

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102521\
 Data File : BF125922.D
 Acq On : 25 Oct 2021 17:39
 Operator : JU/CG
 Sample : PB140166BL
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB140166BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125922.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.210	10	21	26	rVB	240958	324809	6.09%	0.907%
2	5.493	573	579	582	rBV	5004117	5334600	100.00%	14.892%
3	6.492	743	749	752	rBV	4568348	5317431	99.68%	14.844%
4	6.869	809	813	816	rBV	1302007	1052193	19.72%	2.937%
5	7.428	903	908	911	rBV	3419594	3526463	66.11%	9.844%
6	8.151	1026	1031	1034	rVB	1461026	1392628	26.11%	3.888%
7	9.228	1208	1214	1217	rBV	5326480	5163779	96.80%	14.415%
8	9.904	1324	1329	1332	rBV	1788289	1492447	27.98%	4.166%
9	10.692	1457	1463	1466	rBV	3692811	3420753	64.12%	9.549%
10	11.386	1577	1581	1584	rBV	1894572	1541149	28.89%	4.302%
11	12.980	1847	1852	1855	rBV	5358555	5158554	96.70%	14.401%
12	13.510	1939	1942	1947	rBV3	61853	58055	1.09%	0.162%
13	14.021	2025	2029	2033	rBV	1373606	1177228	22.07%	3.286%
14	15.492	2274	2279	2286	rBV	682294	801645	15.03%	2.238%
15	15.551	2286	2289	2296	rVB3	43823	59974	1.12%	0.167%

Sum of corrected areas: 35821708

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102521\
Data File : BF125922.D
Acq On : 25 Oct 2021 17:39
Operator : JU/CG
Sample : PB140166BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB140166BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.210	6.17 ng	324809	1,4-Dichlorobenzene-d4	6.869

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	25
3			1-Propene-1-thiol	74	C3H6S	000925-89-3	9
4			Methane, isothiocyanato-	73	C2H3NS	000556-61-6	9
5			Silane, tetramethyl-	88	C4H12Si	000075-76-3	9

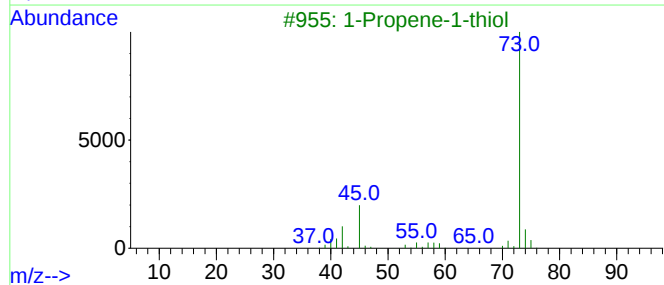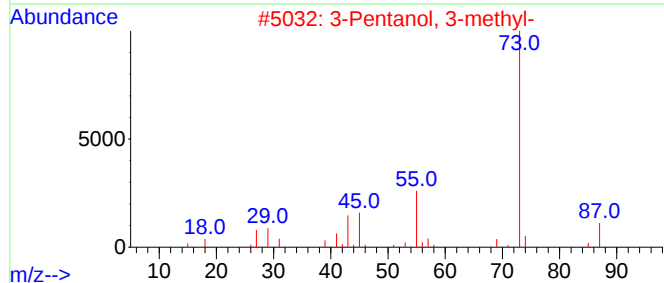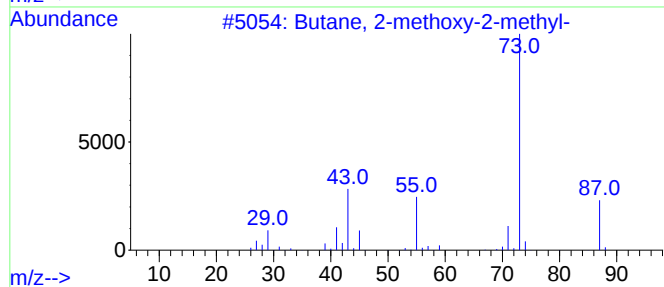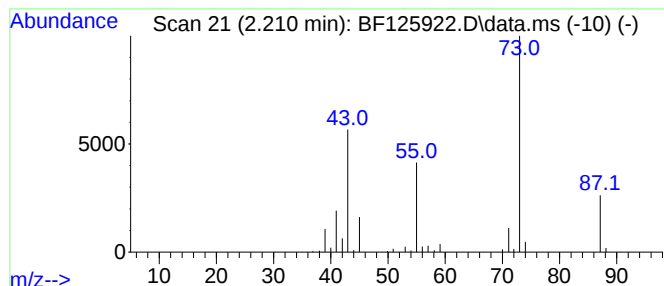

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102521\
Data File : BF125922.D
Acq On : 25 Oct 2021 17:39
Operator : JU/CG
Sample : PB140166BL
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB140166BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.210	6.2	ng	324809	1	6.869	1052190	20.0