


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102521\
 Data File : BF125913.D
 Acq On : 25 Oct 2021 12:40
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 25 18:49:16 2021

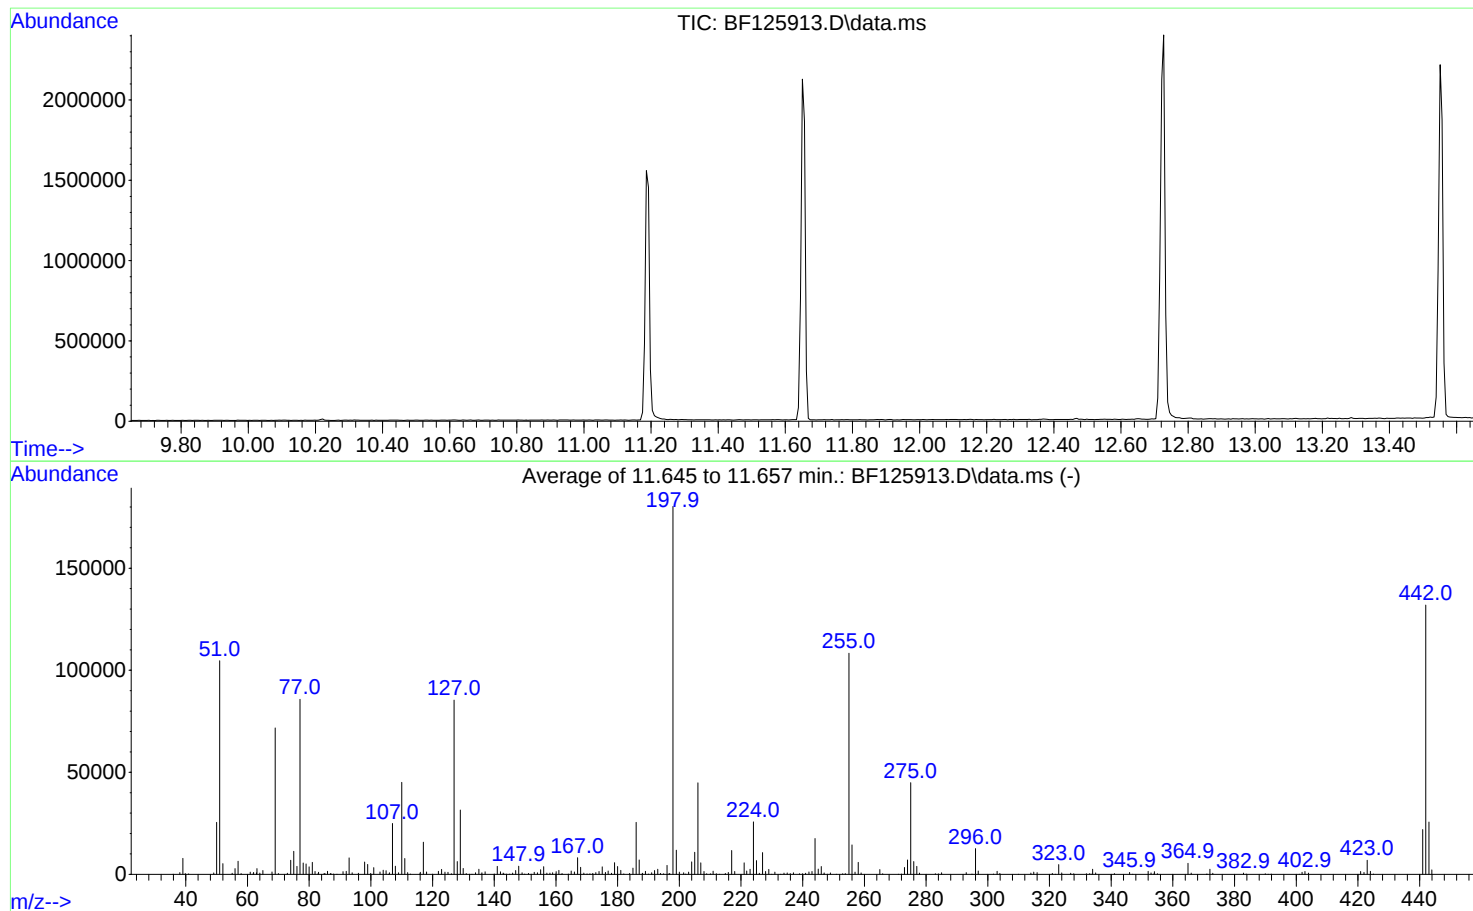




AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1621

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	58.1	104640	PASS
68	69	0.00	2	1.6	1174	PASS
69	198	0.00	100	39.8	71704	PASS
70	69	0.00	2	0.5	372	PASS
127	198	10	80	47.4	85403	PASS
197	198	0.00	2	0.2	432	PASS
198	198	100	100	100.0	180229	PASS
199	198	5	9	6.6	11857	PASS
275	198	10	60	24.9	44910	PASS
365	198	1	100	3.0	5423	PASS
441	198	0.01	100	12.2	21931	PASS
442	442	50	100	100.0	131904	PASS
443	442	15	24	19.5	25678	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102521\
Data File : BF125913.D
Acq On : 25 Oct 2021 12:40
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 25 19:07:07 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 25 18:49:16 2021
Response via : Initial Calibration

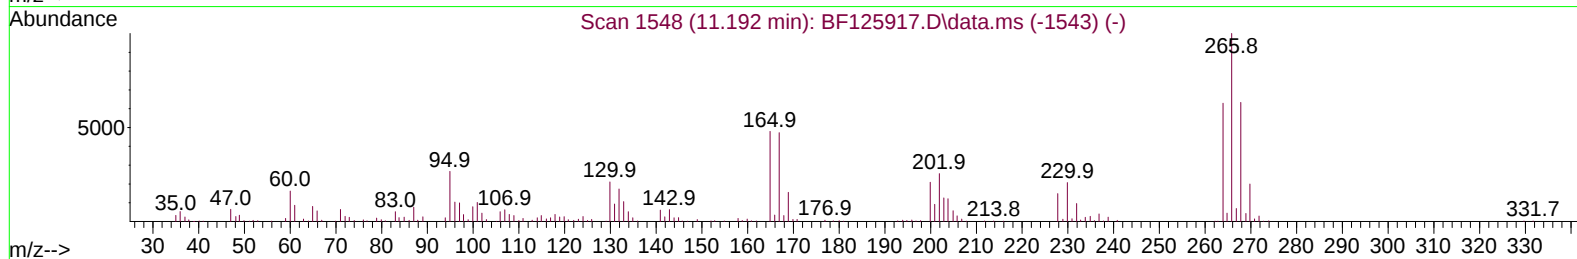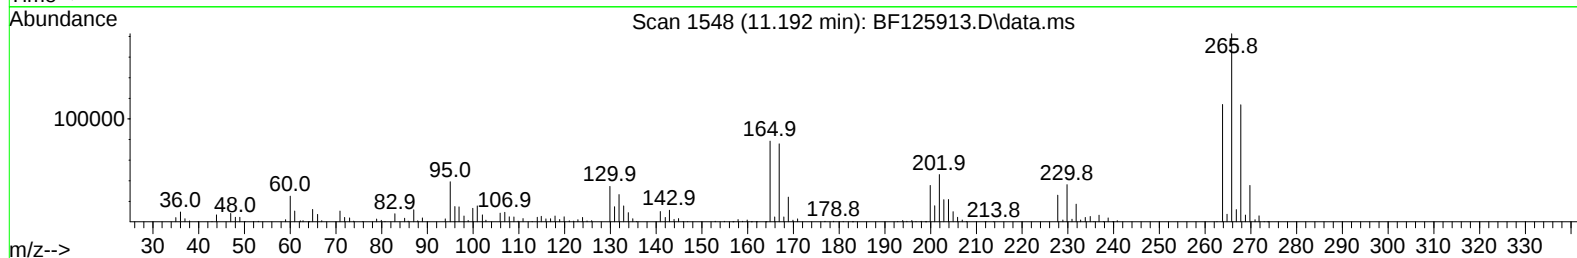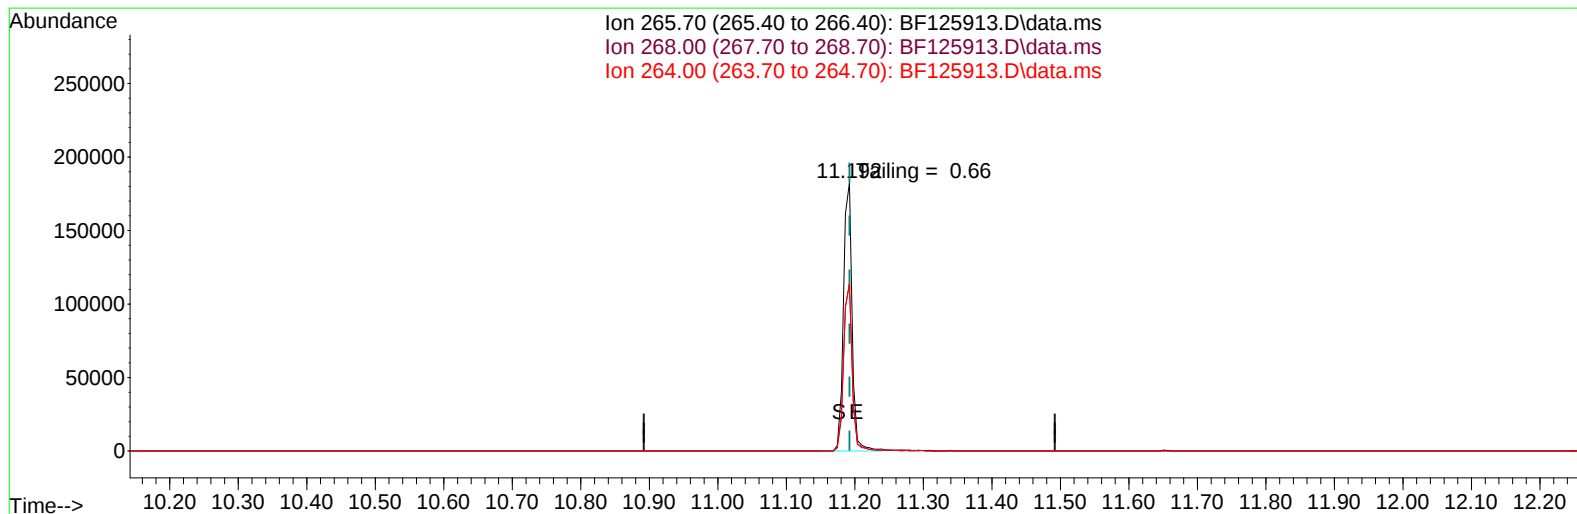

TIC: BF125913.D\data.ms

(70) Pentachlorophenol (C)

11.192min (+ 0.000) 33273.01 ng




response 161200

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.25
264.00	69.90	62.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102521\
 Data File : BF125913.D
 Acq On : 25 Oct 2021 12:40
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 25 19:07:07 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF102521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Oct 25 18:49:16 2021
 Response via : Initial Calibration

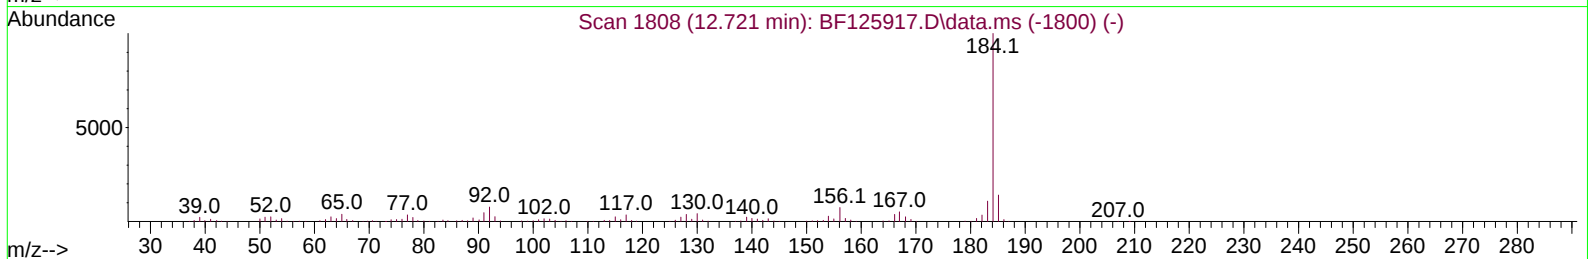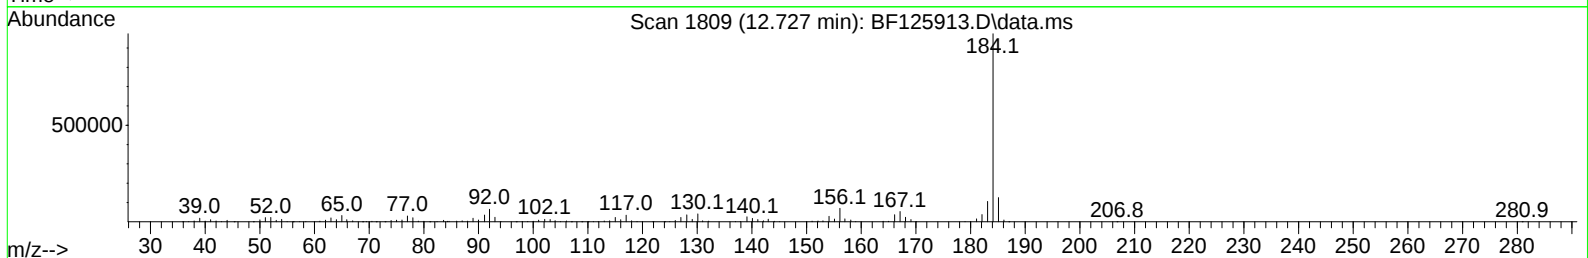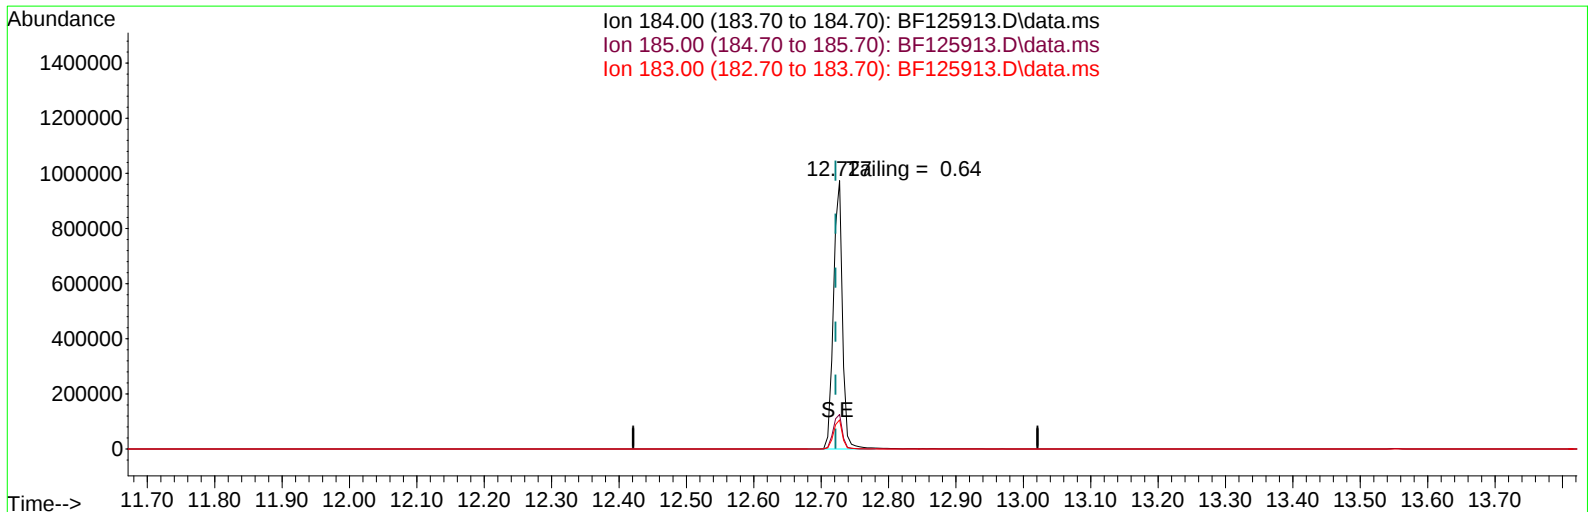

TIC: BF125913.D\data.ms

(77) Benzidine

12.727min (+ 0.006) 0.00 ng

response 906532

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	12.87
183.00	10.10	10.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/25/2021	BNA_F	<u>BF125913.D</u>
Compound Name	Response	Retention Time
DDT	345032	13.55
DDD	620	13.25
DDE	0	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
620	345652	0.18