
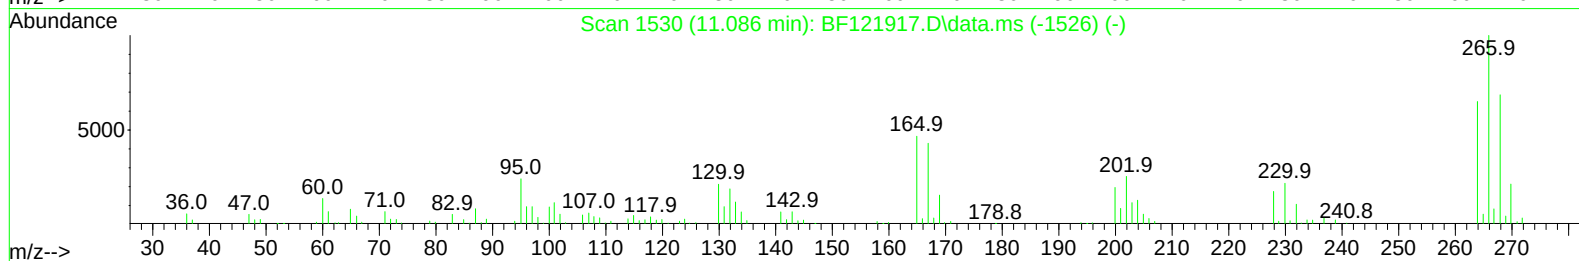
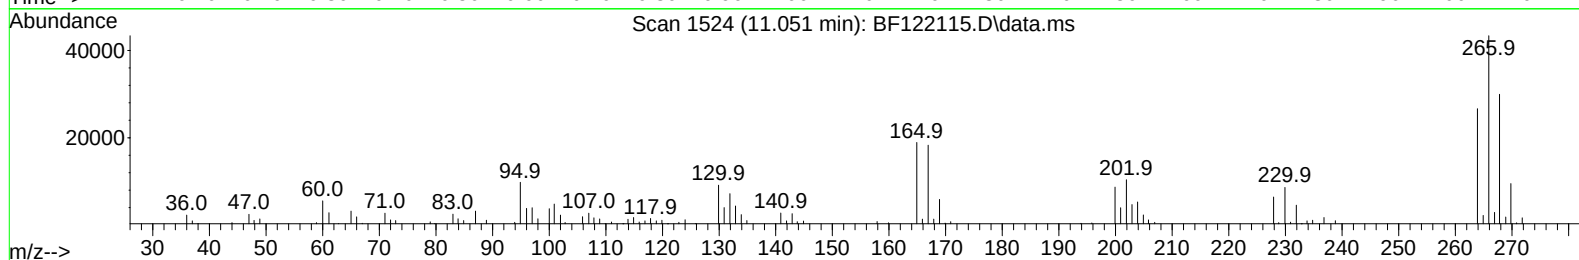


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102620\
Data File : BF122115.D
Acq On : 26 Oct 2020 14:15
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 02:52:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 17:27:32 2020
Response via : Initial Calibration

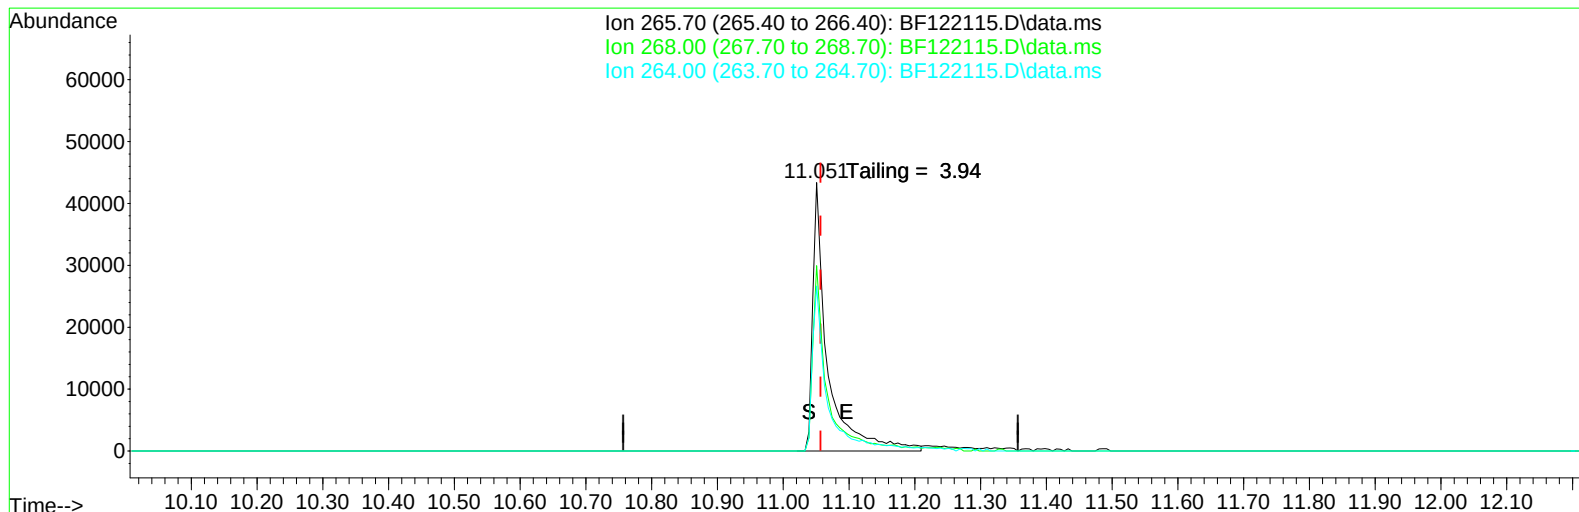

TIC: BF122115.D\data.ms

(70) Pentachlorophenol (C)




11.051min (-0.006) 102254.29 ng

response 68289

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	69.03
264.00	62.40	61.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102620\
Data File : BF122115.D
Acq On : 26 Oct 2020 14:15
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 27 02:52:25 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Oct 26 17:27:32 2020
Response via : Initial Calibration

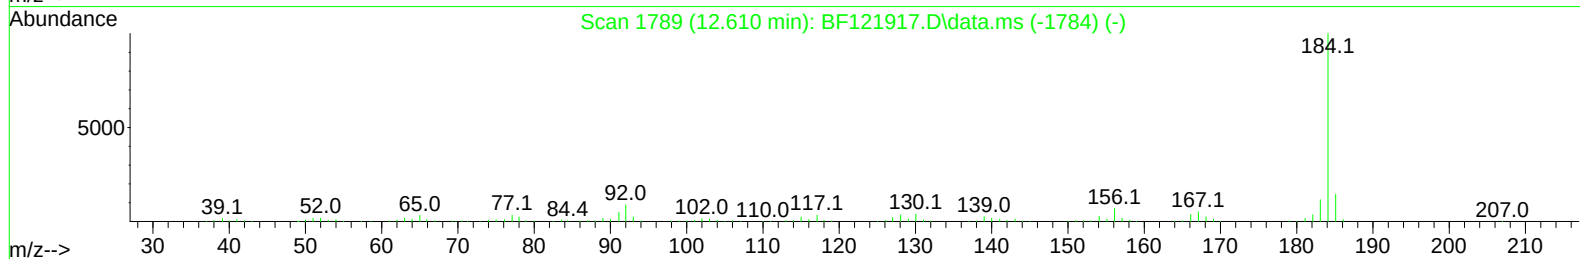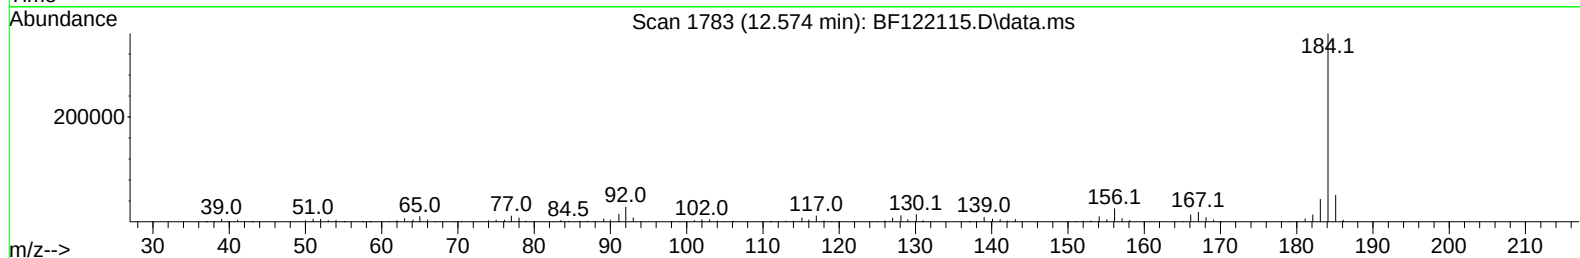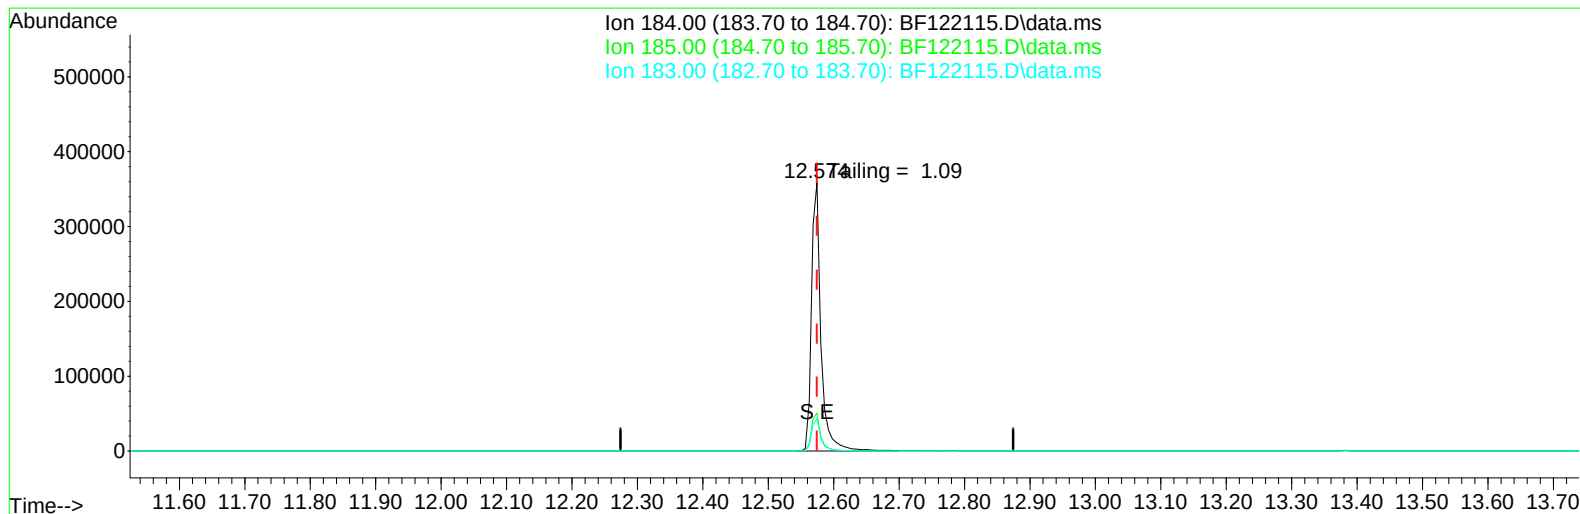

TIC: BF122115.D\data.ms

(77) Benzidine

12.574min (-0.000) 0.00 ng

response 362706

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.17
183.00	11.70	12.04
0.00	0.00	0.00