
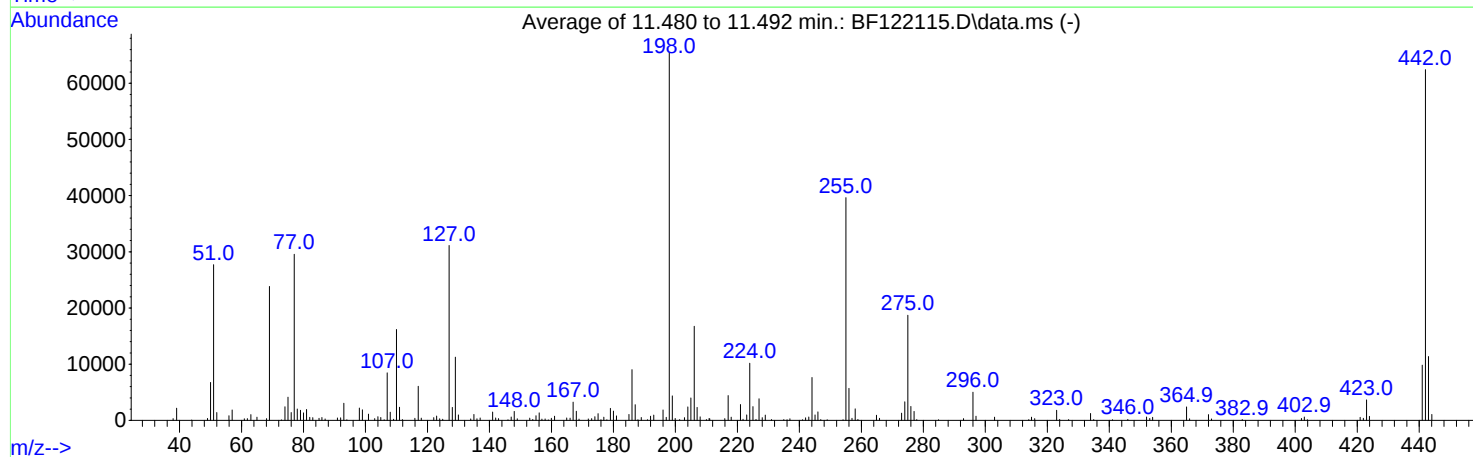


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102620\
 Data File : BF122115.D
 Acq On : 26 Oct 2020 14:15
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF101220.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Oct 26 17:27:32 2020

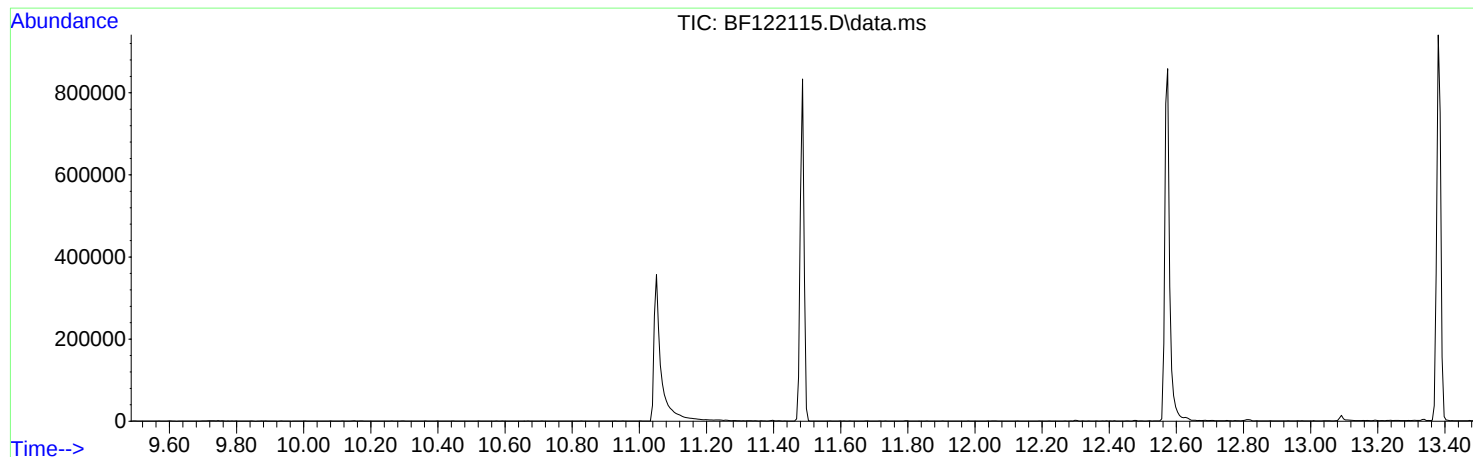

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	27716	PASS
68	69	0.00	2	1.4	327	PASS
69	198	0.00	100	36.4	23827	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.5	31119	PASS
197	198	0.00	2	0.8	549	PASS
198	198	100	100	100.0	65475	PASS
199	198	5	9	6.6	4350	PASS
275	198	10	60	28.6	18721	PASS
365	198	1	100	3.7	2402	PASS
441	198	0.01	100	15.0	9842	PASS
442	198	50	100	95.4	62432	PASS
443	442	15	24	18.2	11375	PASS