
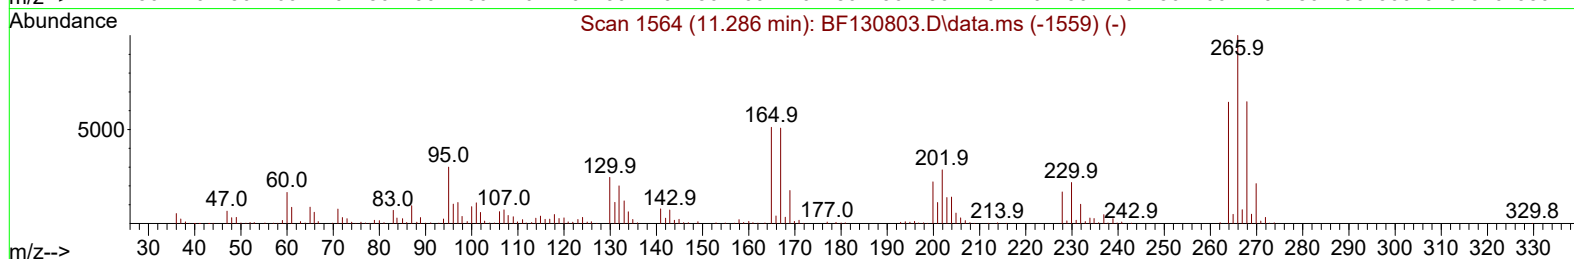
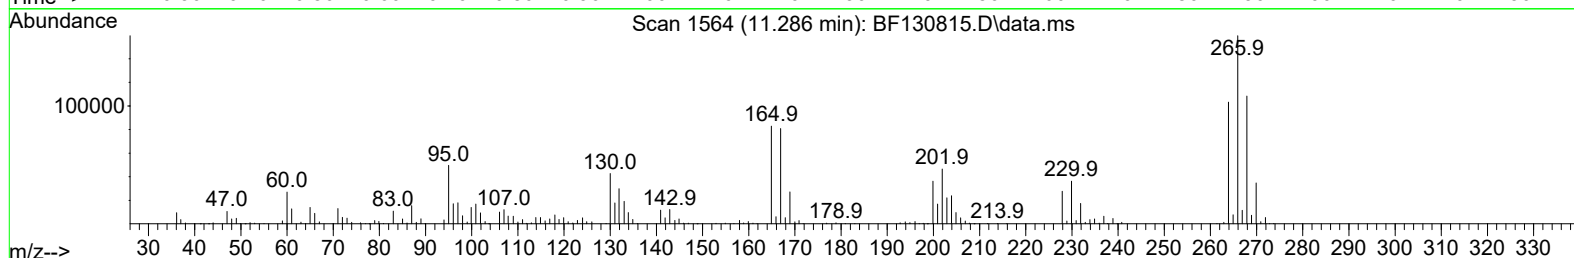


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
Data File : BF130815.D
Acq On : 28 Oct 2022 08:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 08:13:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 05:41:34 2022
Response via : Initial Calibration

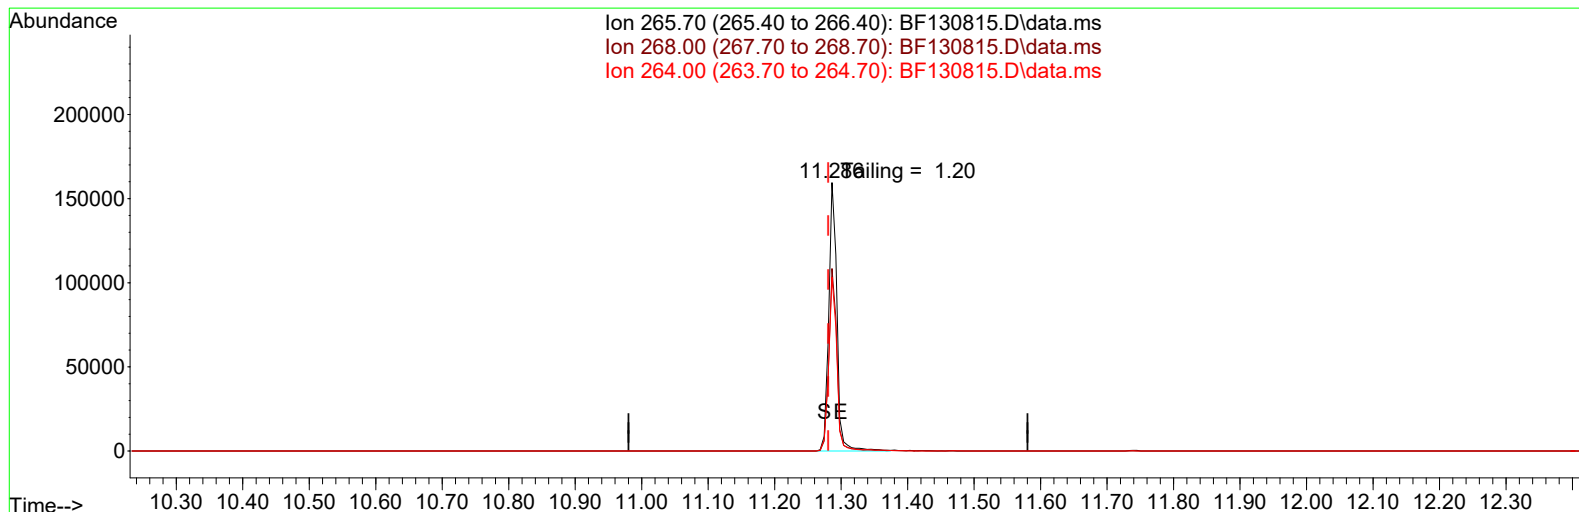

TIC: BF130815.D\data.ms

(70) Pentachlorophenol (C)




11.286min (+ 0.006) 335744.73 ng

response 137983

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	67.97
264.00	64.50	64.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
Data File : BF130815.D
Acq On : 28 Oct 2022 08:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 29 08:13:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 05:41:34 2022
Response via : Initial Calibration

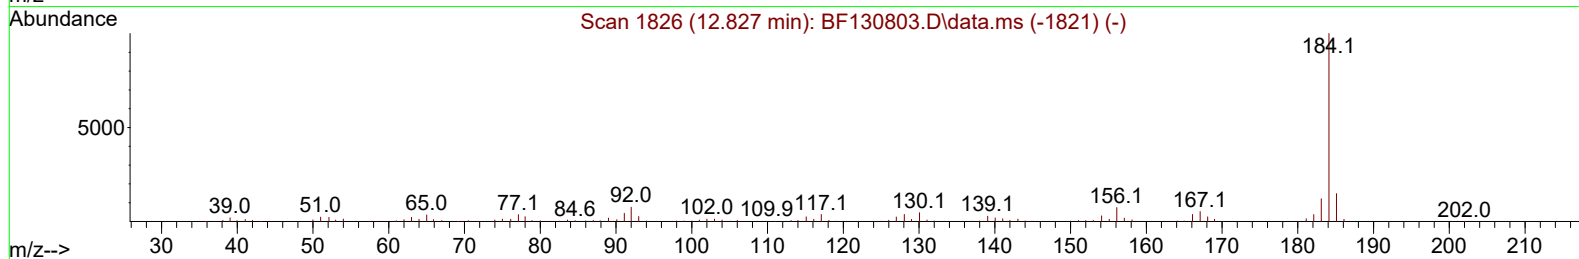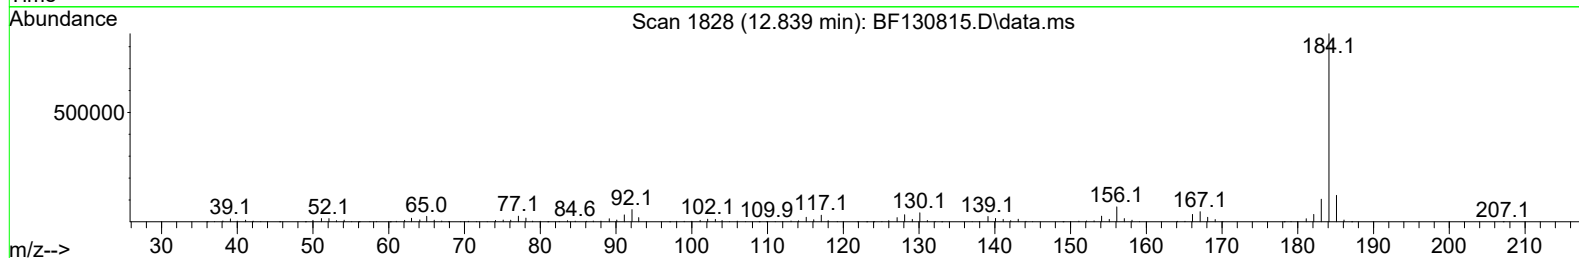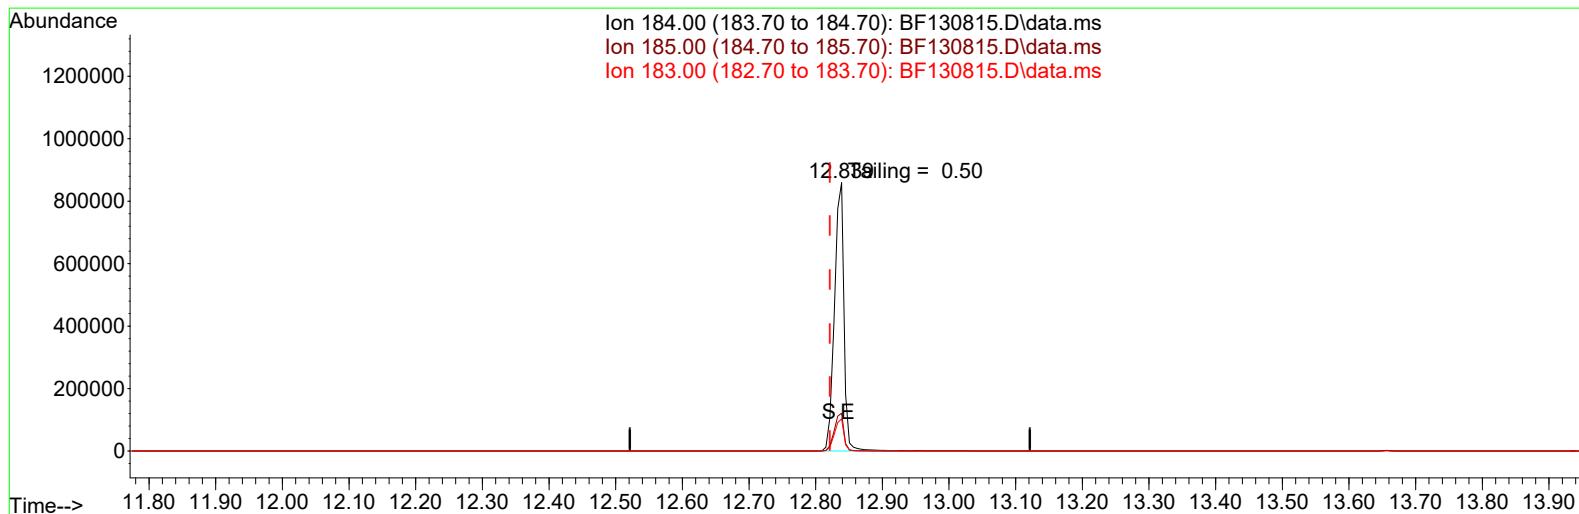

TIC: BF130815.D\data.ms

(77) Benzidine

12.839min (+ 0.017) 0.00 ng

response 856006

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.07
183.00	12.10	12.02
0.00	0.00	0.00