

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
 Data File : BF130849.D
 Acq On : 29 Oct 2022 04:26
 Operator : CG\JU
 Sample : N5281-06
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-6

Quant Time: Oct 29 05:49:24 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 29 05:41:34 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.945	152	92174	20.000	ng	0.00
21) Naphthalene-d8	8.227	136	349169	20.000	ng	0.00
39) Acenaphthene-d10	9.986	164	181822	20.000	ng	-0.01
64) Phenanthrene-d10	11.480	188	293318	20.000	ng	0.00
76) Chrysene-d12	14.121	240	173342	20.000	ng	#-0.01
86) Perylene-d12	15.639	264	167079	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.563	112	542990	102.126	ng	0.00
7) Phenol-d6	6.557	99	727869	105.347	ng	0.00
23) Nitrobenzene-d5	7.504	82	477154	82.401	ng	-0.01
42) 2,4,6-Tribromophenol	10.780	330	135876	88.774	ng	0.00
45) 2-Fluorobiphenyl	9.310	172	861956	71.673	ng	0.00
79) Terphenyl-d14	13.068	244	668895	70.711	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
Data File : BF130849.D
Acq On : 29 Oct 2022 04:26
Operator : CG\JU
Sample : N5281-06
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-6

Quant Time: Oct 29 05:49:24 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 05:41:34 2022
Response via : Initial Calibration




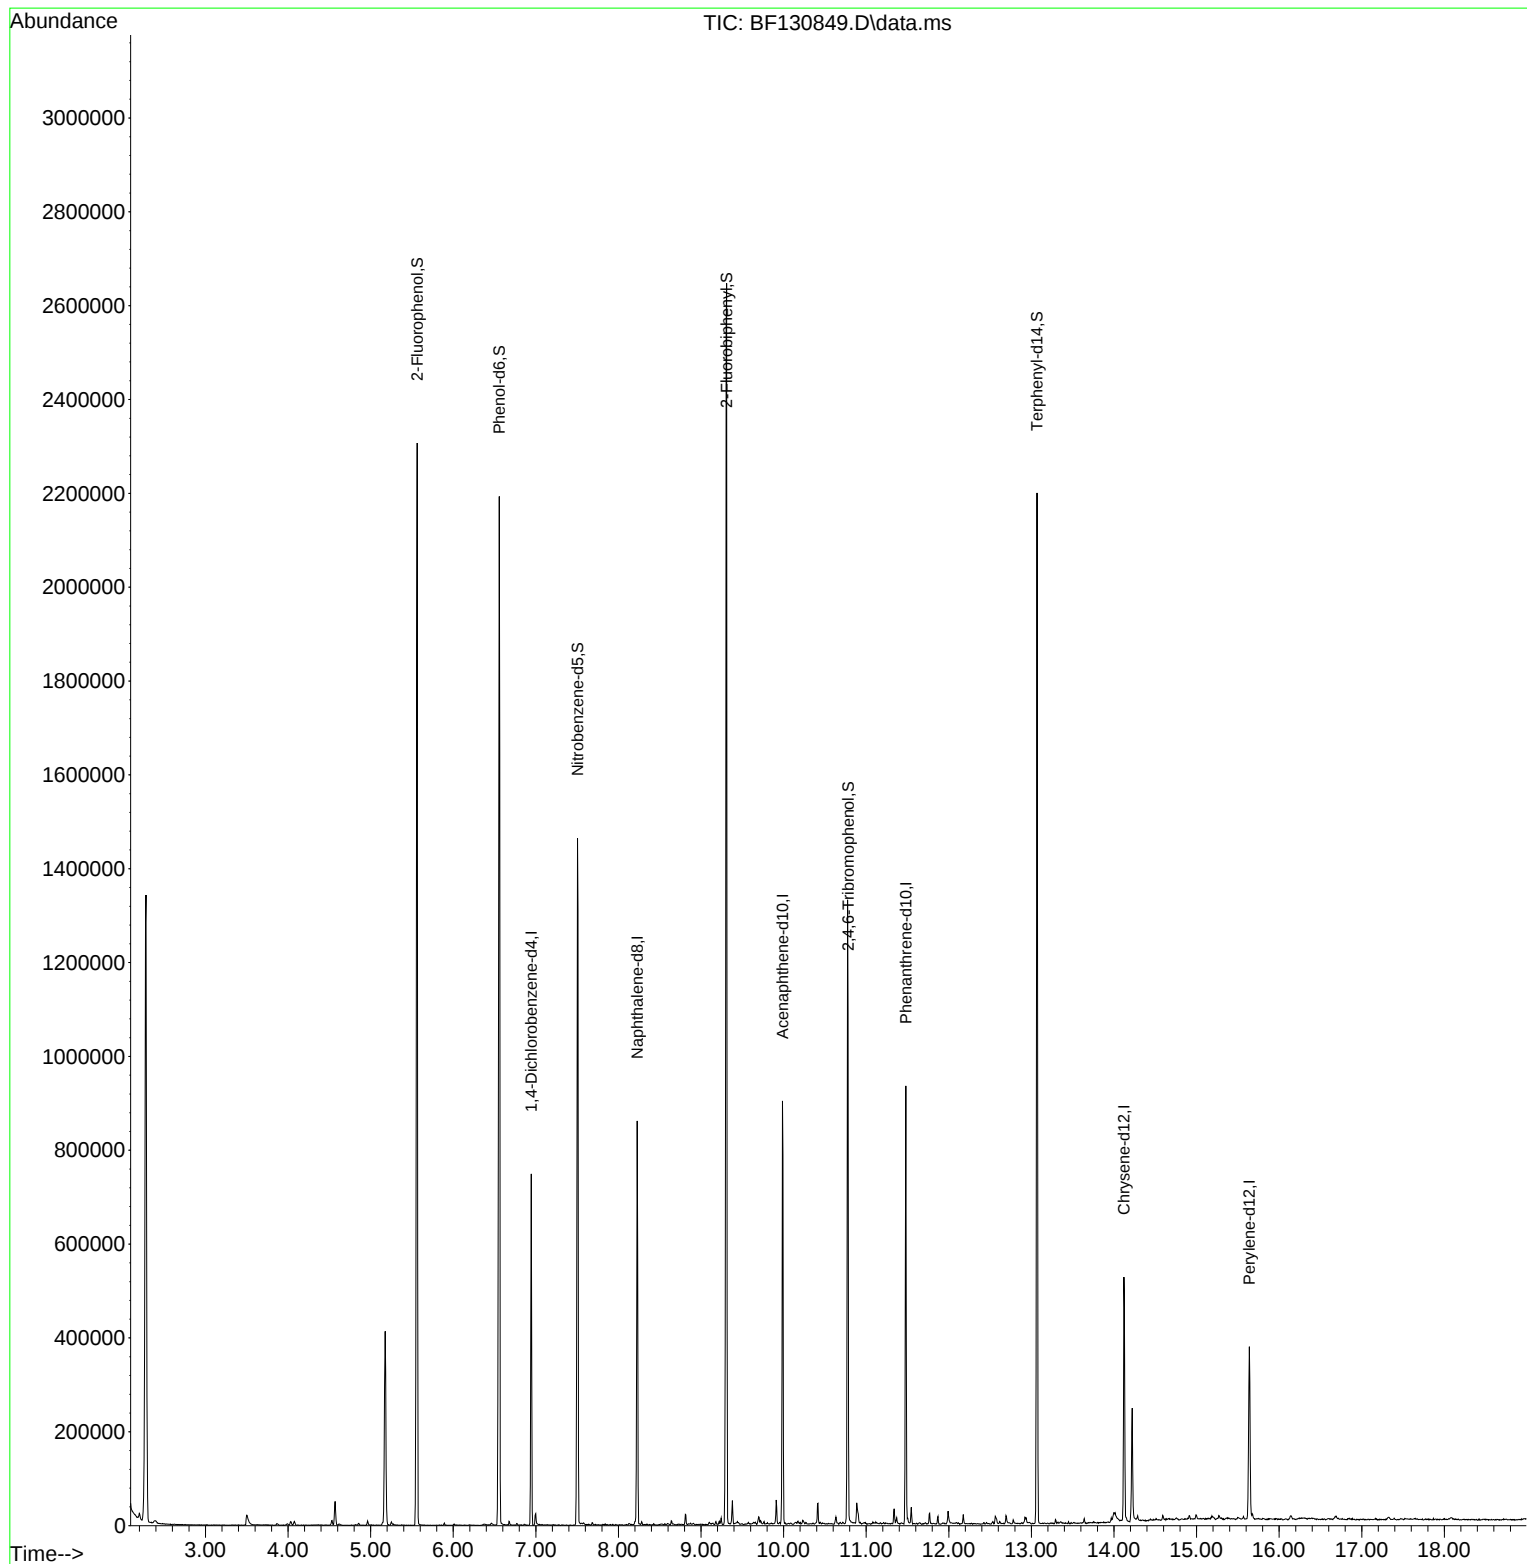


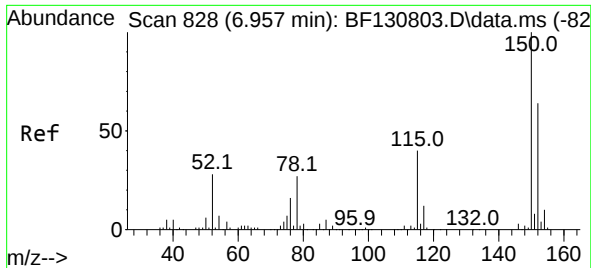

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.945 min Scan# 81
Delta R.T. 0.000 min
Lab File: BF130849.D
Acq: 29 Oct 2022 04:26




Instrument :
BNA_F
ClientSampleId :
SB-6

Tgt Ion:152 Resp: 92174
Ion Ratio Lower Upper
152 100
150 155.4 124.1 186.1
115 60.9 50.1 75.1

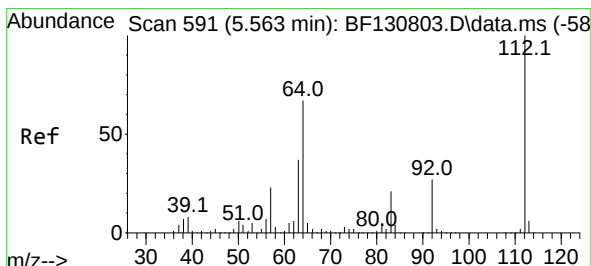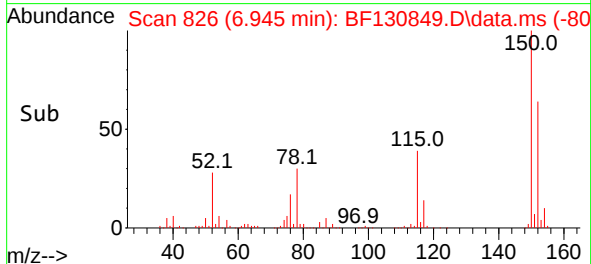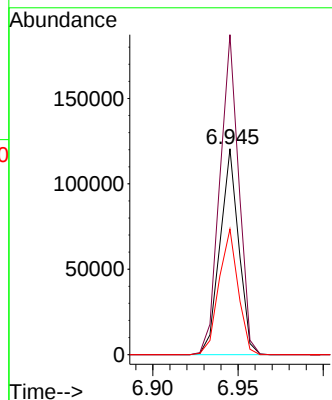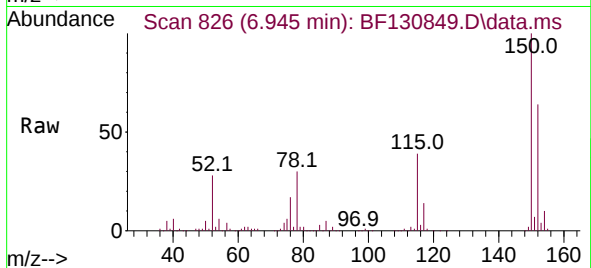

#5
2-Fluorophenol
Concen: 102.126 ng
RT: 5.563 min Scan# 591
Delta R.T. 0.006 min
Lab File: BF130849.D
Acq: 29 Oct 2022 04:26

Tgt Ion:112 Resp: 542990
Ion Ratio Lower Upper
112 100
64 67.6 53.9 80.9
63 38.0 29.4 44.2

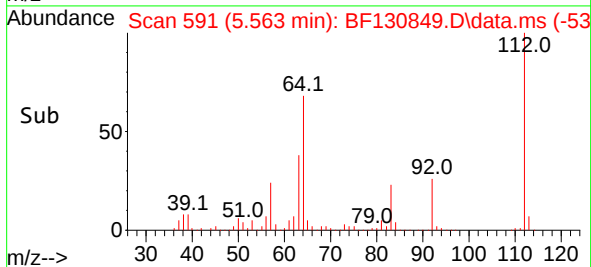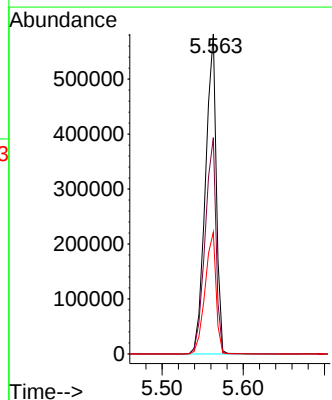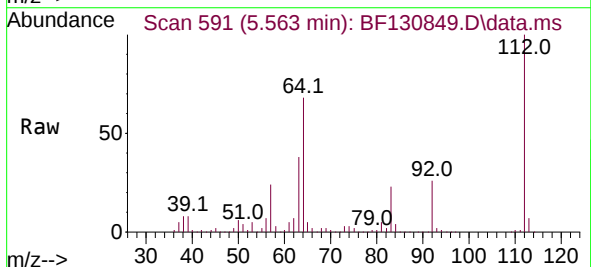



#7
Phenol-d6
Concen: 105.347 ng
RT: 6.557 min Scan# 760
Delta R.T. -0.006 min
Lab File: BF130849.D
Acq: 29 Oct 2022 04:26





Instrument :

BNA_F

ClientSampleId :




SB-6

Tgt Ion: 99 Resp: 727869
Ion Ratio Lower Upper
99 100
42 25.4 18.8 28.2
71 42.0 31.4 47.0

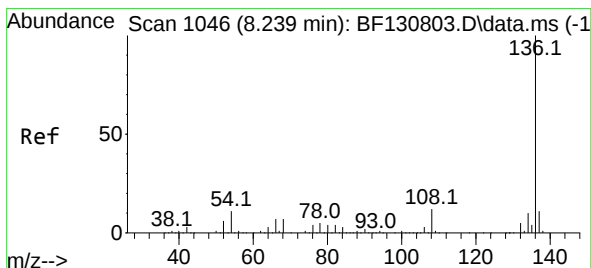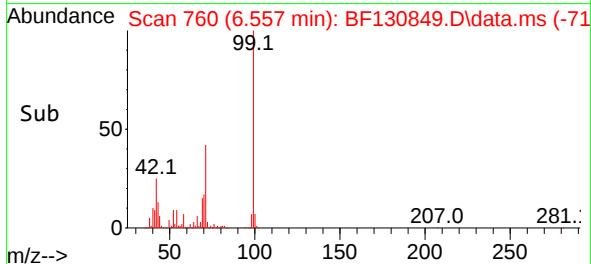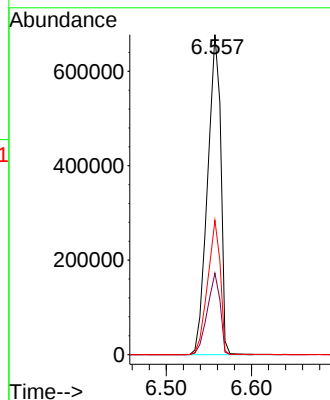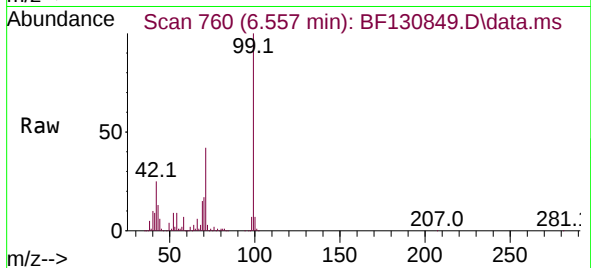

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 8.227 min Scan# 1044
Delta R.T. -0.006 min
Lab File: BF130849.D
Acq: 29 Oct 2022 04:26

Tgt Ion: 136 Resp: 349169
Ion Ratio Lower Upper
136 100
137 10.3 9.2 13.8
54 10.2 8.8 13.2
68 5.5 5.2 7.8


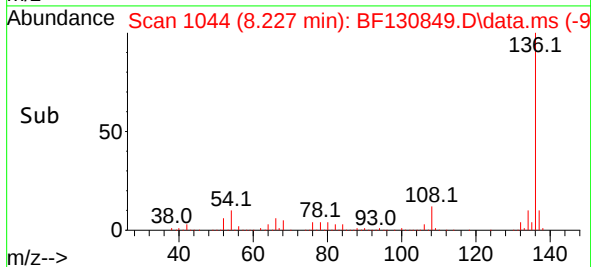
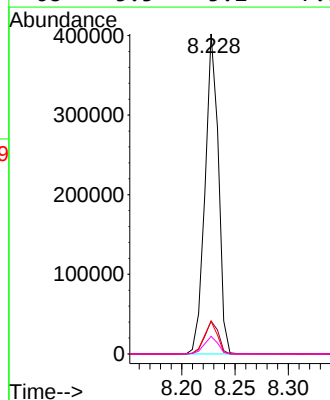
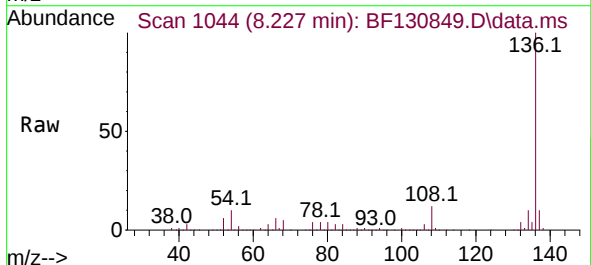




#23
Nitrobenzene-d5
Concen: 82.401 ng
RT: 7.504 min Scan# 91
Delta R.T. -0.012 min
Lab File: BF130849.D
Acq: 29 Oct 2022 04:26




Instrument :
BNA_F
ClientSampleId :
SB-6


Tgt Ion: 82 Resp: 477154
Ion Ratio Lower Upper
82 100
128 39.3 31.2 46.8
54 61.2 48.0 72.0

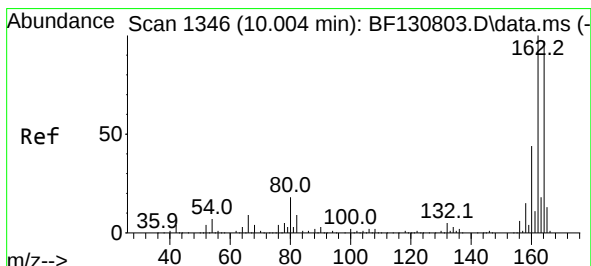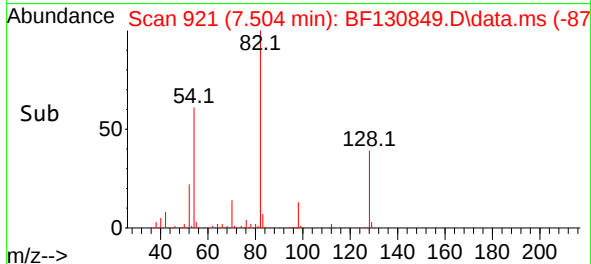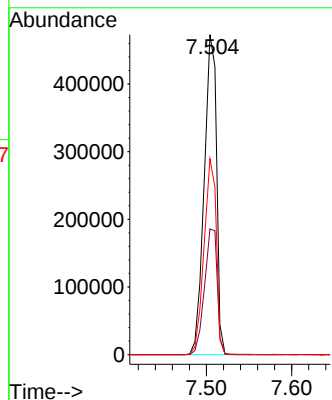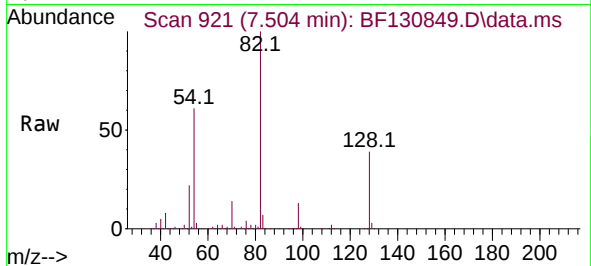

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.986 min Scan# 1343
Delta R.T. -0.012 min
Lab File: BF130849.D
Acq: 29 Oct 2022 04:26

Tgt Ion:164 Resp: 181822
Ion Ratio Lower Upper
164 100
162 98.7 82.2 123.2
160 45.9 36.6 54.8

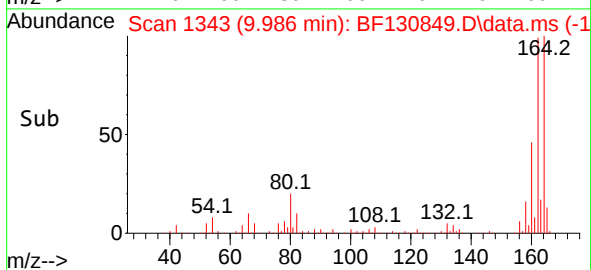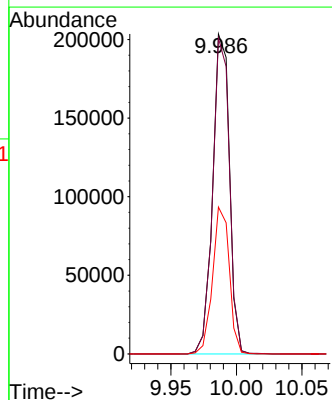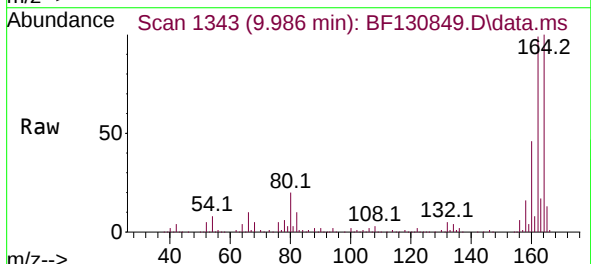

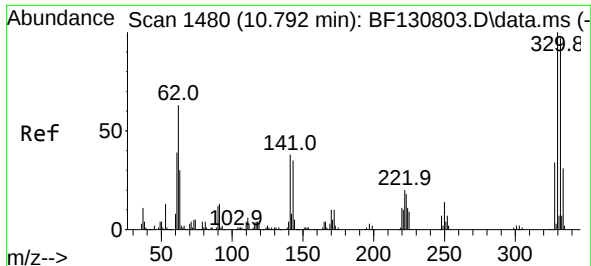

#42

2,4,6-Tribromophenol

Concen: 88.774 ng

RT: 10.780 min Scan# 1480

Delta R.T. -0.006 min

Lab File: BF130849.D

Acq: 29 Oct 2022 04:26

Instrument :

BNA_F

ClientSampleId :

SB-6





Tgt Ion:330 Resp: 135876

Ion Ratio Lower Upper

330 100

332 94.6 76.2 114.4

141 38.3 31.4 47.0

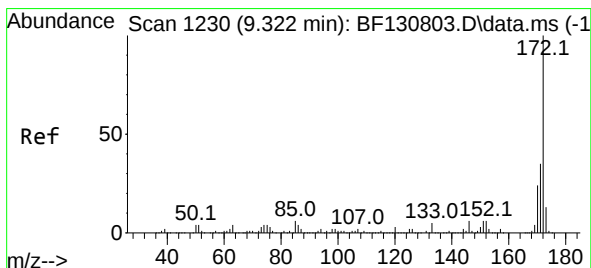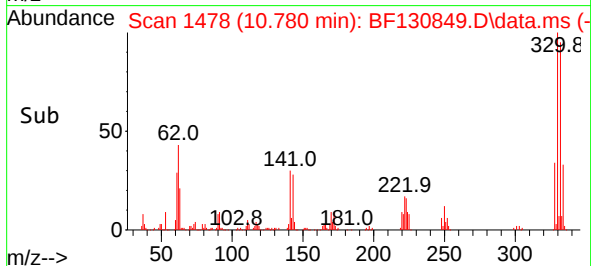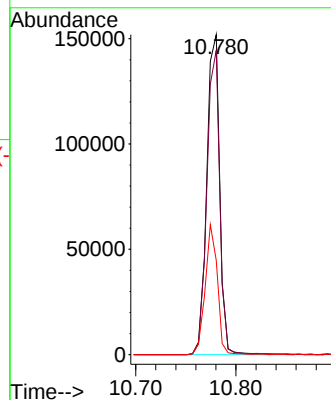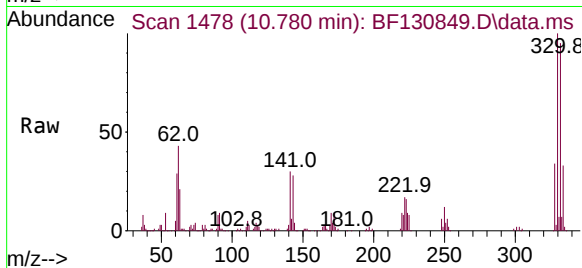

#45

2-Fluorobiphenyl

Concen: 71.673 ng

RT: 9.310 min Scan# 1228

Delta R.T. -0.000 min

Lab File: BF130849.D

Acq: 29 Oct 2022 04:26




Tgt Ion:172 Resp: 861956


Ion Ratio Lower Upper

172 100

171 35.5 28.1 42.1

170 23.4 19.0 28.4

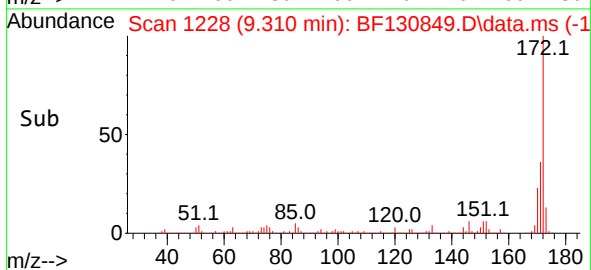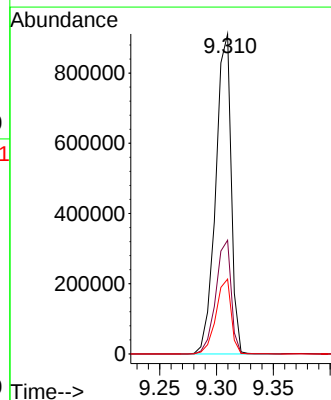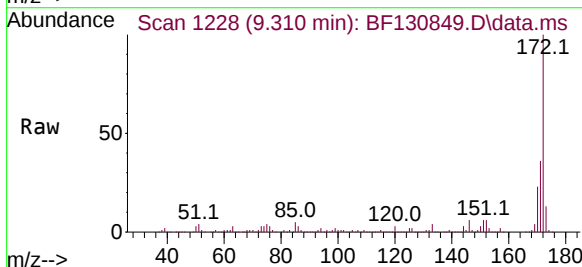

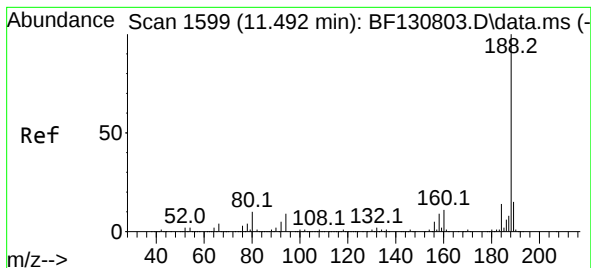

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.480 min Scan# 11

Delta R.T. -0.006 min

Lab File: BF130849.D

Acq: 29 Oct 2022 04:26

Instrument :

BNA_F

ClientSampleId :

SB-6





Tgt Ion:188 Resp: 293318

Ion Ratio Lower Upper

188 100

94 8.2 7.4 11.2

80 8.9 8.0 12.0

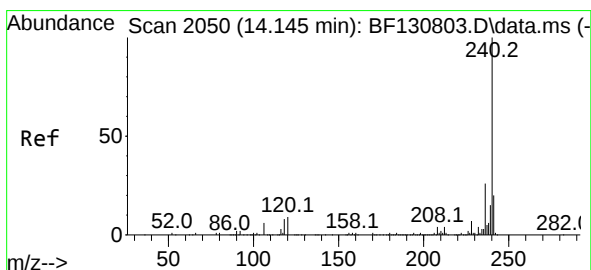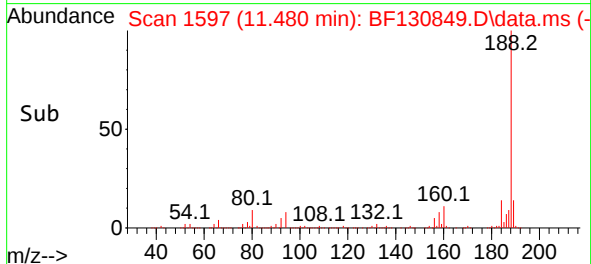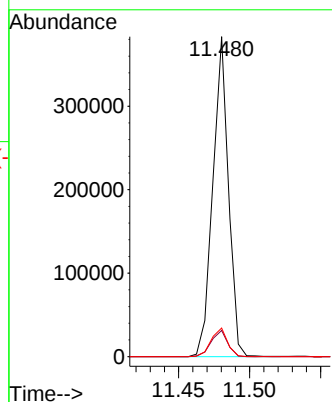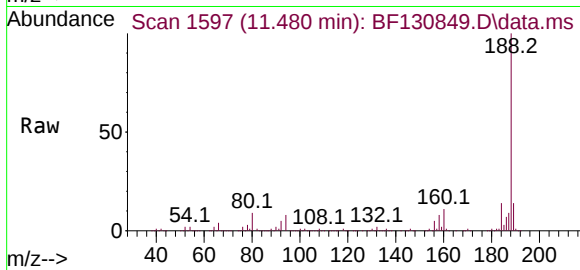

#76

Chrysene-d12

Concen: 20.000 ng

RT: 14.121 min Scan# 2046

Delta R.T. -0.012 min

Lab File: BF130849.D

Acq: 29 Oct 2022 04:26




Tgt Ion:240 Resp: 173342


Ion Ratio Lower Upper

240 100

120 11.4 7.0 10.4#

236 25.1 20.5 30.7


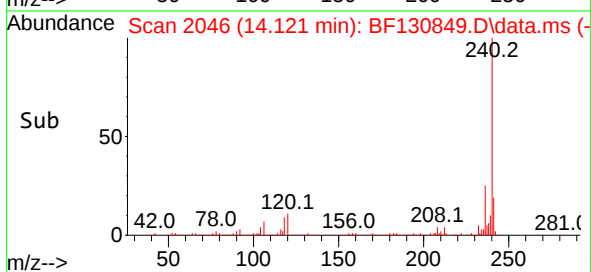
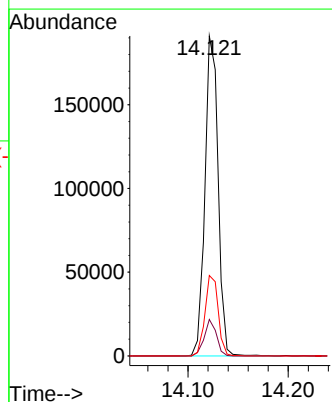
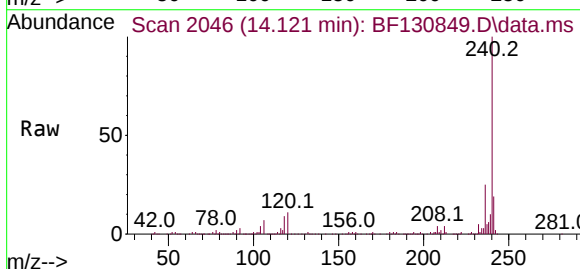


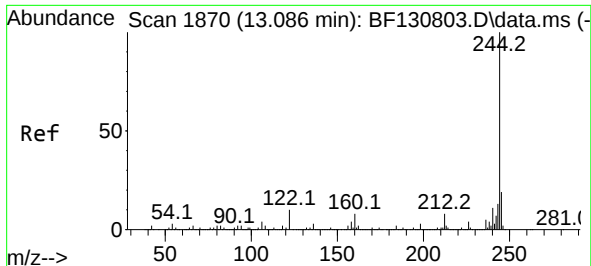

#79
 Terphenyl-d14
 Concen: 70.711 ng
 RT: 13.068 min Scan# 1870
 Delta R.T. -0.006 min
 Lab File: BF130849.D
 Acq: 29 Oct 2022 04:26

Instrument :
 BNA_F
 ClientSampleId :
 SB-6

Tgt Ion:244 Resp: 668895
 Ion Ratio Lower Upper
 244 100
 212 7.8 6.2 9.2
 122 10.3 7.9 11.9

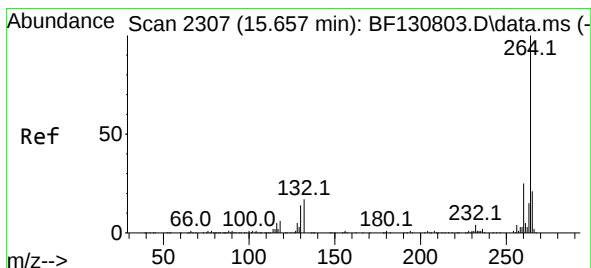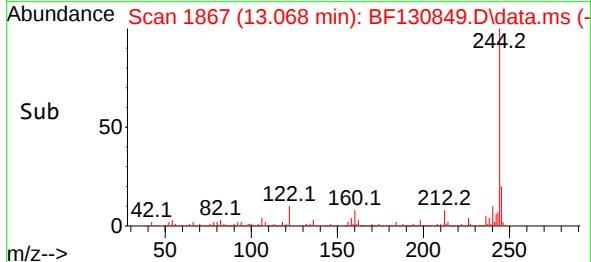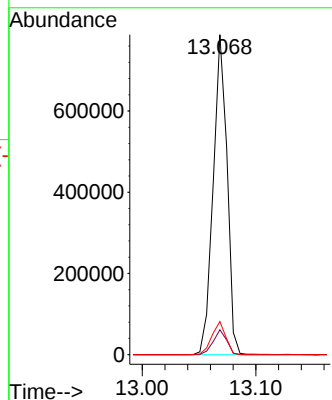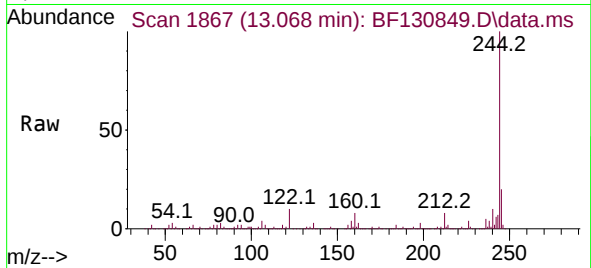

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.639 min Scan# 2304
 Delta R.T. -0.006 min
 Lab File: BF130849.D
 Acq: 29 Oct 2022 04:26

Tgt Ion:264 Resp: 167079
 Ion Ratio Lower Upper
 264 100
 260 23.7 19.9 29.9
 265 22.0 17.0 25.6

