
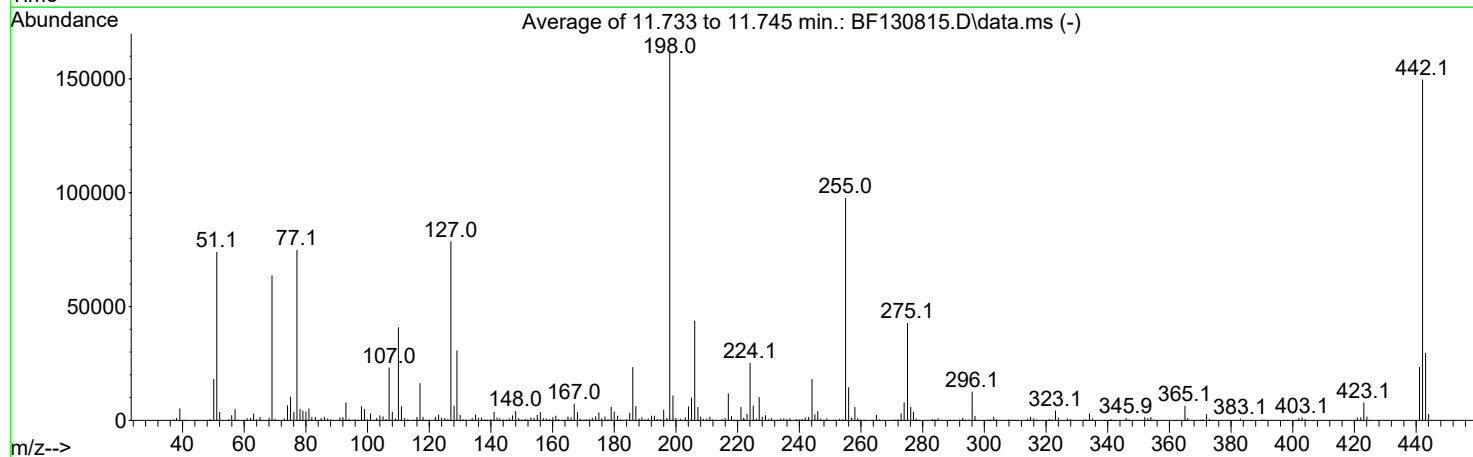


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
 Data File : BF130815.D
 Acq On : 28 Oct 2022 08:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 29 05:41:34 2022

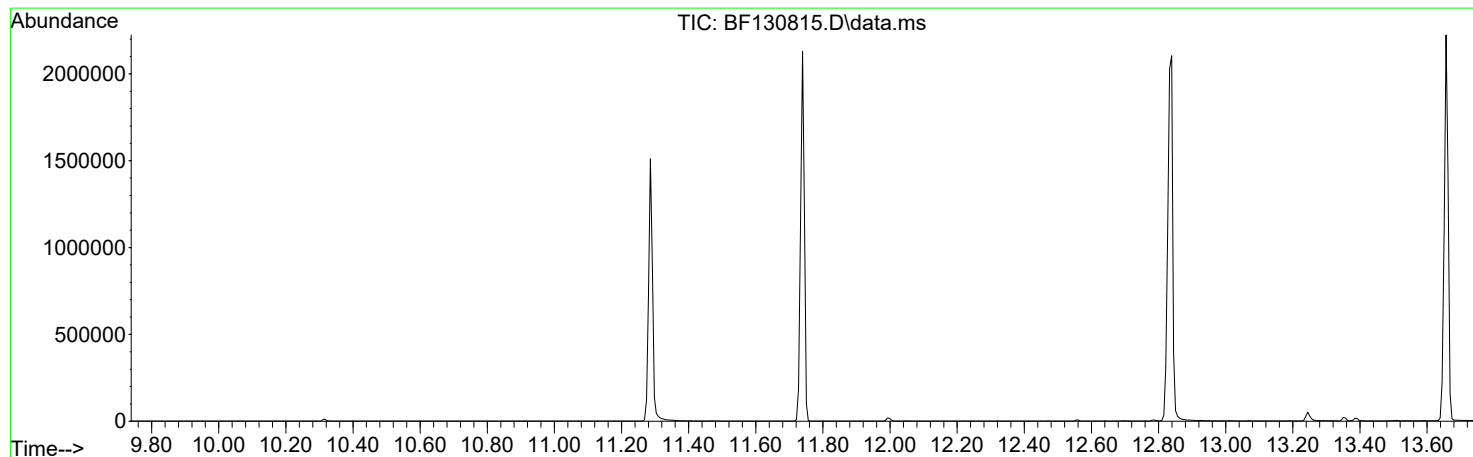

AutoFind: Scans 1640, 1641, 1642; Background Corrected with Scan 1635

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	73819	PASS
68	69	0.00	2	1.6	1037	PASS
69	198	0.00	100	39.3	63544	PASS
70	69	0.00	2	0.7	438	PASS
127	198	10	80	48.6	78579	PASS
197	198	0.00	2	0.6	1008	PASS
198	198	100	100	100.0	161627	PASS
199	198	5	9	6.7	10859	PASS
275	198	10	60	26.4	42616	PASS
365	198	1	100	3.9	6226	PASS
441	198	0.01	100	14.4	23277	PASS
442	442	50	100	100.0	149637	PASS
443	442	15	24	19.7	29476	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
10/28/2022	BNA_F	<u>BF130815.D</u>
Compound Name	Response	Retention Time
DDT	330836	13.657
DDD	6548	13.351
DDE	384	13.015
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6932	337768	2.05

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
 Data File : BF130815.D
 Acq On : 28 Oct 2022 08:41
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 29 08:13:03 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Oct 29 05:41:34 2022
 Response via : Initial Calibration

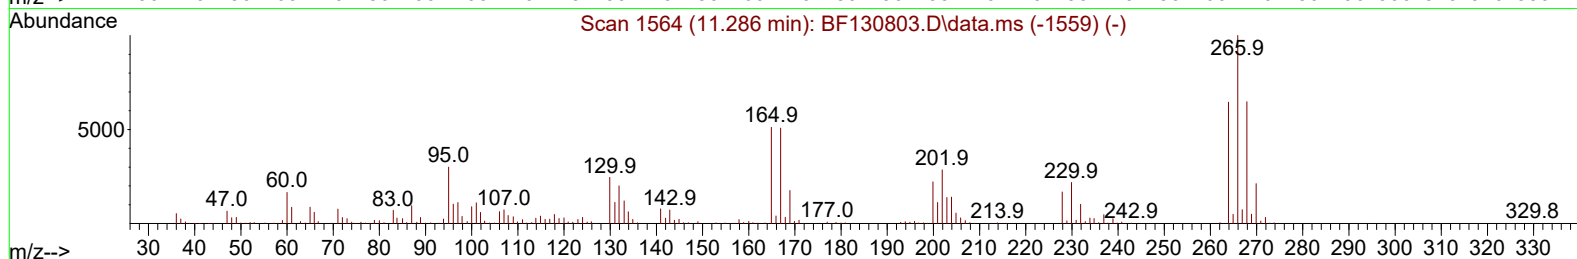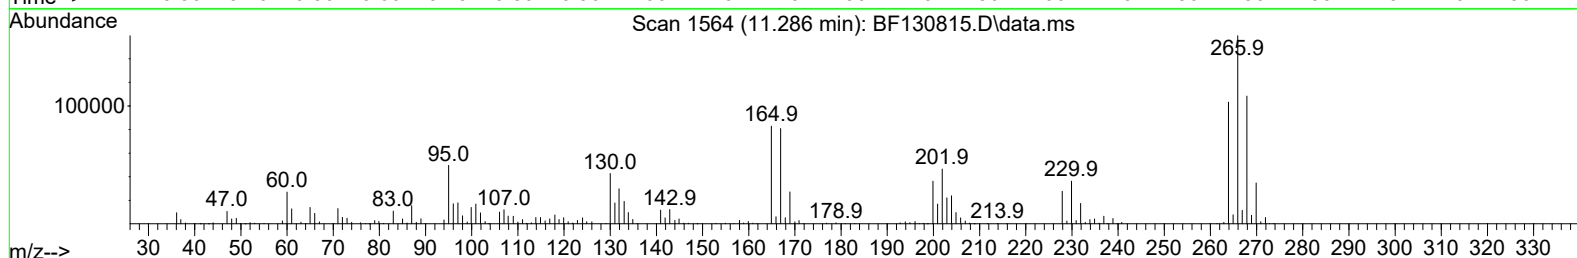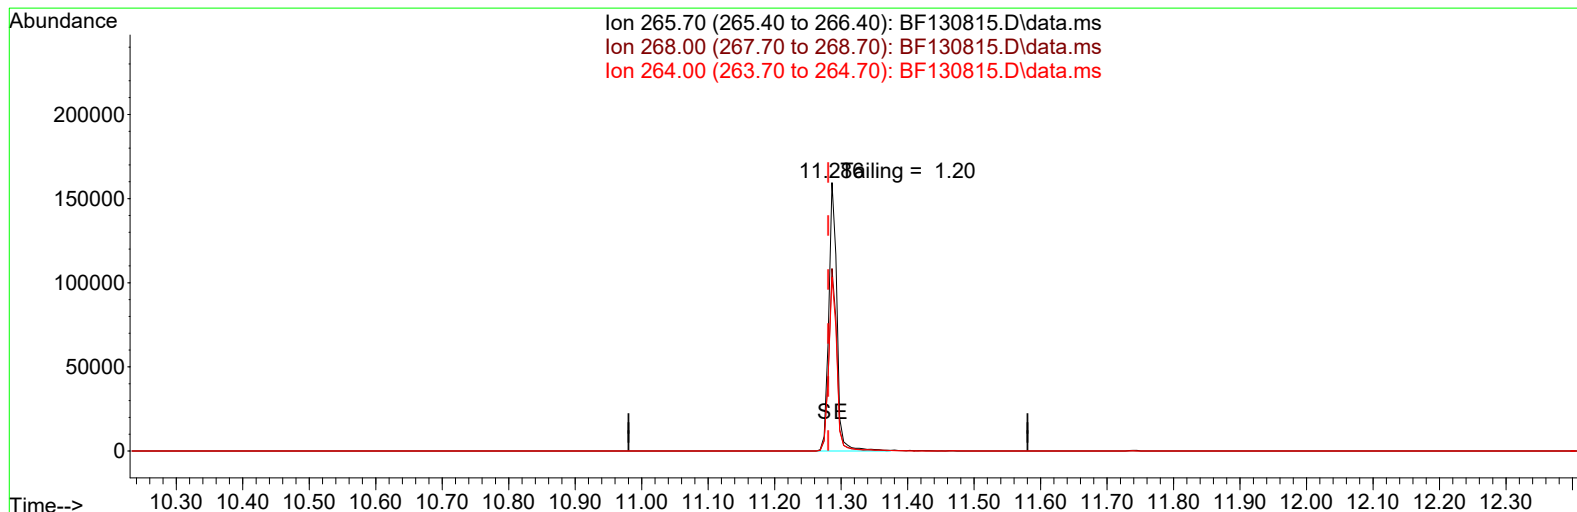

TIC: BF130815.D\data.ms

(70) Pentachlorophenol (C)

11.286min (+ 0.006) 335744.73 ng




response 137983

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	67.97
264.00	64.50	64.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
Data File : BF130815.D
Acq On : 28 Oct 2022 08:41
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 29 08:13:03 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 05:41:34 2022
Response via : Initial Calibration

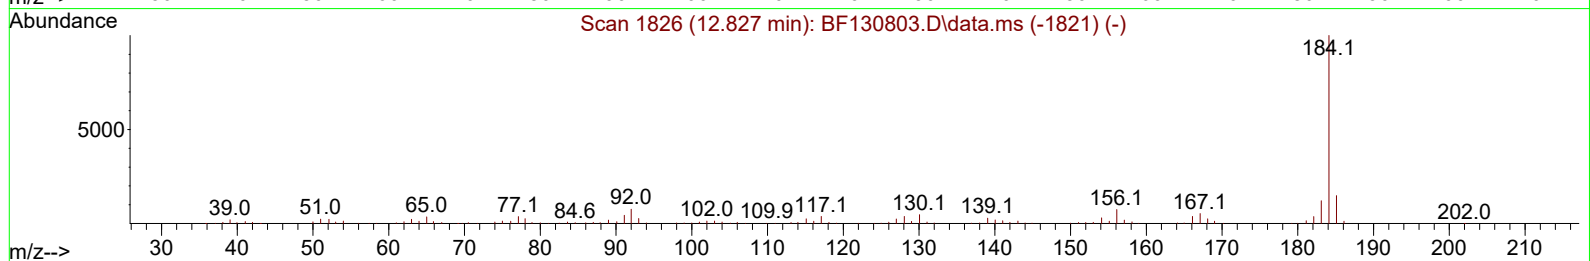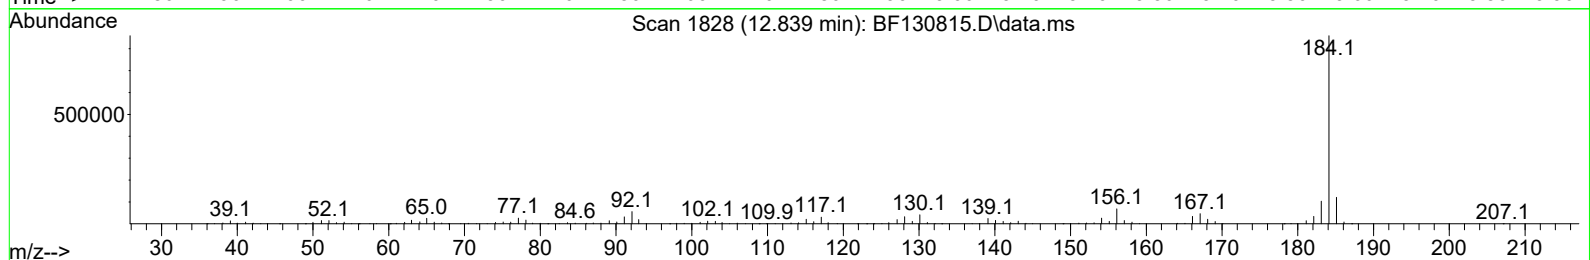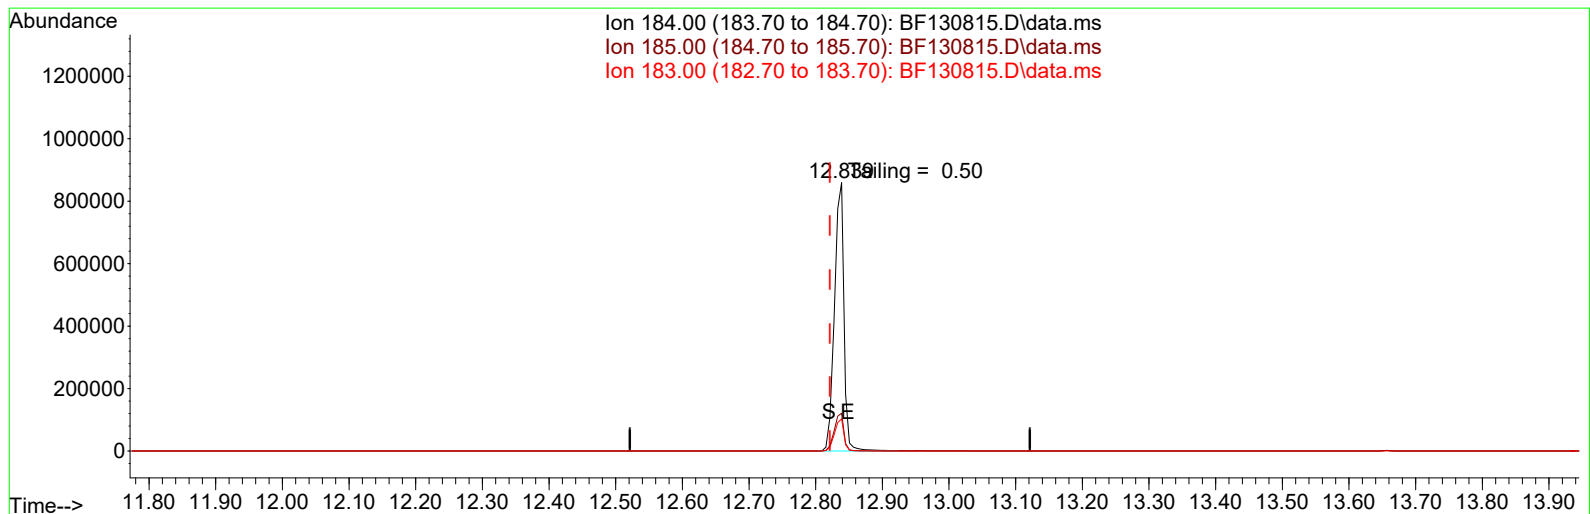

TIC: BF130815.D\data.ms

(77) Benzidine

12.839min (+ 0.017) 0.00 ng

response 856006

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.07
183.00	12.10	12.02
0.00	0.00	0.00