


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
 Data File : BF130828.D
 Acq On : 28 Oct 2022 17:49
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Oct 29 05:41:34 2022

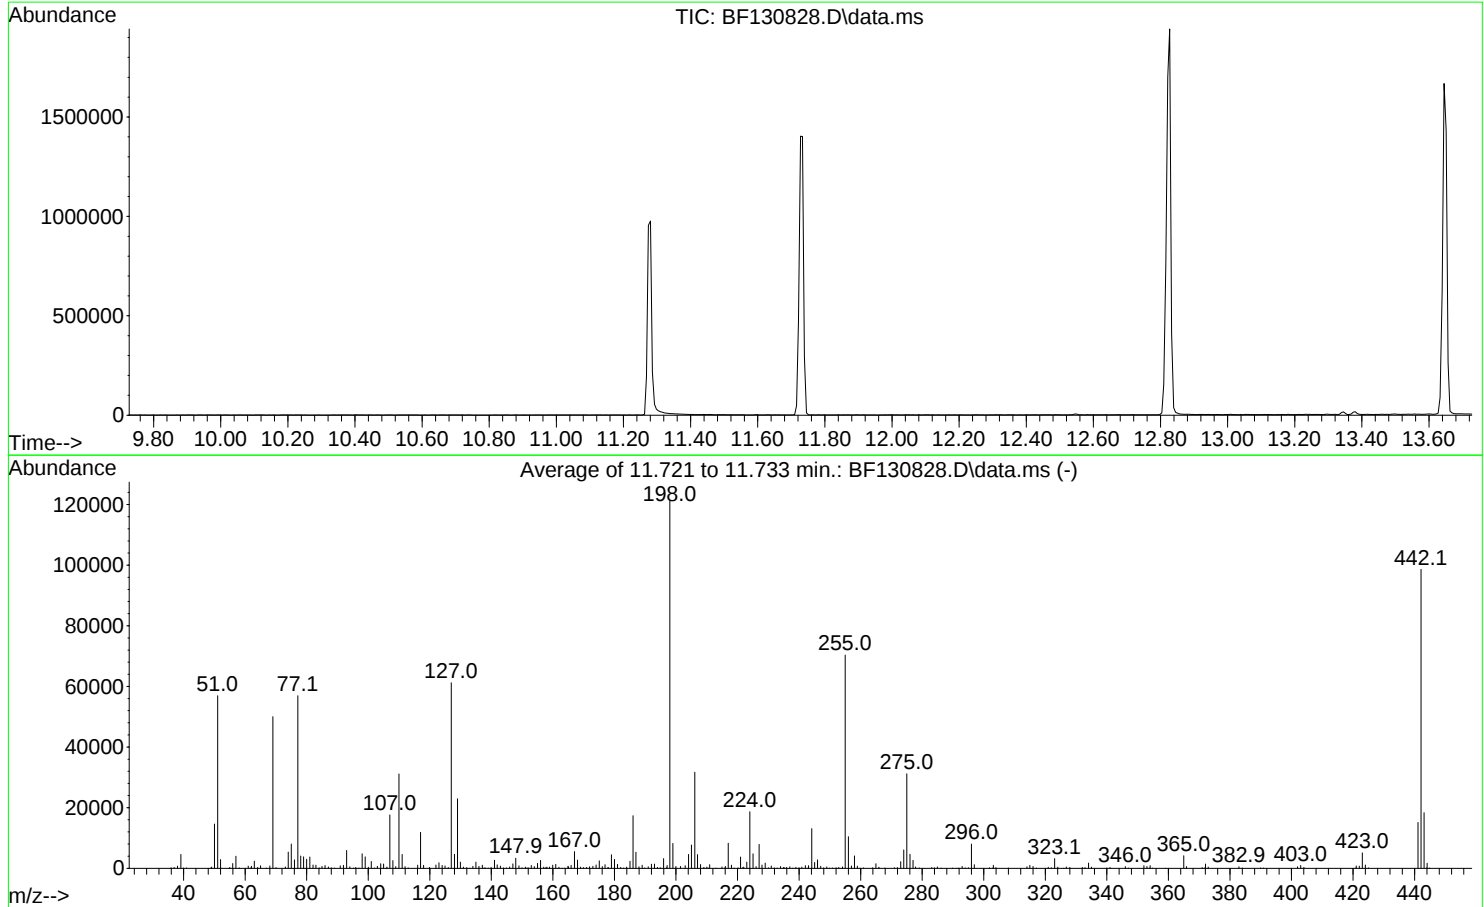




AutoFind: Scans 1638, 1639, 1640; Background Corrected with Scan 1633

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.9	56909	PASS
68	69	0.00	2	1.6	778	PASS
69	198	0.00	100	41.2	49992	PASS
70	69	0.00	2	0.5	246	PASS
127	198	10	80	50.4	61203	PASS
197	198	0.00	2	0.8	930	PASS
198	198	100	100	100.0	121363	PASS
199	198	5	9	6.8	8219	PASS
275	198	10	60	25.7	31180	PASS
365	198	1	100	3.4	4150	PASS
441	198	0.01	100	12.5	15141	PASS
442	442	50	100	100.0	98651	PASS
443	442	15	24	18.6	18338	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
Data File : BF130828.D
Acq On : 28 Oct 2022 17:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 29 08:15:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 05:41:34 2022
Response via : Initial Calibration

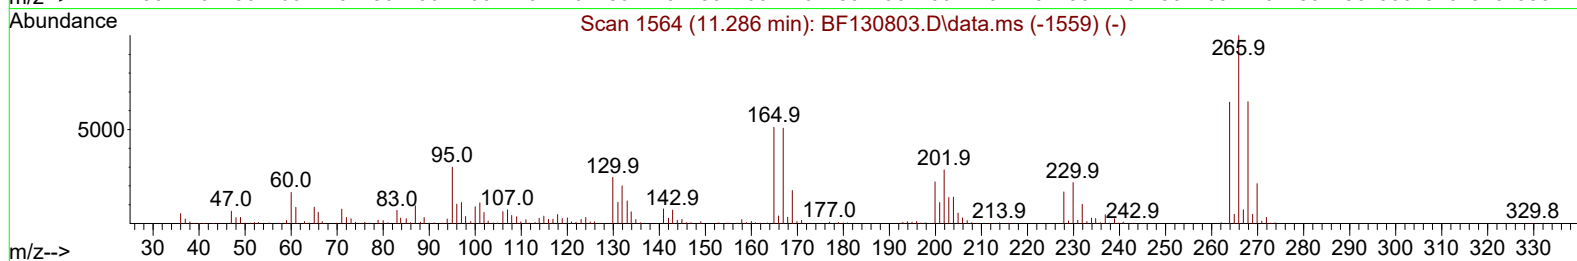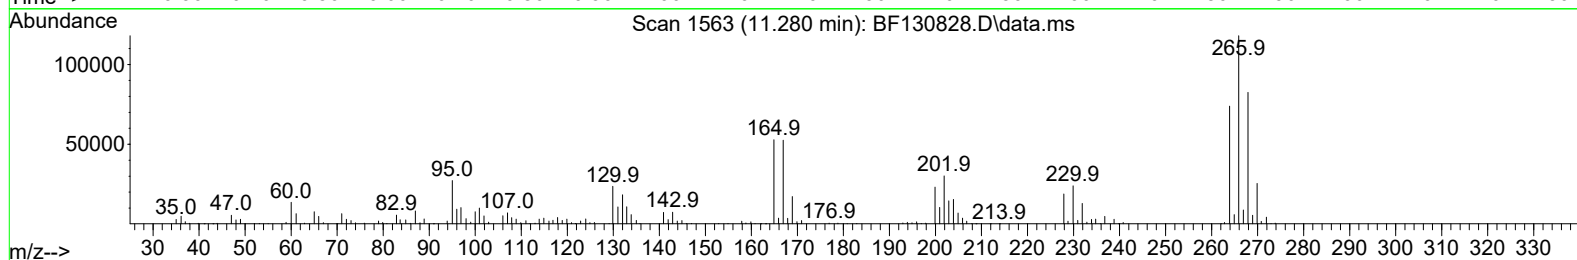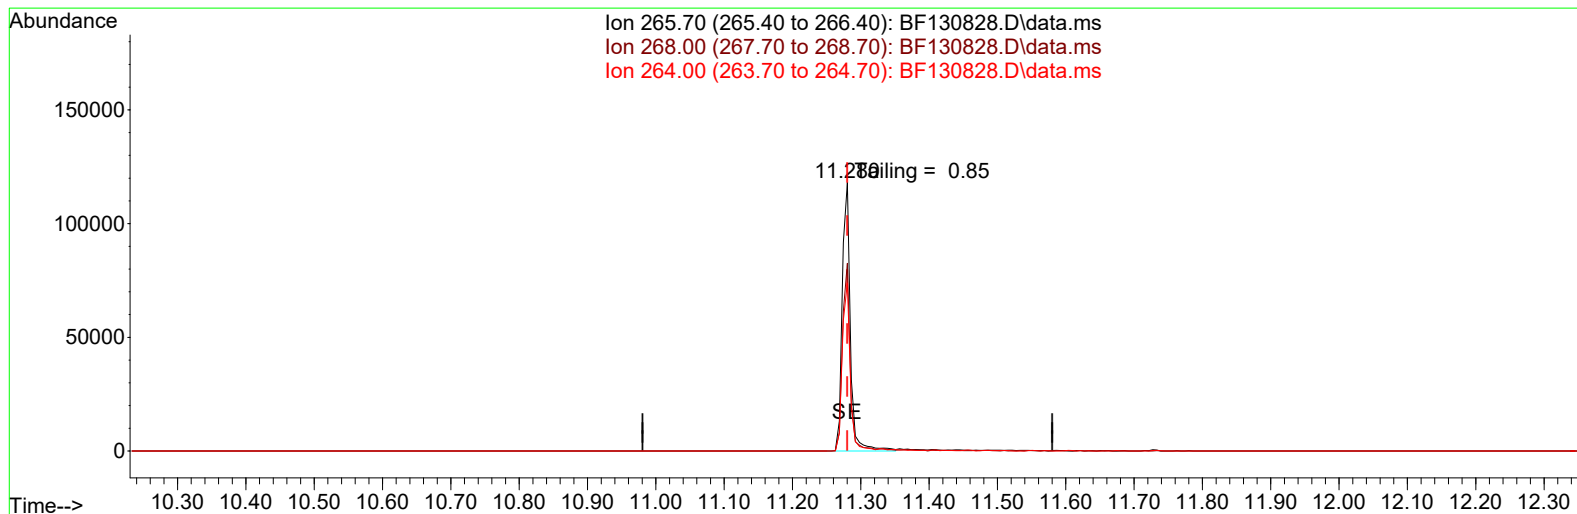

TIC: BF130828.D\data.ms

(70) Pentachlorophenol (C)

11.280min (-0.000) 28674.34 ng




response 98083

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	69.95
264.00	64.50	62.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF102822\
Data File : BF130828.D
Acq On : 28 Oct 2022 17:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 29 08:15:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Oct 29 05:41:34 2022
Response via : Initial Calibration

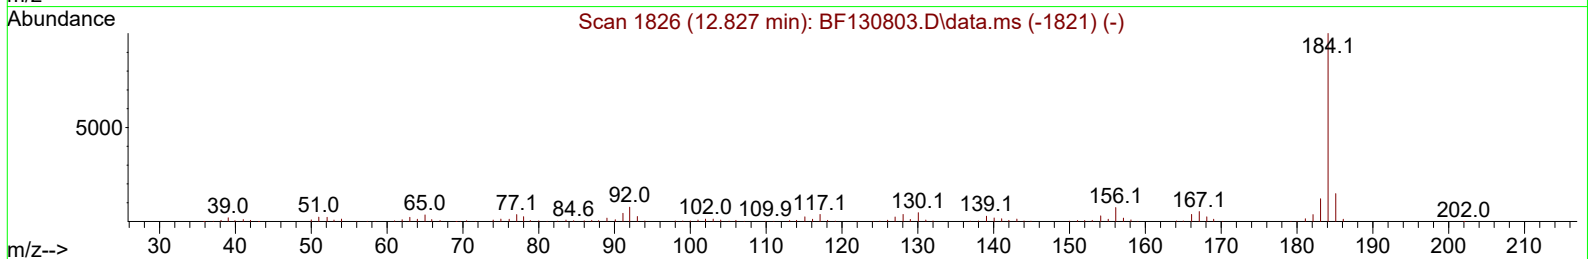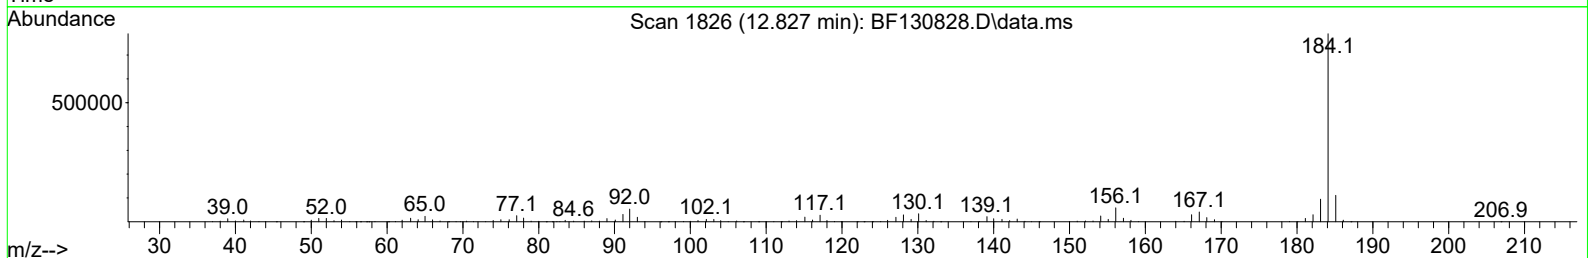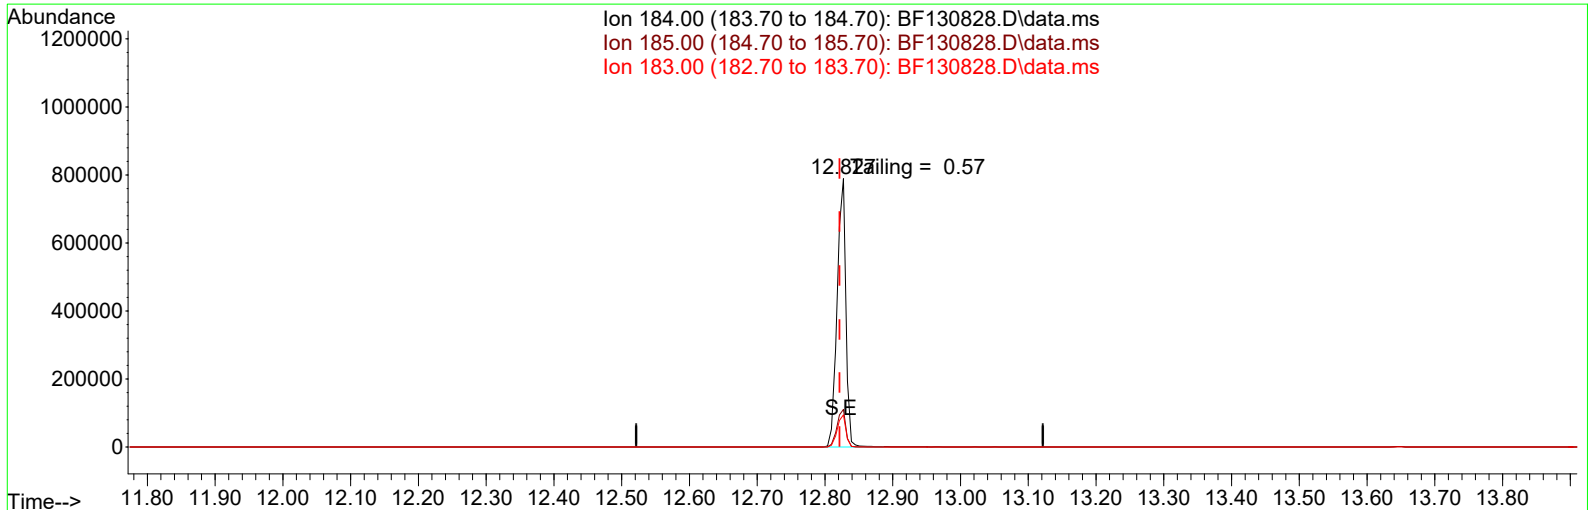

TIC: BF130828.D\data.ms

(77) Benzidine

12.827min (+ 0.006) 0.00 ng

response 710655

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	14.04
183.00	12.10	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/28/2022	BNA_F	<u>BF130828.D</u>
Compound Name	Response	Retention Time
DDT	266588	13.645
DDD	5253	13.345
DDE	233	13.01
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5486	272074	2.02

Instrument :
BNA_F
ClientSampleId :
DFTPP