


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110222\
Data File : BF130923.D
Acq On : 02 Nov 2022 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Nov 03 03:37:09 2022

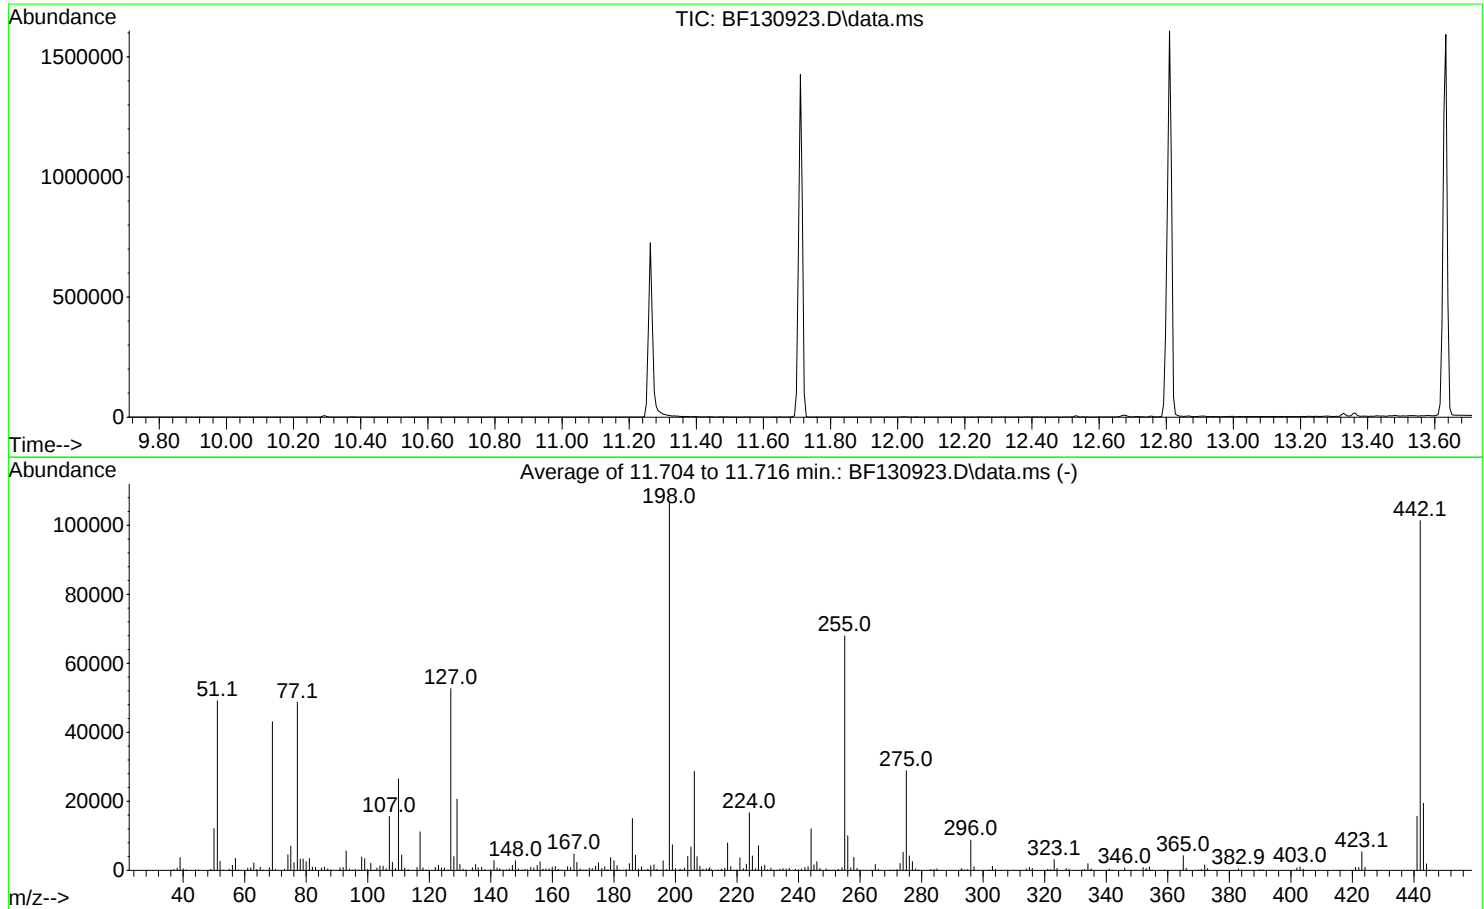




AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.1	49117	PASS
68	69	0.00	2	1.8	767	PASS
69	198	0.00	100	40.4	43056	PASS
70	69	0.00	2	0.6	257	PASS
127	198	10	80	49.4	52656	PASS
197	198	0.00	2	0.3	267	PASS
198	198	100	100	100.0	106632	PASS
199	198	5	9	6.9	7405	PASS
275	198	10	60	27.1	28853	PASS
365	198	1	100	4.0	4243	PASS
441	198	0.01	100	14.7	15637	PASS
442	442	50	100	100.0	101349	PASS
443	442	15	24	19.2	19418	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110222\
 Data File : BF130923.D
 Acq On : 02 Nov 2022 10:37
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Nov 03 09:09:00 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Nov 03 03:37:09 2022
 Response via : Initial Calibration

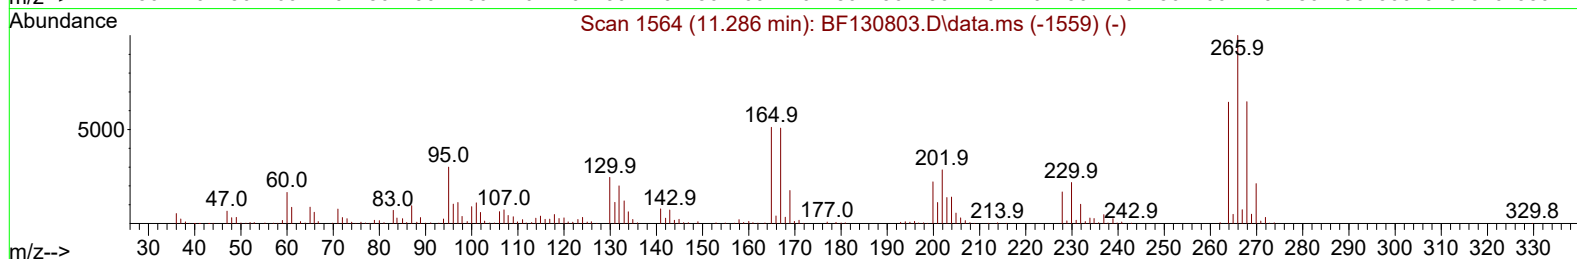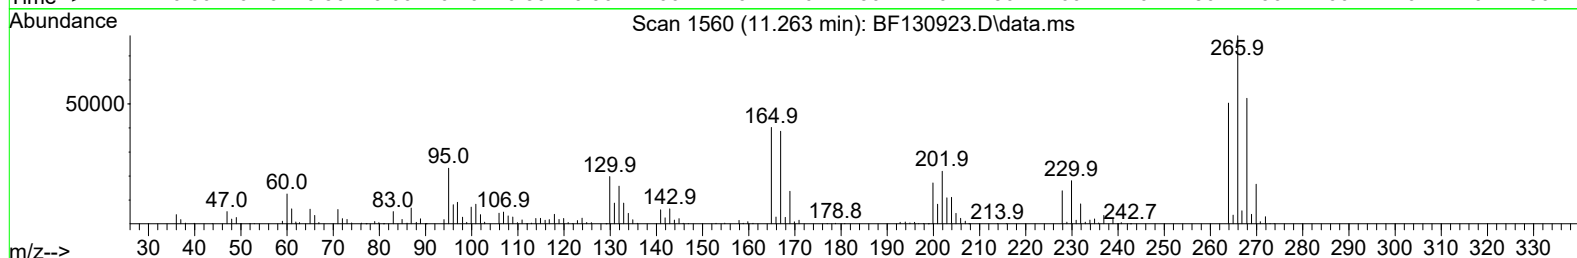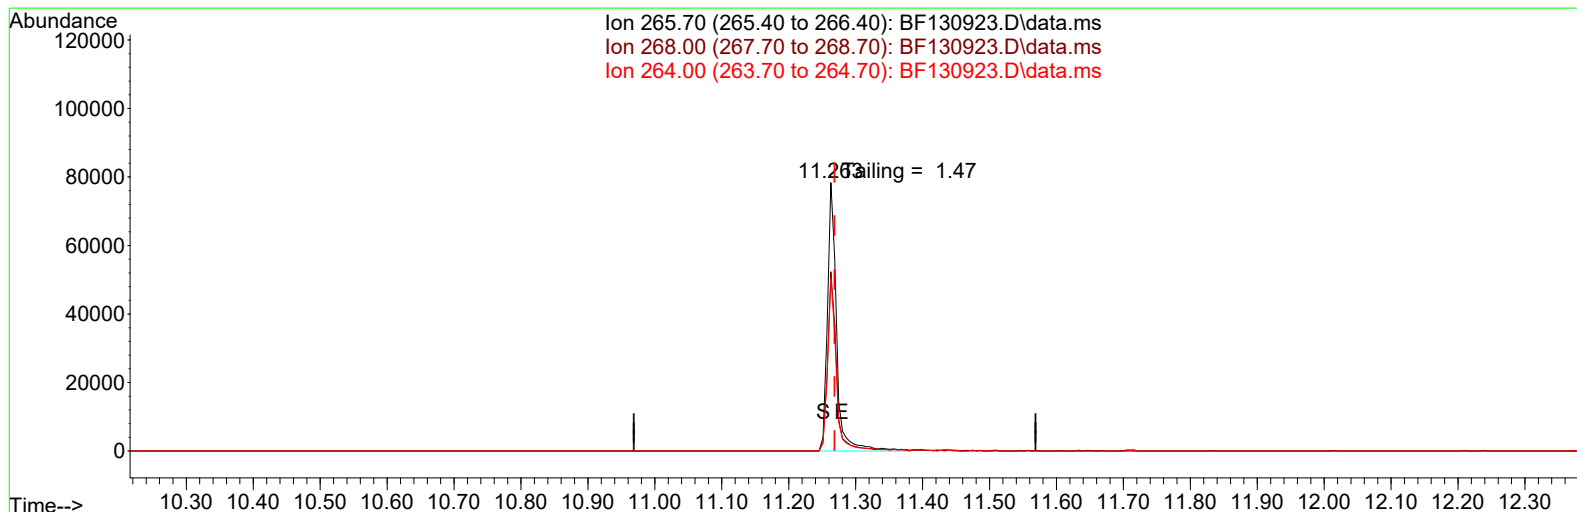

TIC: BF130923.D\data.ms

(70) Pentachlorophenol (C)

11.263min (-0.006) 29528.22 ng




response 74866

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	66.79
264.00	64.50	64.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110222\
Data File : BF130923.D
Acq On : 02 Nov 2022 10:37
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 03 09:09:00 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 03 03:37:09 2022
Response via : Initial Calibration

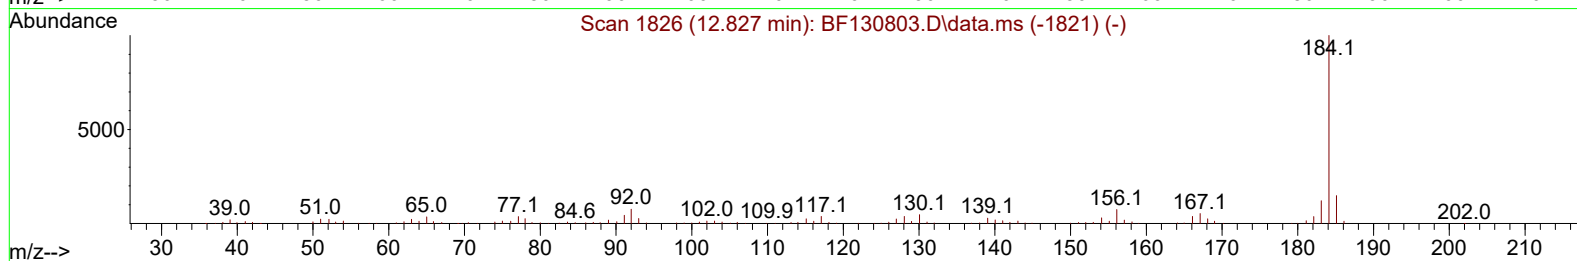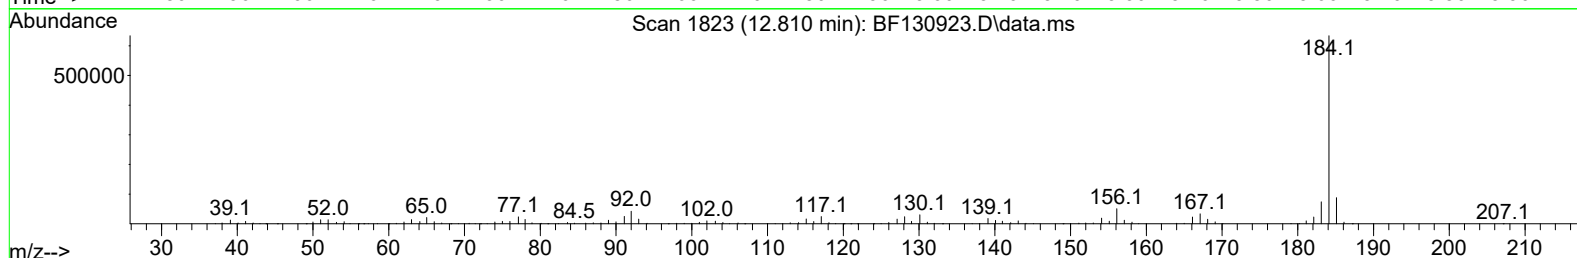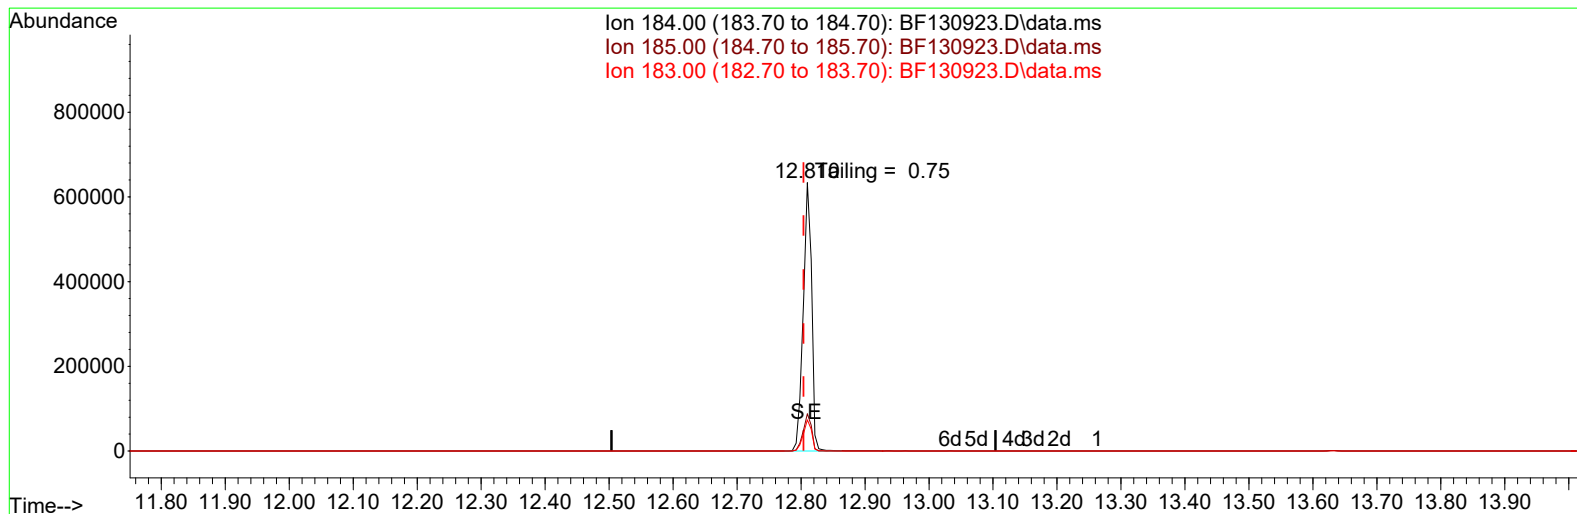

TIC: BF130923.D\data.ms

(77) Benzidine

12.810min (+ 0.006) 421068.09 ng m

response 582620

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.91
183.00	12.10	11.65
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/2/2022	BNA_F	<u>BF130923.D</u>
Compound Name	Response	Retention Time
DDT	255331	13.633
DDD	4937	13.363
DDE	381	12.986
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5318	260649	2.04

Instrument :
BNA_F
ClientSampleId :
DFTPP