


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF110222\  
Data File : BF130931.D  
Acq On : 02 Nov 2022 15:22  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF102722.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Thu Nov 03 03:37:09 2022

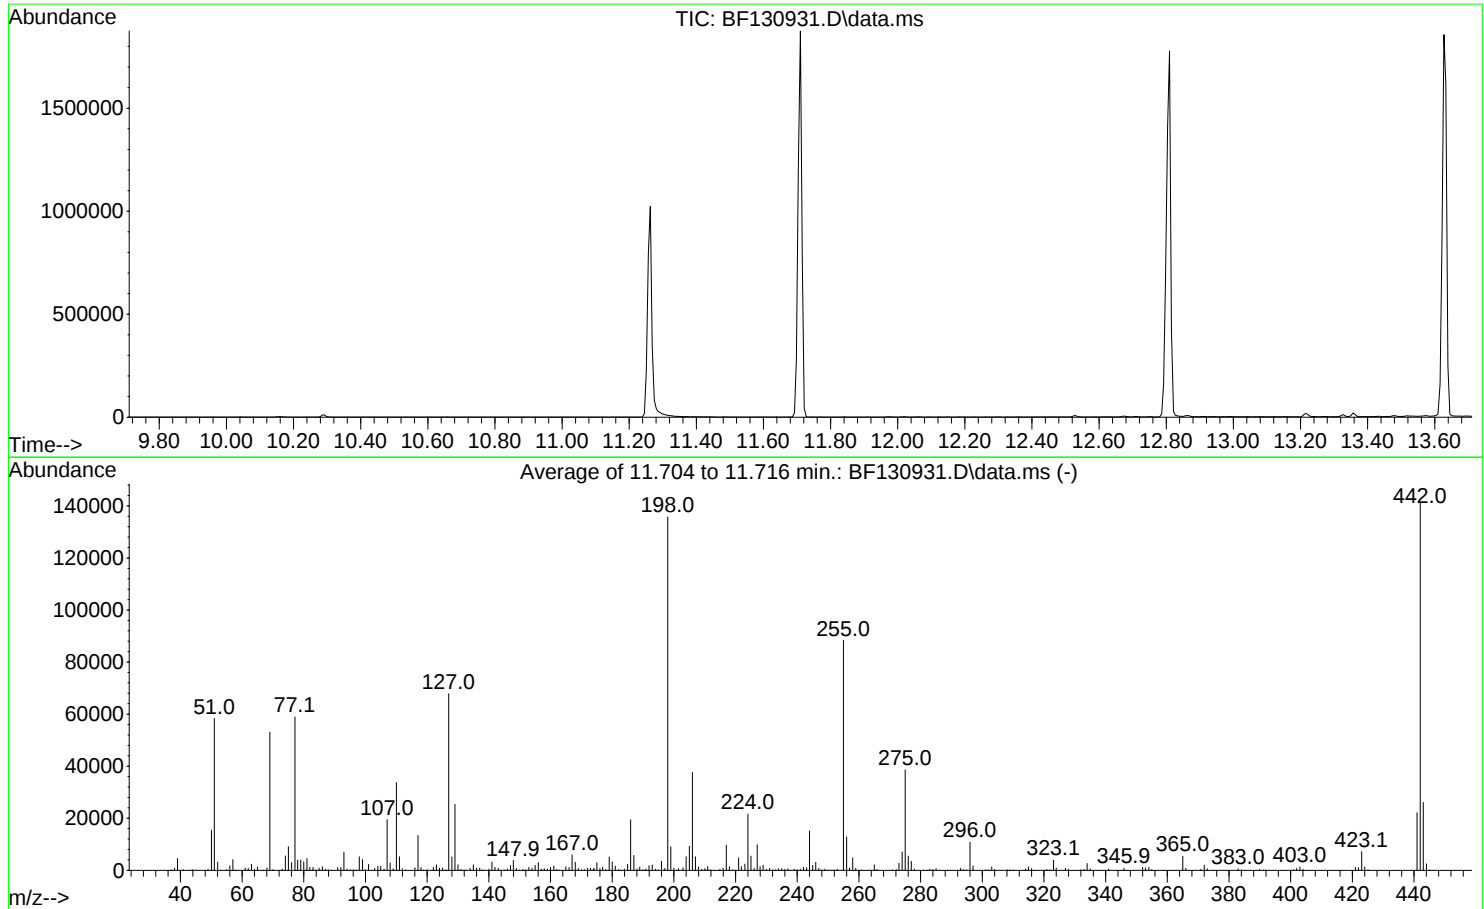


AutoFind: Scans 1635, 1636, 1637; Background Corrected with Scan 1630

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 43.0         | 58397      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 893        | PASS                |
| 69             | 198             | 0.00            | 100             | 39.1         | 53077      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.5          | 250        | PASS                |
| 127            | 198             | 10              | 80              | 50.0         | 67824      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.5          | 737        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 135741     | PASS                |
| 199            | 198             | 5               | 9               | 6.6          | 9016       | PASS                |
| 275            | 198             | 10              | 60              | 28.4         | 38600      | PASS                |
| 365            | 198             | 1               | 100             | 4.0          | 5408       | PASS                |
| 441            | 198             | 0.01            | 100             | 16.3         | 22098      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 141339     | PASS                |
| 443            | 442             | 15              | 24              | 18.5         | 26115      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF110222\  
Data File : BF130931.D  
Acq On : 02 Nov 2022 15:22  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 03 09:11:01 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF102722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 03 03:37:09 2022  
Response via : Initial Calibration

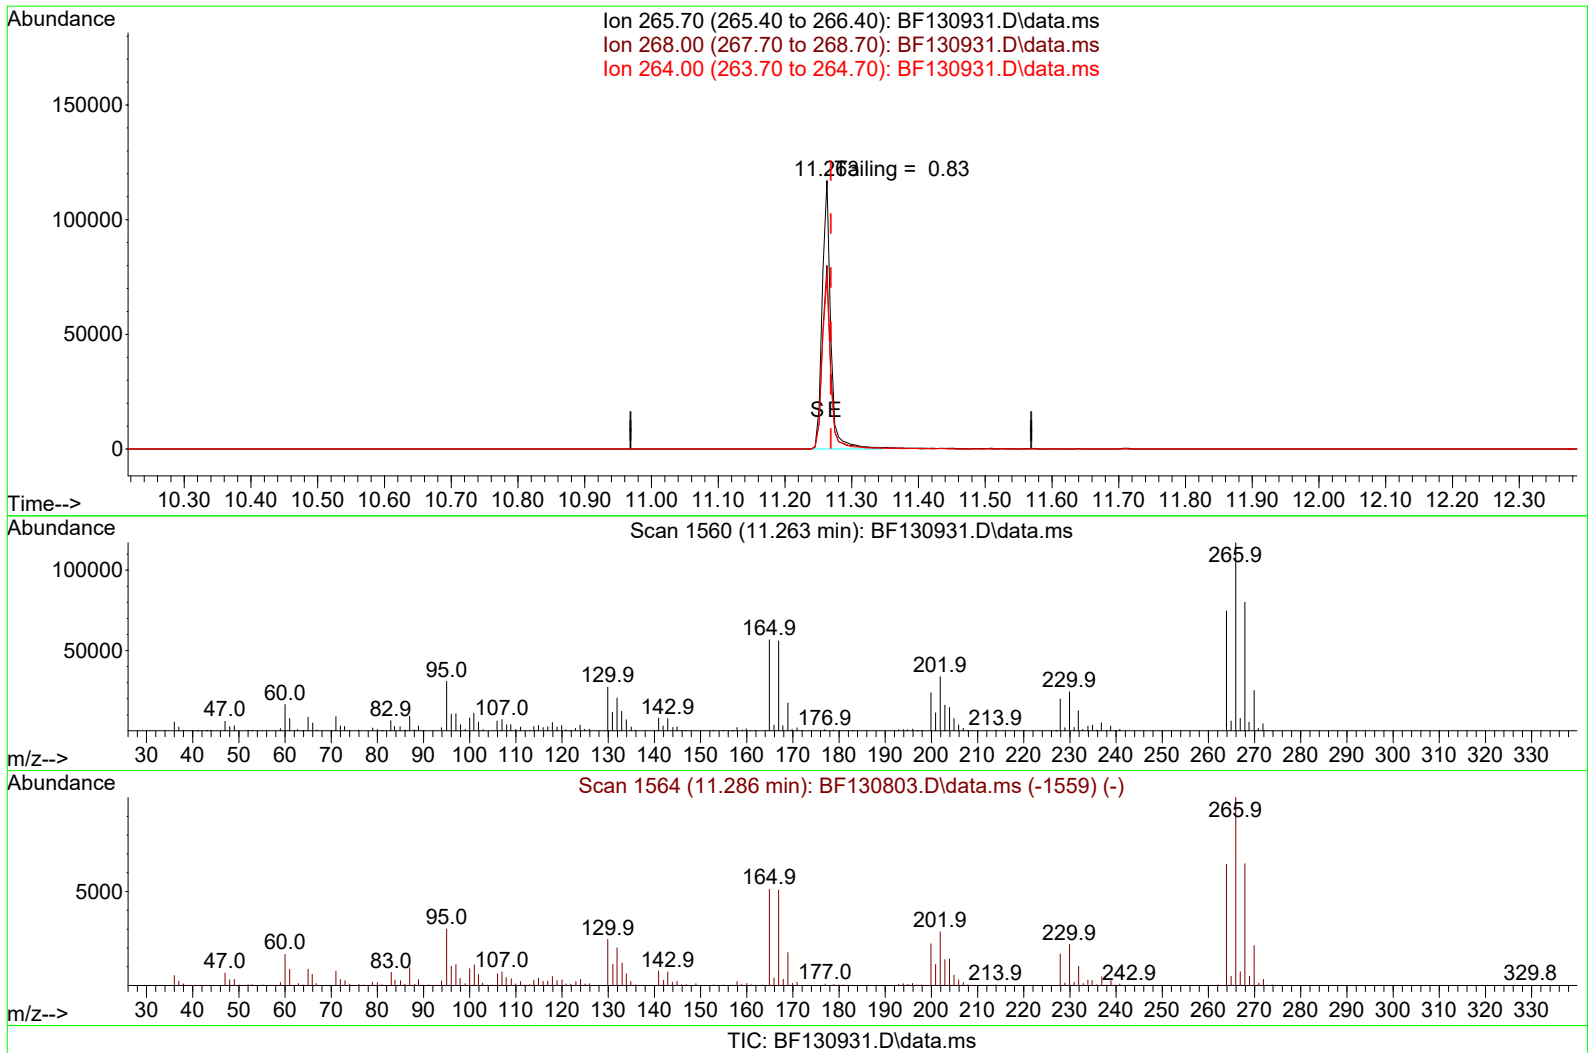

(70) Pentachlorophenol (C)

11.263min (-0.006) 29934.02 ng




response 104663

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 64.70  | 68.40  |
| 264.00 | 64.50  | 63.76  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF110222\  
Data File : BF130931.D  
Acq On : 02 Nov 2022 15:22  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Nov 03 09:11:01 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF102722.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Thu Nov 03 03:37:09 2022  
Response via : Initial Calibration

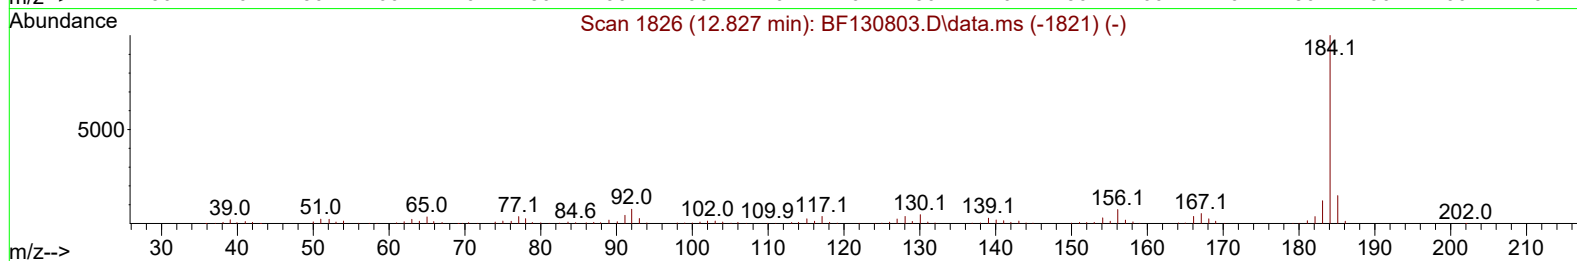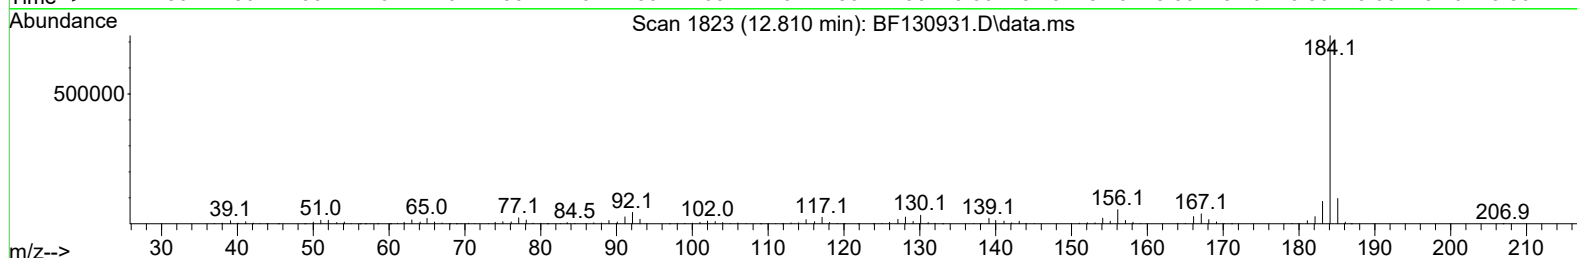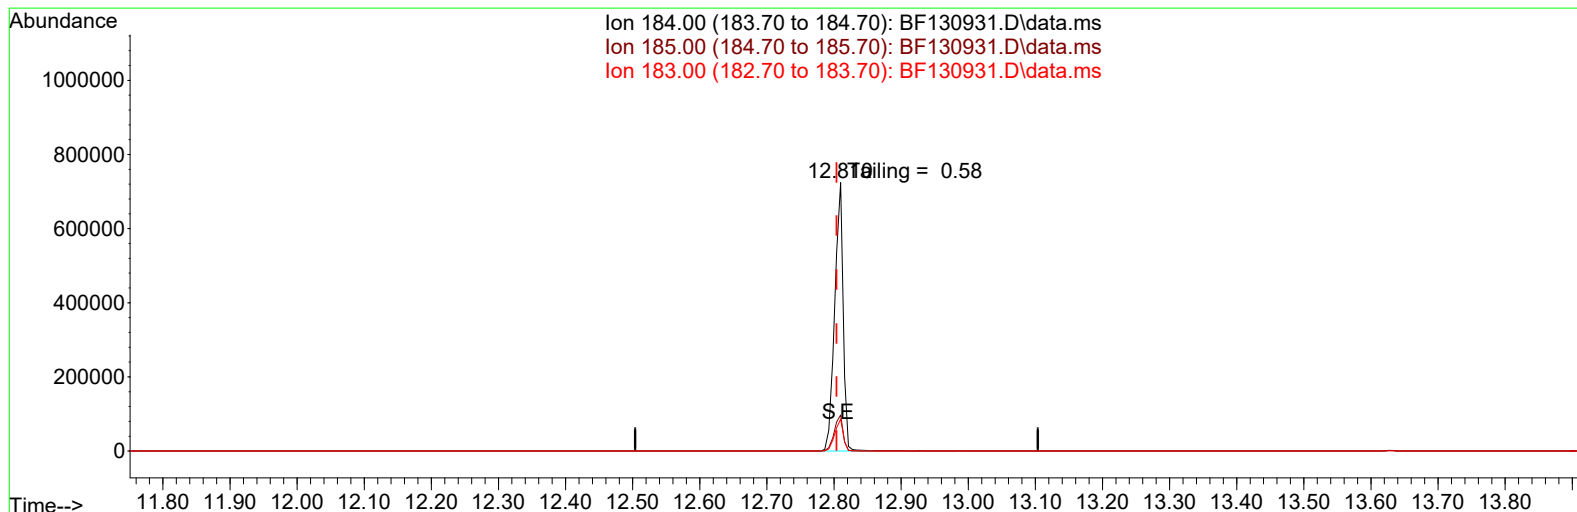

TIC: BF130931.D\data.ms

(77) Benzidine

12.810min (+ 0.006) 0.00 ng

response 635232

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.80  | 13.44  |
| 183.00 | 12.10  | 11.91  |
| 0.00   | 0.00   | 0.00   |

### DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 11/2/2022     | BNA_F            | <u>BF130931.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 321226           | 13.627             |
| DDD           | 5201             | 13.57              |
| DDE           | 305              | 12.992             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 5506          | 326732           | 1.69               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP