

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110522\
 Data File : BF131024.D
 Acq On : 05 Nov 2022 17:38
 Operator : CG\JU
 Sample : N5335-03
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 SB-3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF131024.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.199	8	19	30	rVB	470751	594736	31.07%	4.586%
2	5.122	512	516	523	rBV	300294	355630	18.58%	2.742%
3	5.522	579	584	587	rBV	1625900	1477203	77.18%	11.390%
4	6.522	749	754	758	rBV	1466307	1560468	81.53%	12.032%
5	6.904	815	819	822	rBV	530106	468982	24.50%	3.616%
6	7.463	909	914	918	rBV	1082935	1103277	57.65%	8.507%
7	8.086	1016	1020	1033	rBV	35655	72229	3.77%	0.557%
8	8.186	1033	1037	1040	rBV	753857	635084	33.18%	4.897%
9	9.263	1215	1220	1223	rBV	2296527	1913878	100.00%	14.758%
10	9.945	1332	1336	1340	rBV	851141	684092	35.74%	5.275%
11	10.739	1466	1471	1474	rBV	991530	921109	48.13%	7.102%
12	11.216	1541	1552	1560	rBV6	16265	38792	2.03%	0.299%
13	11.439	1586	1590	1593	rBV	764779	614456	32.11%	4.738%
14	13.027	1856	1860	1863	rBV	1773312	1531847	80.04%	11.812%
15	13.986	2014	2023	2033	rBV7	24881	83325	4.35%	0.643%
16	14.086	2037	2040	2043	rVV	503934	409216	21.38%	3.155%
17	14.180	2051	2056	2061	rBV	69461	68418	3.57%	0.528%
18	15.139	2213	2219	2222	rBV	16794	25077	1.31%	0.193%
19	15.586	2287	2295	2303	rBV	256339	349575	18.27%	2.696%
20	16.062	2371	2376	2384	rVB2	18313	28012	1.46%	0.216%
21	16.580	2460	2464	2471	rVB5	17312	33424	1.75%	0.258%




Sum of corrected areas: 12968830

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110522\
Data File : BF131024.D
Acq On : 05 Nov 2022 17:38
Operator : CG\JU
Sample : N5335-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

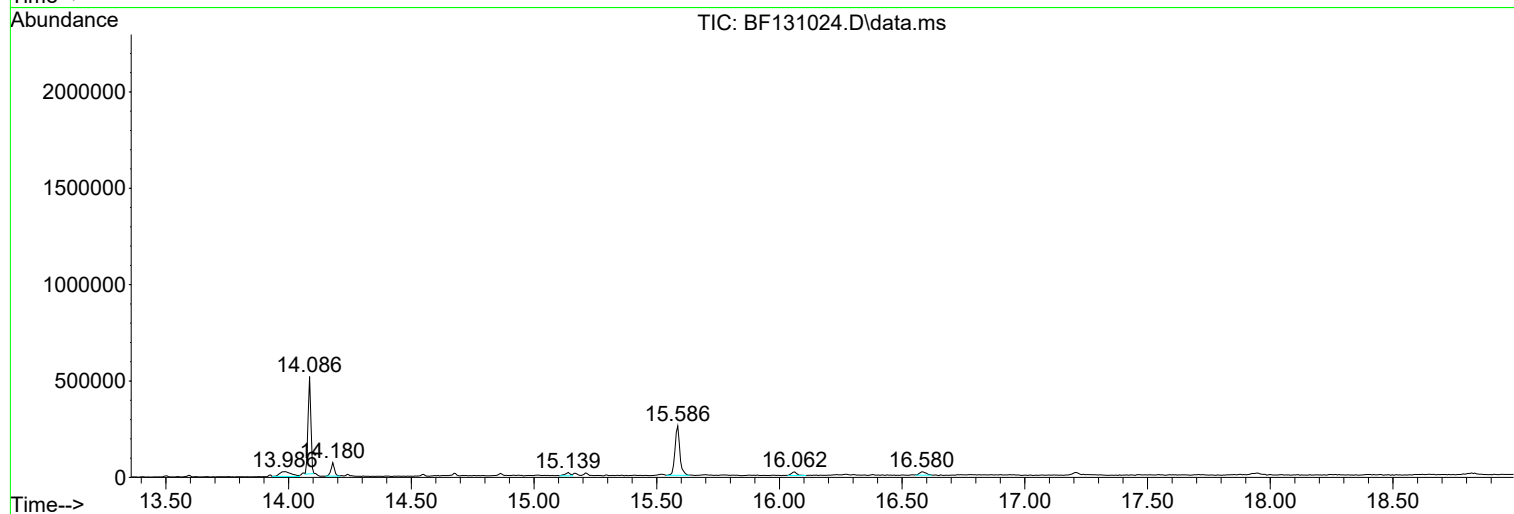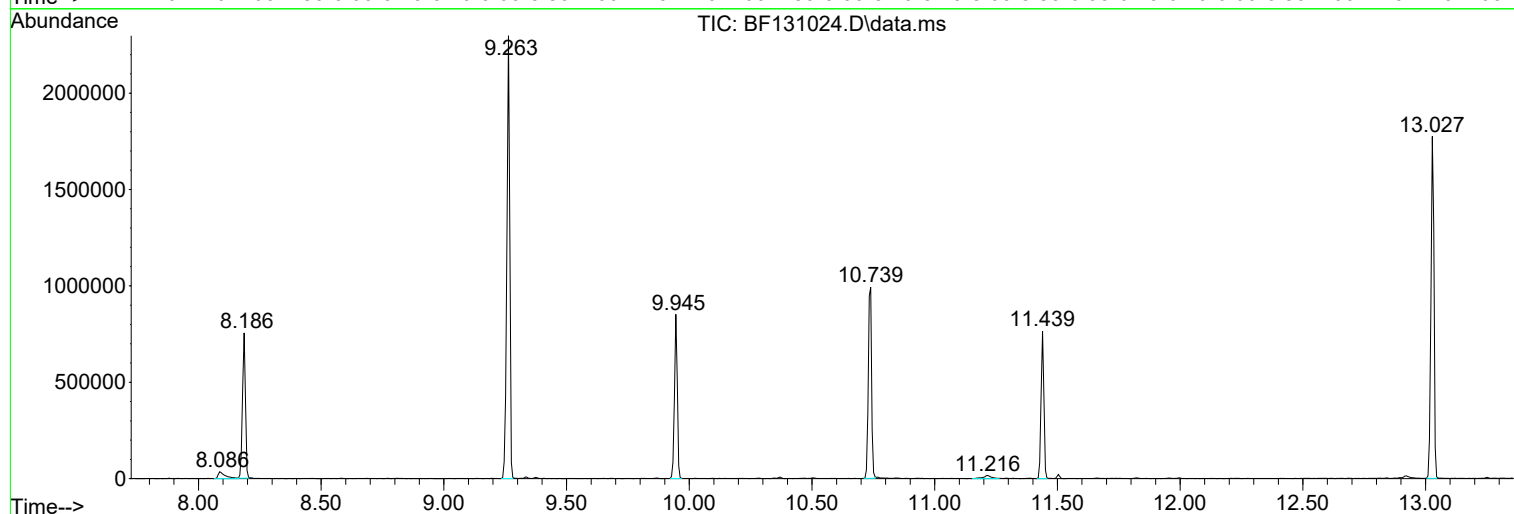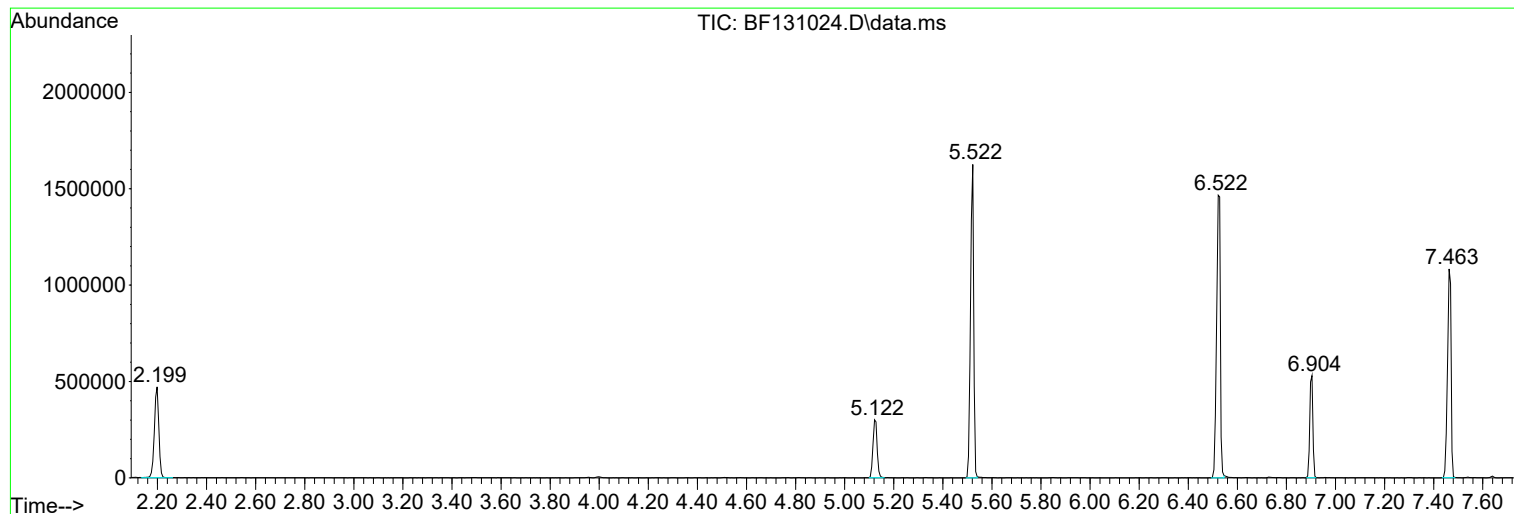

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110522\
Data File : BF131024.D
Acq On : 05 Nov 2022 17:38
Operator : CG\JU
Sample : N5335-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110522\
Data File : BF131024.D
Acq On : 05 Nov 2022 17:38
Operator : CG\JU
Sample : N5335-03
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
SB-3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc