


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110522\
Data File : BF131014.D
Acq On : 05 Nov 2022 11:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Mon Nov 07 00:46:02 2022

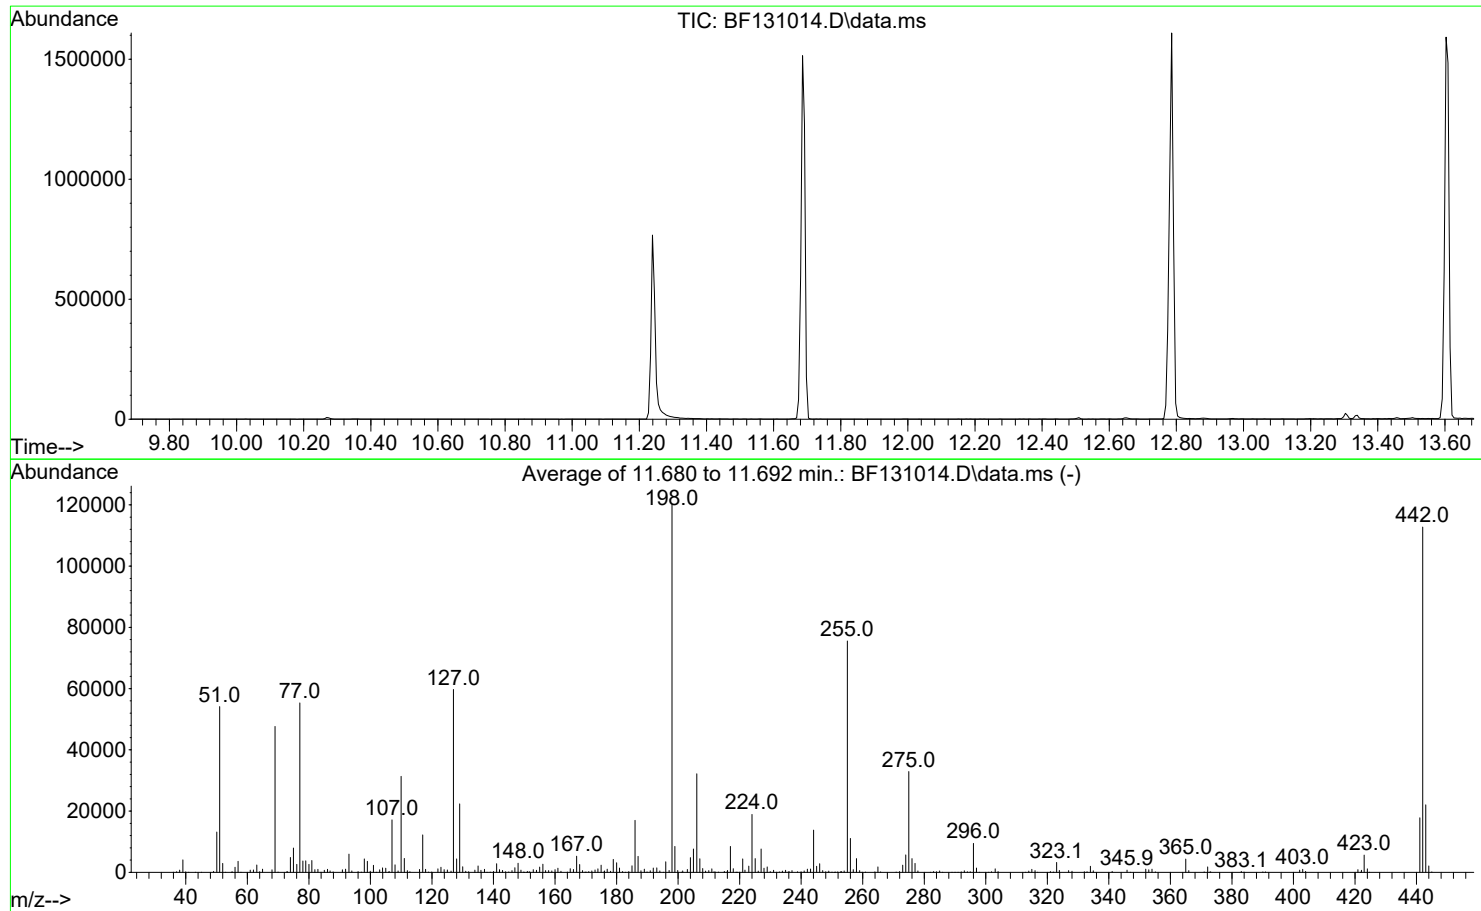




AutoFind: Scans 1631, 1632, 1633; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.1	54152	PASS
68	69	0.00	2	1.8	859	PASS
69	198	0.00	100	39.7	47659	PASS
70	69	0.00	2	0.2	108	PASS
127	198	10	80	49.7	59728	PASS
197	198	0.00	2	0.5	631	PASS
198	198	100	100	100.0	120115	PASS
199	198	5	9	7.1	8471	PASS
275	198	10	60	27.4	32901	PASS
365	198	1	100	3.6	4324	PASS
441	198	0.01	100	14.8	17816	PASS
442	442	50	100	100.0	112736	PASS
443	442	15	24	19.6	22064	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110522\
Data File : BF131014.D
Acq On : 05 Nov 2022 11:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 07 03:19:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:46:02 2022
Response via : Initial Calibration

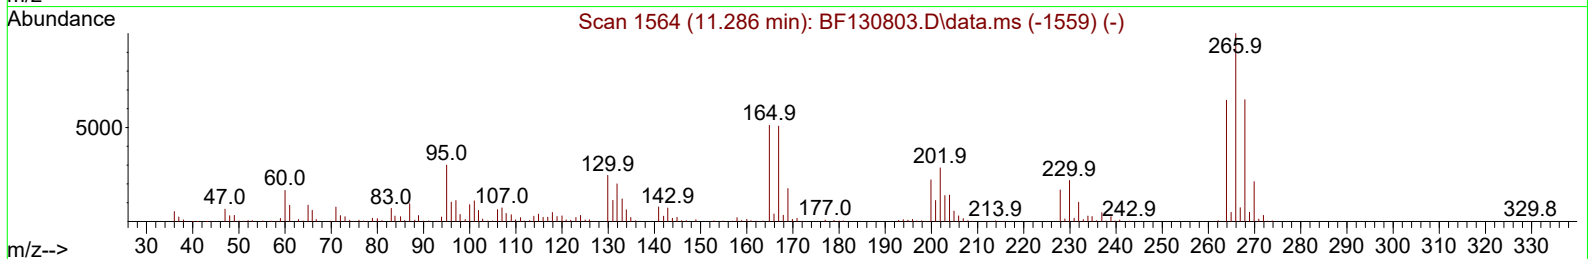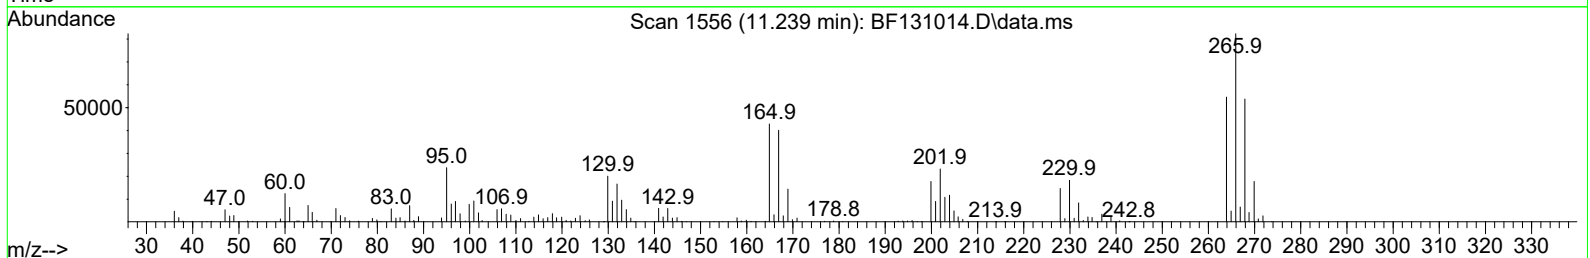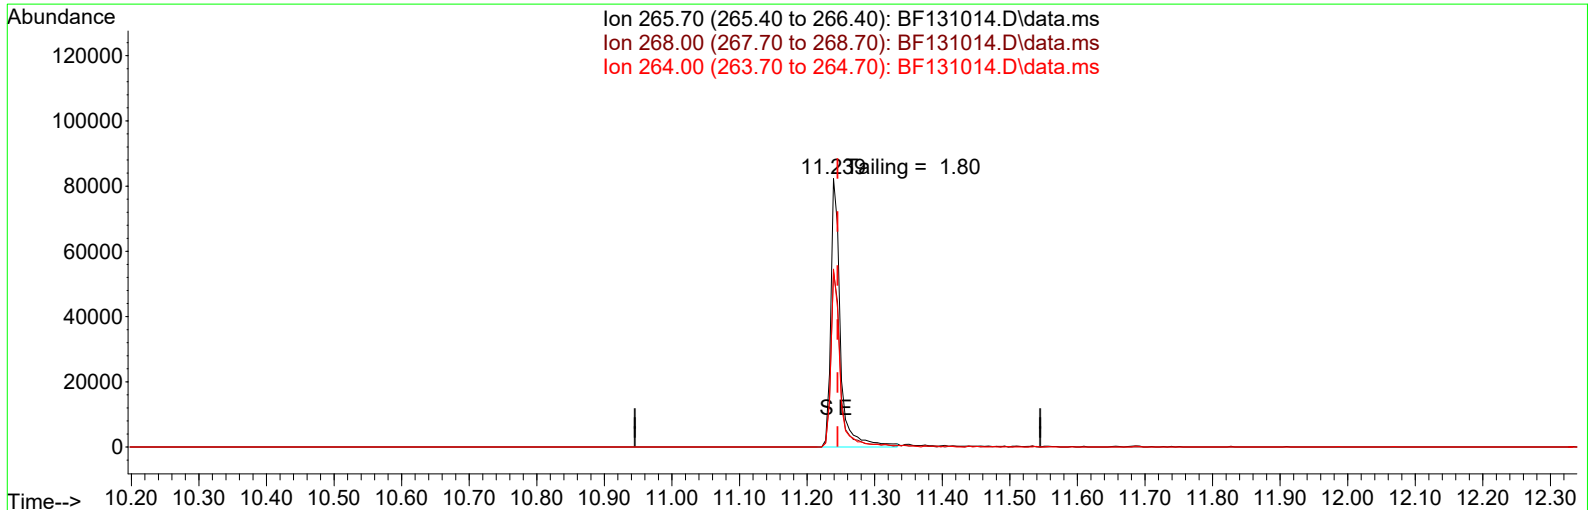

TIC: BF131014.D\data.ms

(70) Pentachlorophenol (C)

11.239min (-0.006) 22760.45 ng




response 81020

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.70	65.34
264.00	64.50	66.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF110522\
Data File : BF131014.D
Acq On : 05 Nov 2022 11:27
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 07 03:19:31 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF102722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Nov 07 00:46:02 2022
Response via : Initial Calibration

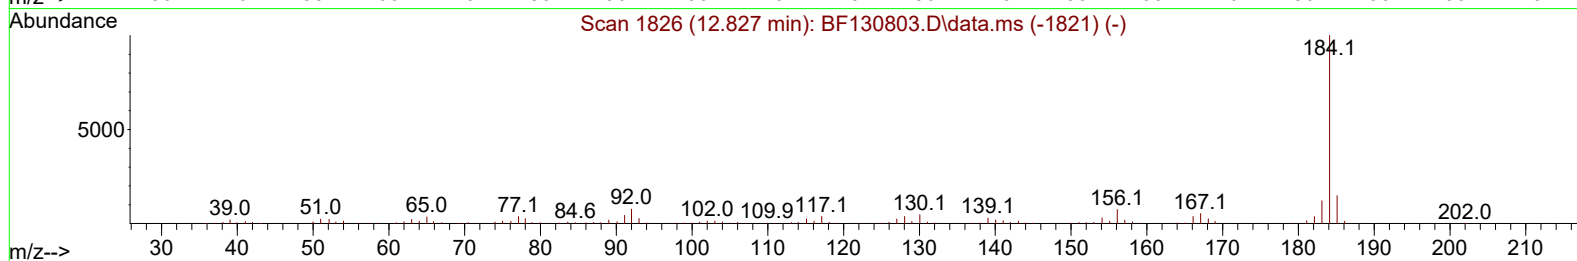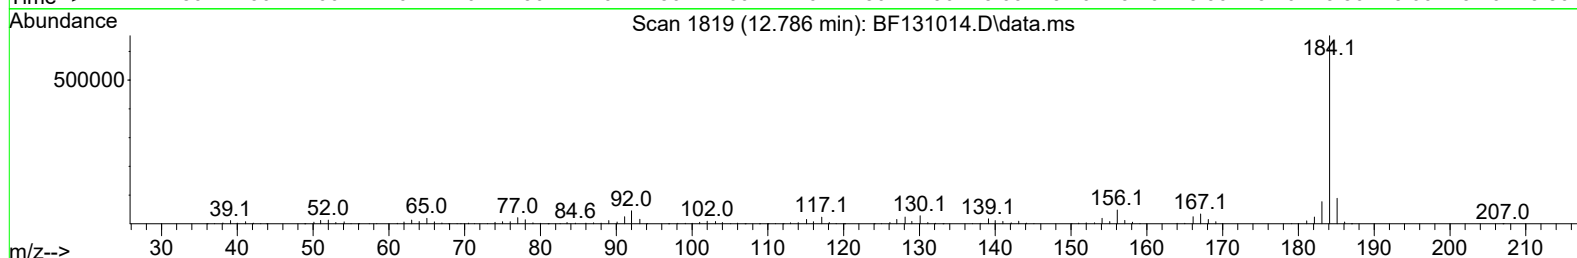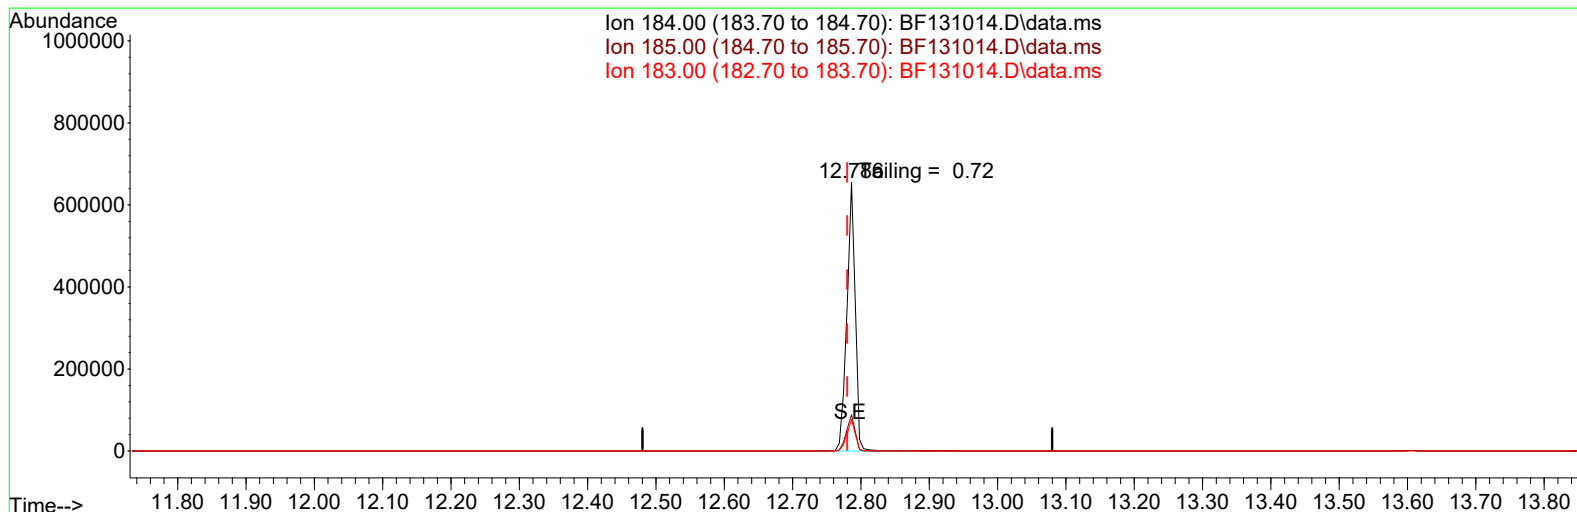

TIC: BF131014.D\data.ms

(77) Benzidine

12.786min (+ 0.006) 0.00 ng

response 556682

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.57
183.00	12.10	11.79
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/5/2022	BNA_F	BF131014.D
Compound Name	Response	Retention Time
DDT	281646	13.61
DDD	6888	13.304
DDE	544	12.968
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
7432	289078	2.57

Instrument :
BNA_F
ClientSampleId :
DFTPP