
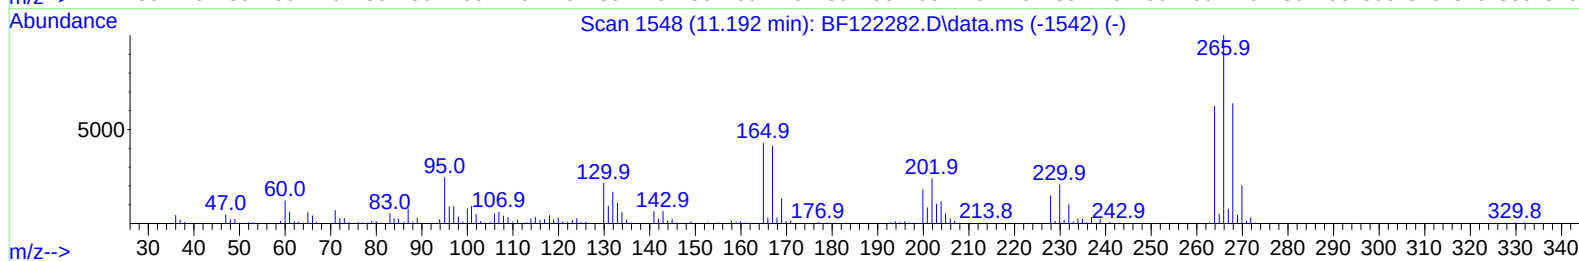
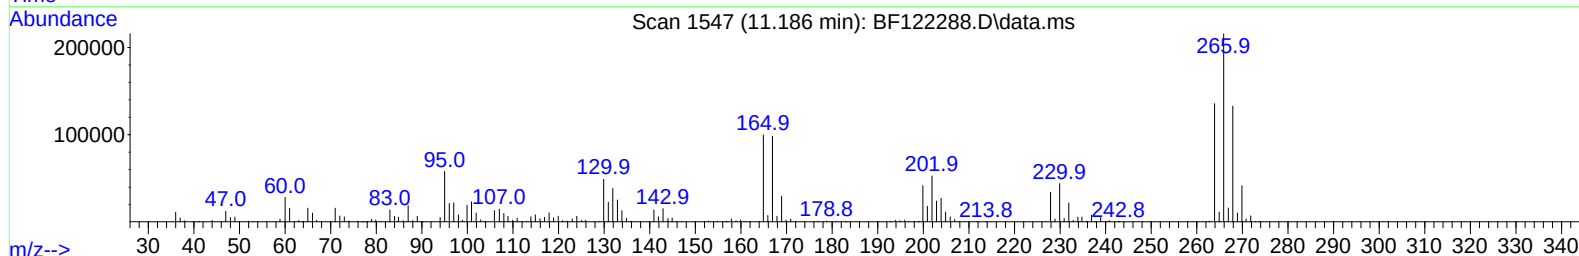


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111020\
Data File : BF122288.D
Acq On : 10 Nov 2020 9:31
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 04:10:21 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 10 12:25:42 2020
Response via : Initial Calibration

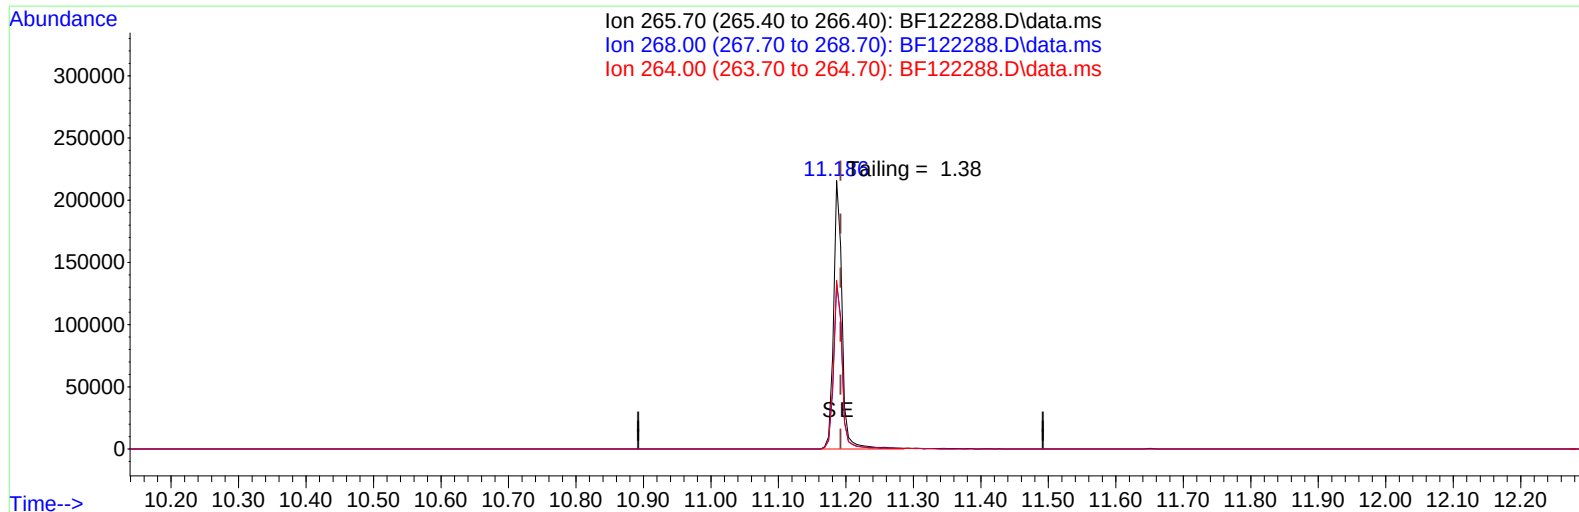

TIC: BF122288.D\data.ms

(70) Pentachlorophenol (C)




11.186min (-0.006) 241608.33 ng

response 189101

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.50	61.58
264.00	62.40	62.86
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111020\
 Data File : BF122288.D
 Acq On : 10 Nov 2020 9:31
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 11 04:10:21 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Nov 10 12:25:42 2020
 Response via : Initial Calibration

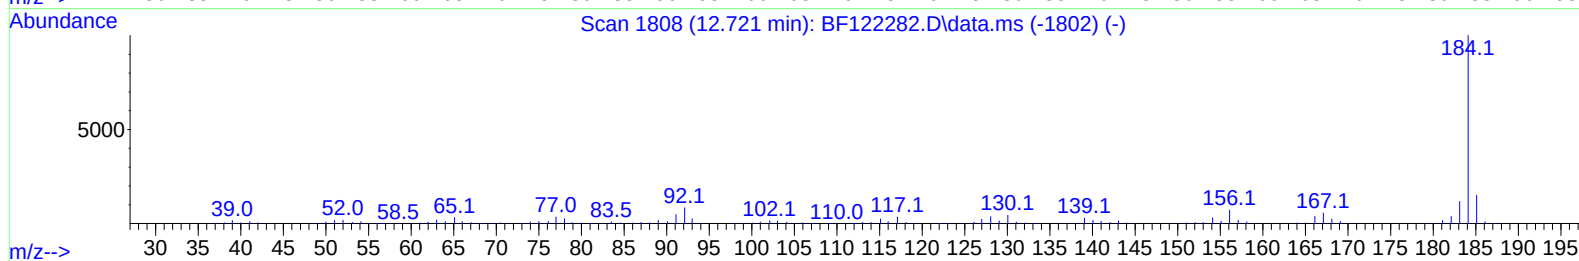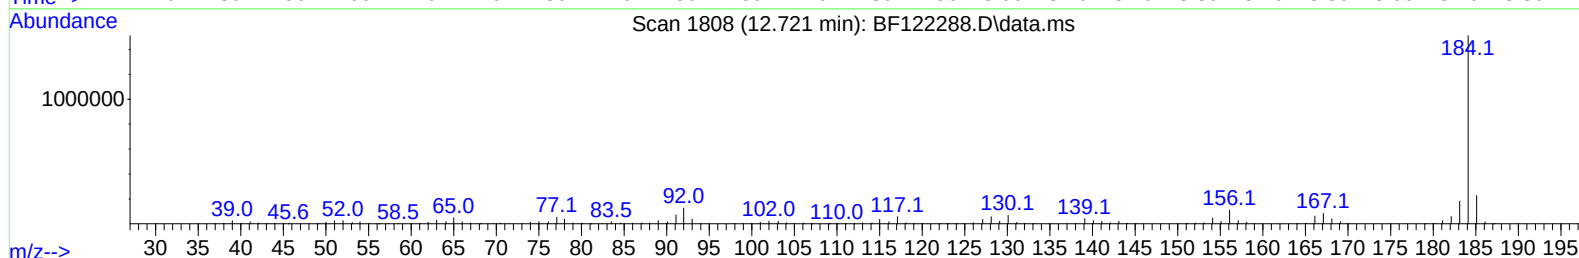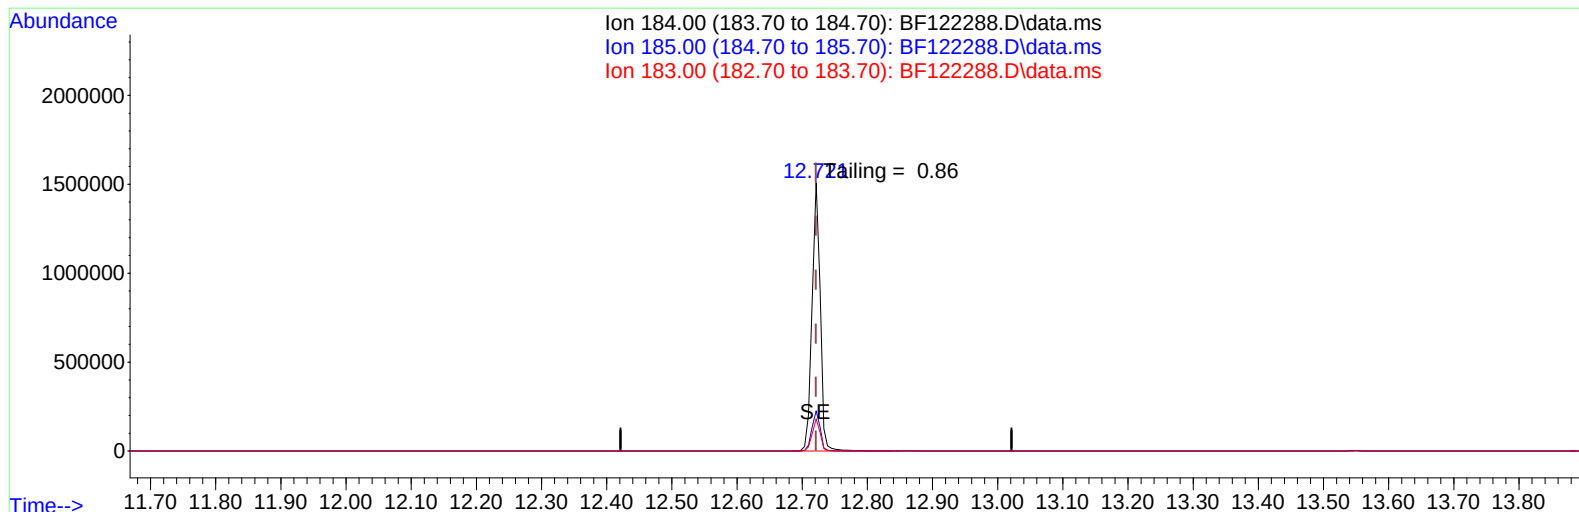

TIC: BF122288.D\data.ms

(77) Benzidine

12.721min (+ 0.000) 65656.18 ng

response 1329359

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.97
183.00	11.70	11.99
0.00	0.00	0.00