


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111020\
Data File : BF122288.D
Acq On : 10 Nov 2020 9:31
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Nov 10 12:25:42 2020

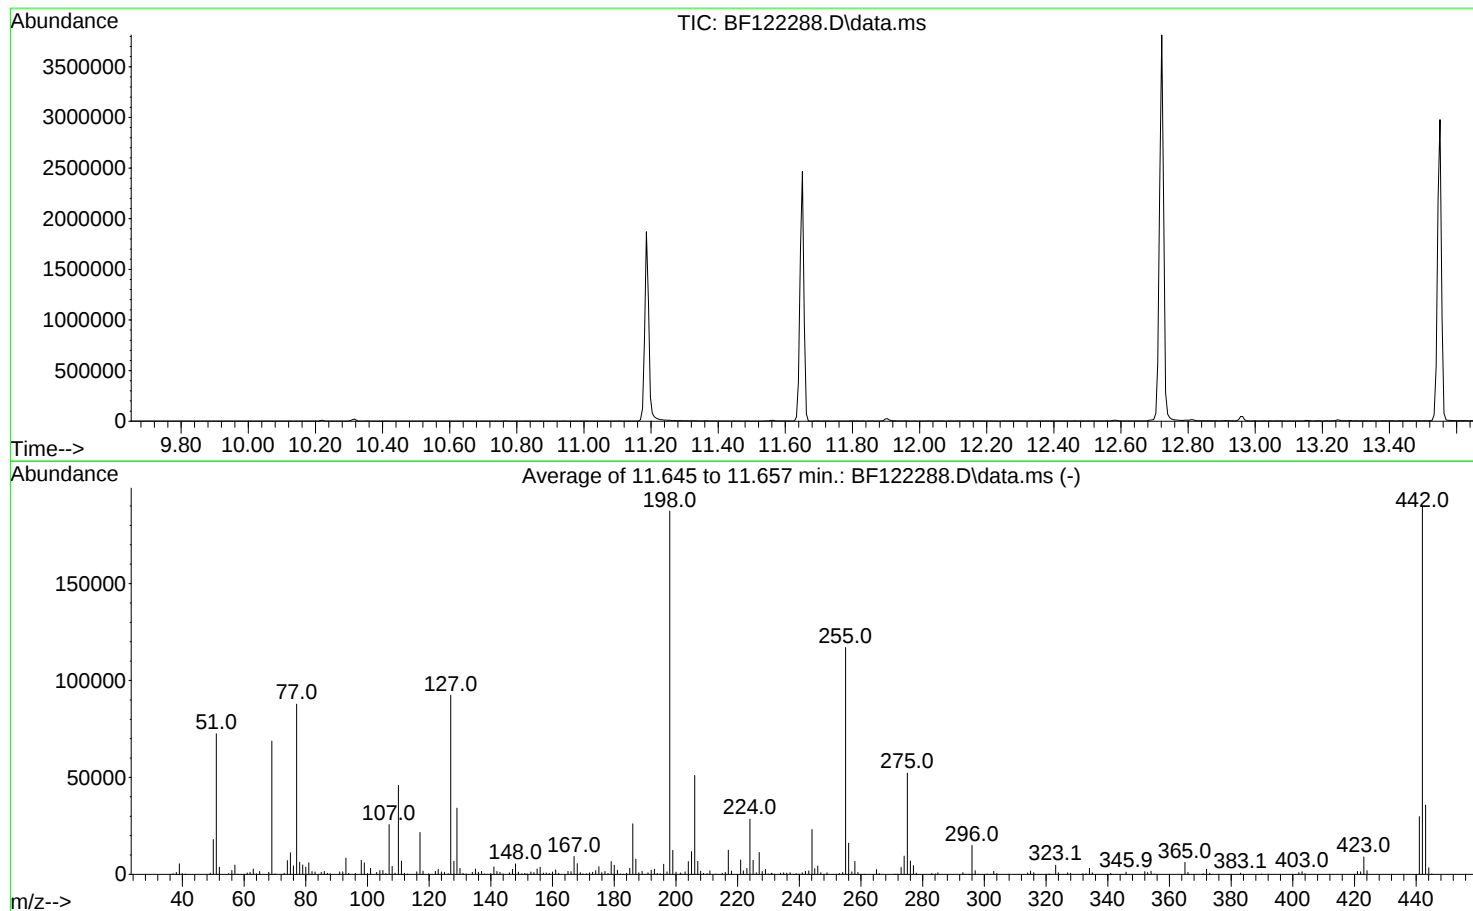

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.7	72533	PASS
68	69	0.00	2	1.5	1061	PASS
69	198	0.00	100	36.7	68771	PASS
70	69	0.00	2	0.4	250	PASS
127	198	10	80	49.3	92339	PASS
197	198	0.00	2	0.7	1364	PASS
198	198	100	100	100.0	187336	PASS
199	198	5	9	6.6	12354	PASS
275	198	10	60	27.9	52213	PASS
365	198	1	100	3.3	6157	PASS
441	198	0.01	100	15.9	29794	PASS
442	442	100	100	100.0	189755	PASS
443	442	15	24	18.8	35709	PASS