


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111324\
Data File : BF140331.D
Acq On : 13 Nov 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Nov 13 14:40:06 2024

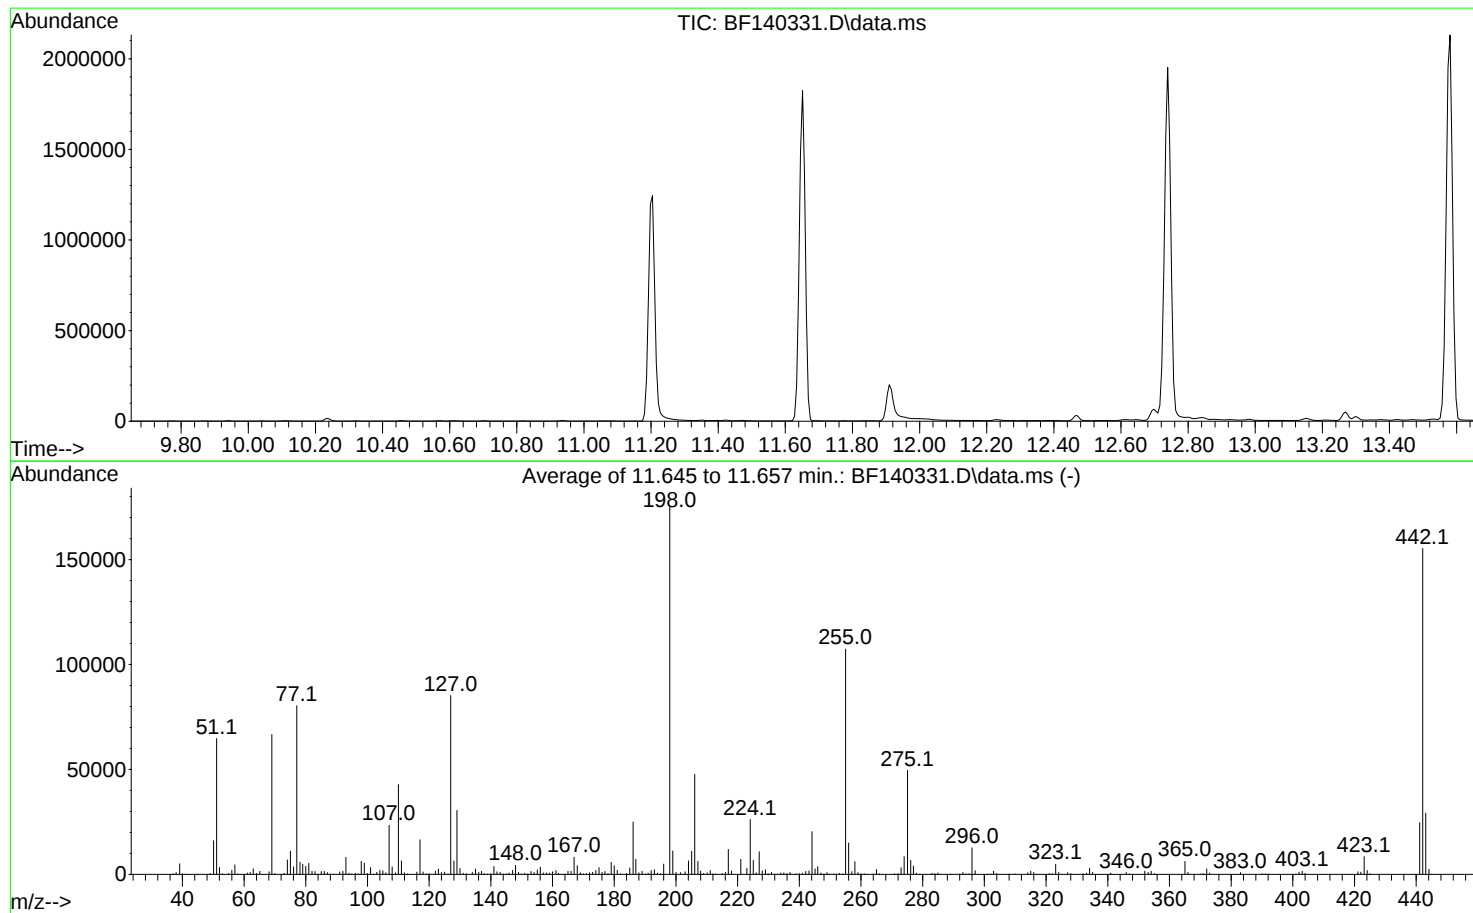




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1617

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	36.9	64757	PASS
68	69	0.00	2	1.8	1226	PASS
69	198	0.00	100	38.0	66677	PASS
70	69	0.00	2	0.6	372	PASS
127	198	10	80	48.6	85245	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	175296	PASS
199	198	5	9	6.4	11148	PASS
275	198	10	60	28.3	49536	PASS
365	198	1	100	3.5	6203	PASS
441	198	0.01	100	14.0	24595	PASS
442	442	50	100	100.0	155288	PASS
443	442	15	24	18.8	29203	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111324\
Data File : BF140331.D
Acq On : 13 Nov 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 13 14:44:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

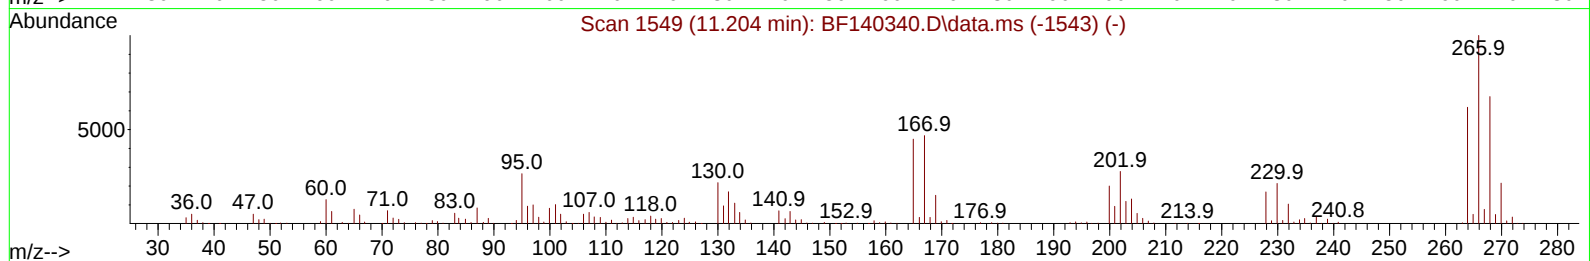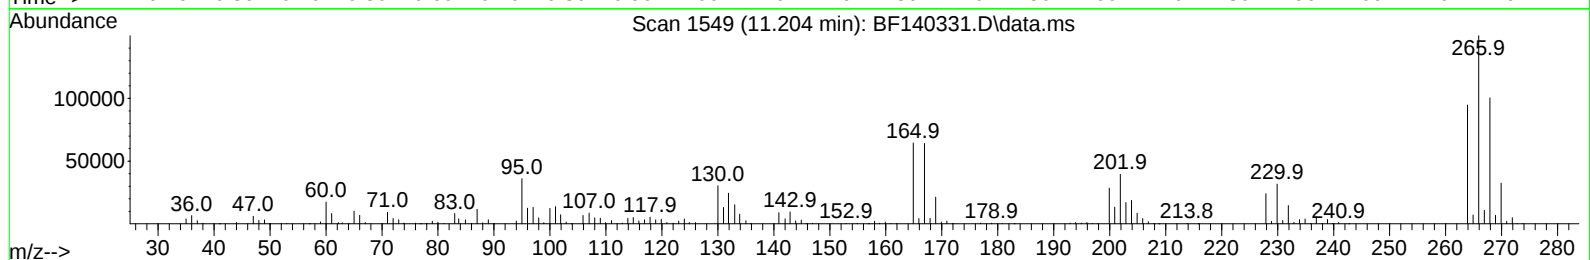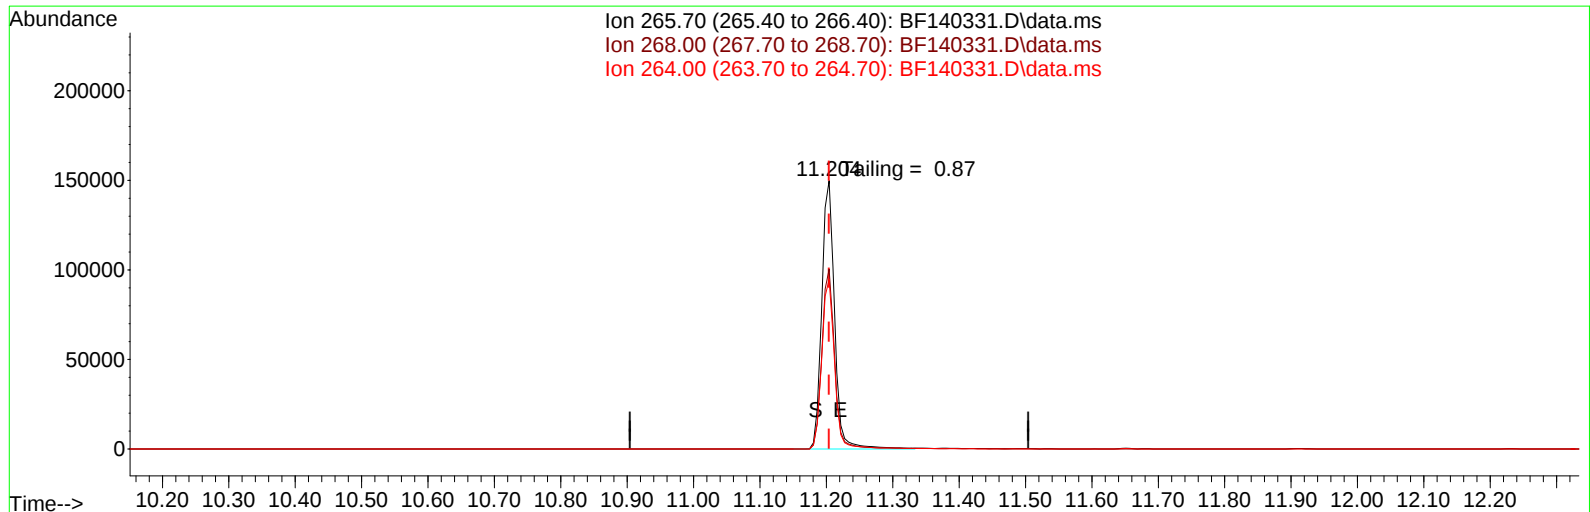

TIC: BF140331.D\data.ms

(70) Pentachlorophenol (C)

11.204min (0.000) 23118.21 ng




response 201406

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.05
264.00	62.90	63.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111324\
Data File : BF140331.D
Acq On : 13 Nov 2024 08:35
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 13 14:44:41 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF111324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 13 14:40:06 2024
Response via : Initial Calibration

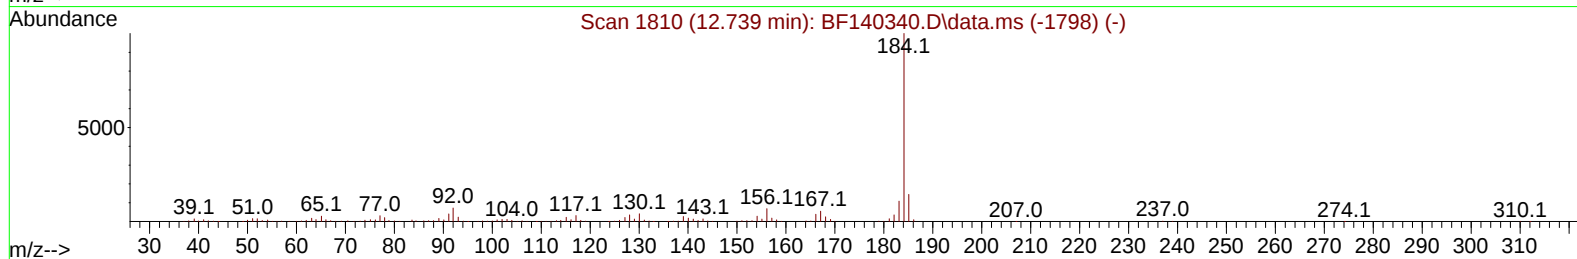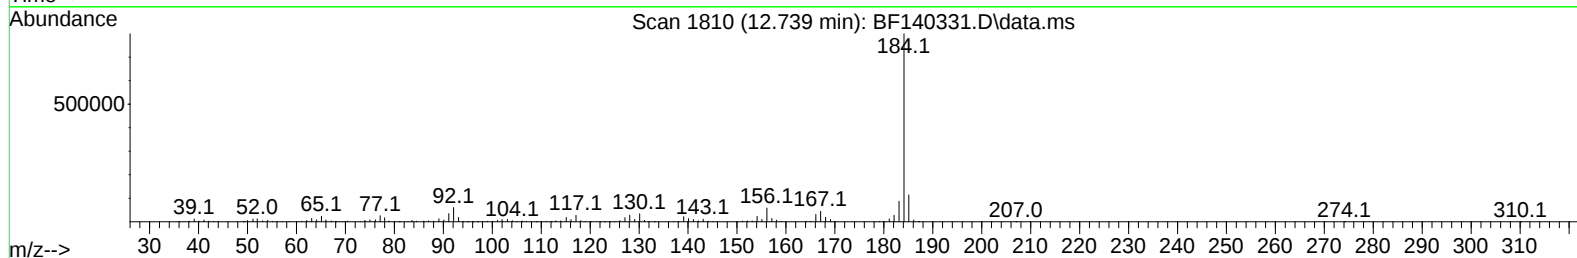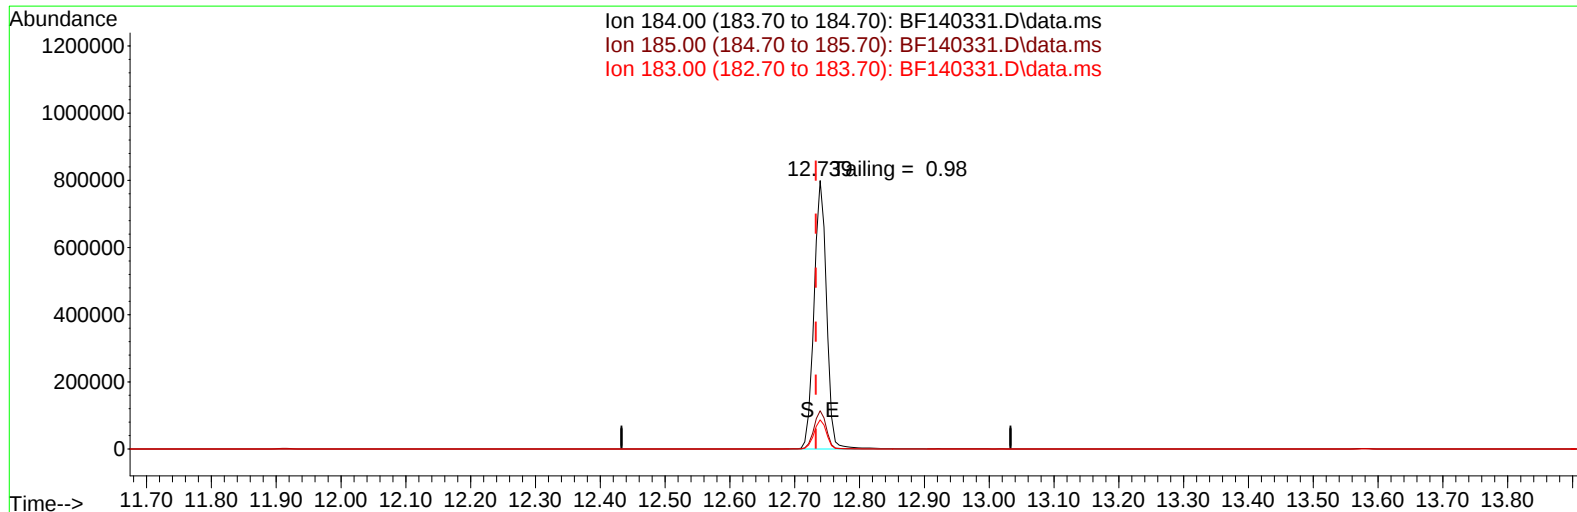

TIC: BF140331.D\data.ms

(77) Benzidine

12.739min (+ 0.006) 47514.94 ng

response 1075955

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.90	14.29
183.00	10.80	10.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/13/2024	BNA_F	<u>BF140331.D</u>
Compound Name	Response	Retention Time
DDT	544964	13.58
DDD	17817	13.269
DDE	776	12.927
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
18593	563557	3.30

Instrument :
BNA_F
ClientSampleId :
DFTPP