
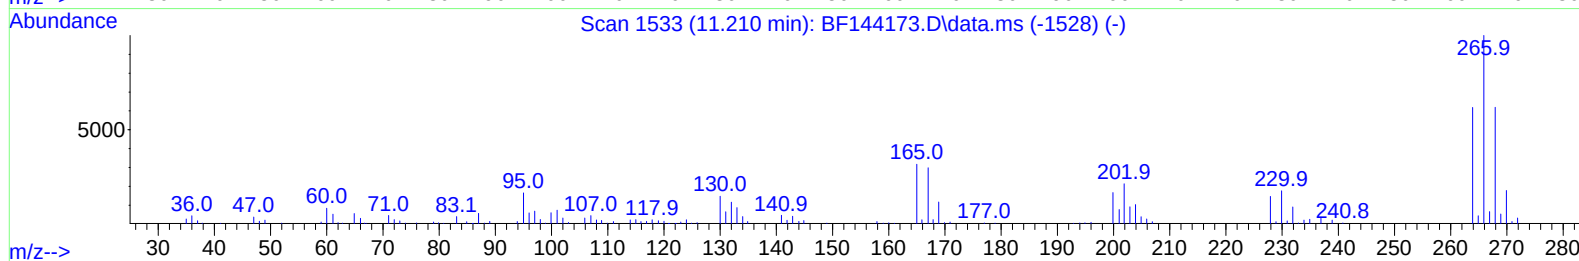
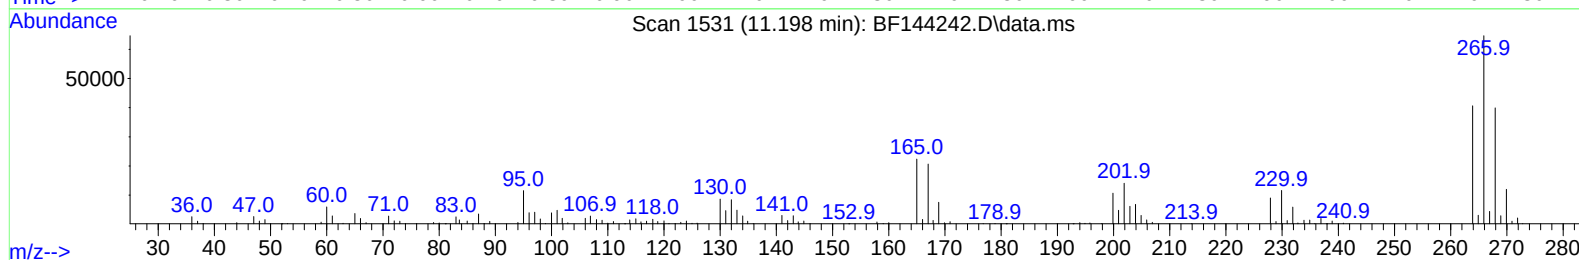


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111325\
Data File : BF144242.D
Acq On : 13 Nov 2025 14:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 13 15:07:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

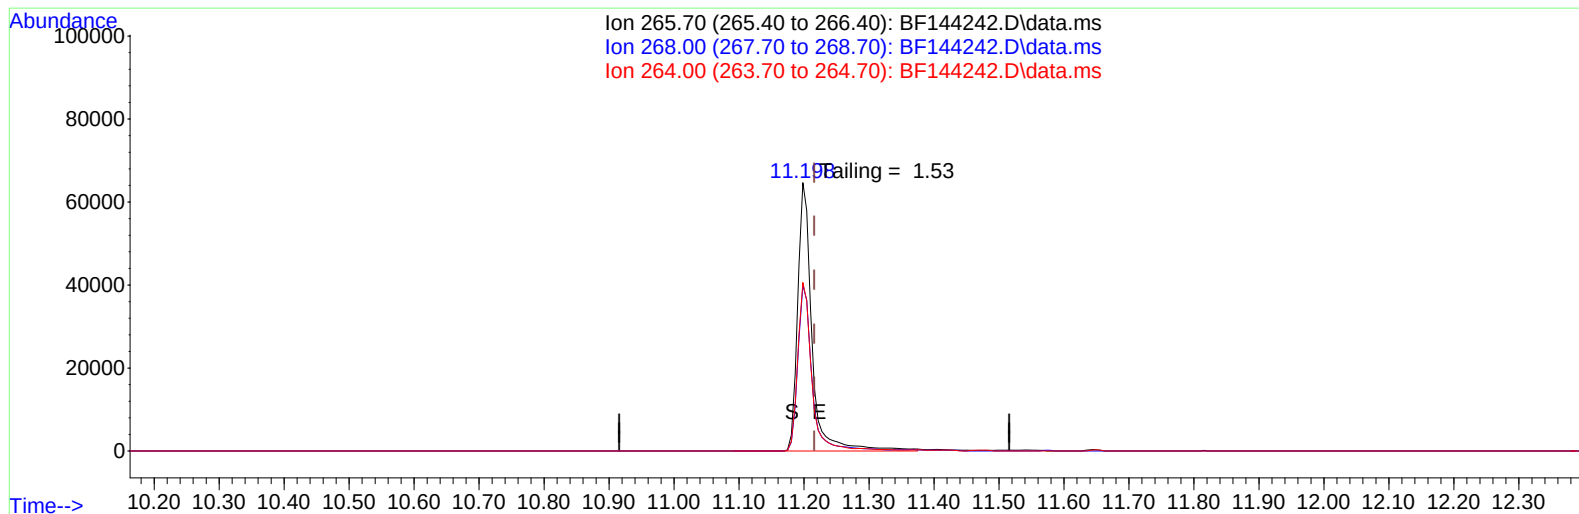

TIC: BF144242.D\data.ms

(70) Pentachlorophenol (C)




11.198min (-0.017) 60191.23 ng

response 99588

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.90	61.71
264.00	61.80	62.80
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF111325\  
Data File : BF144242.D  
Acq On    : 13 Nov 2025  14:26  
Operator  : RC/JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 13 15:07:56 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF110525.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Nov 05 18:37:33 2025
Response via : Initial Calibration

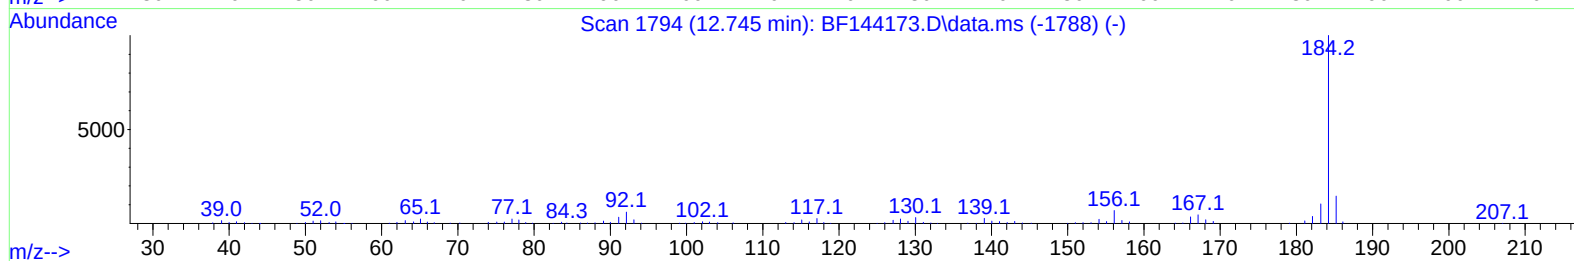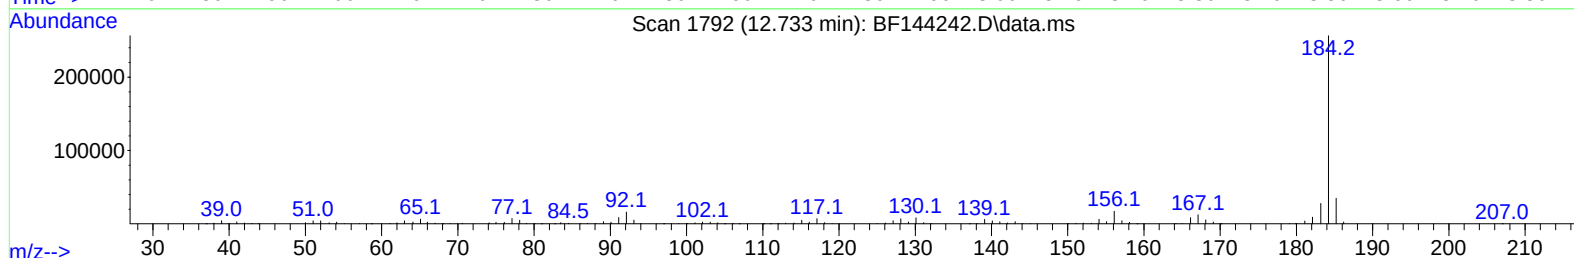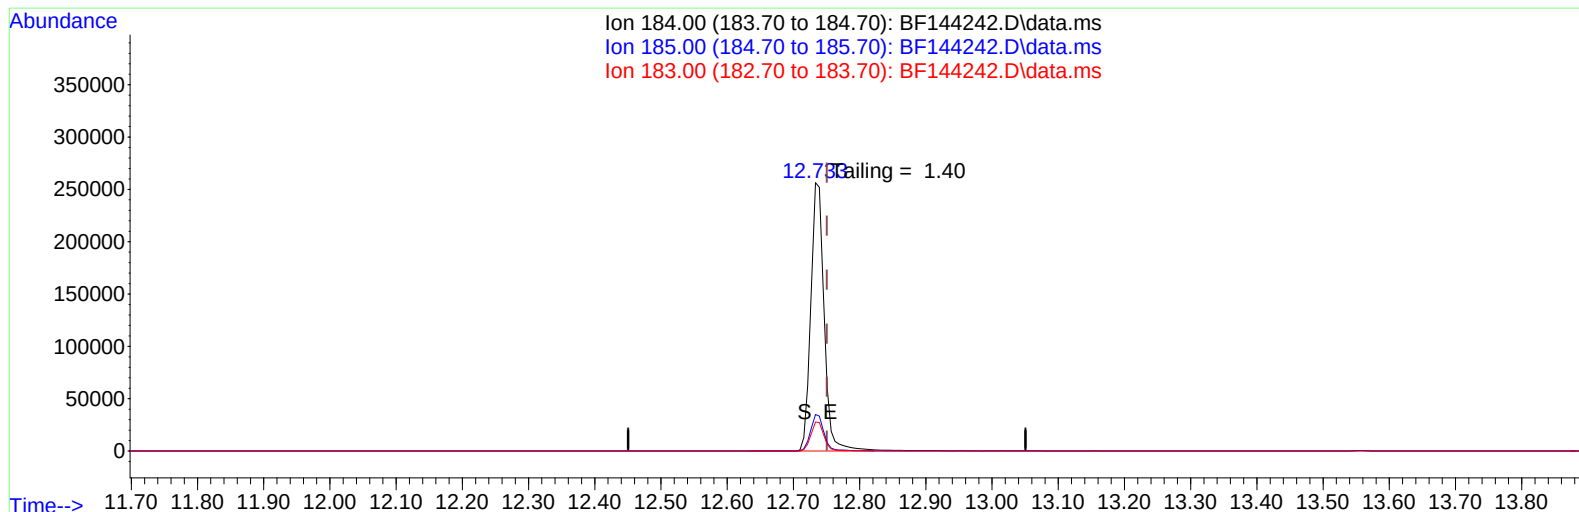

TIC: BF144242.D\data.ms

(77) Benzidine

12.733min (-0.017) 0.00 ng

response **363312**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.60
183.00	10.40	10.83
0.00	0.00	0.00