
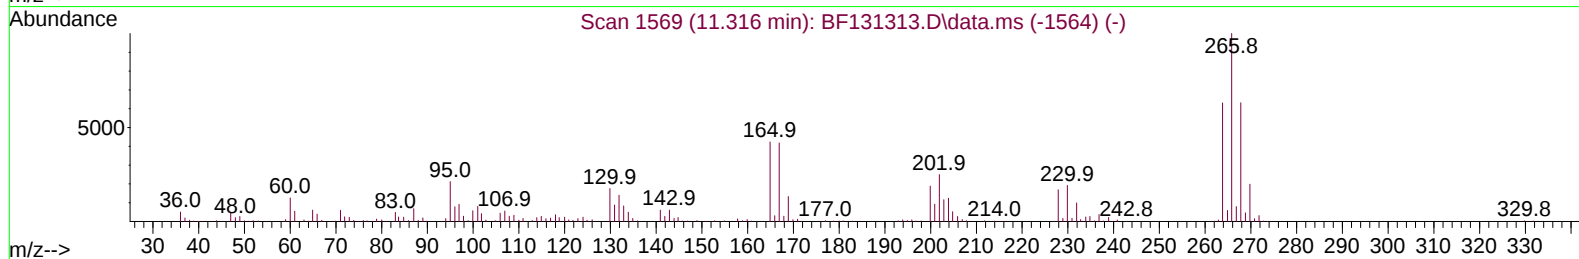
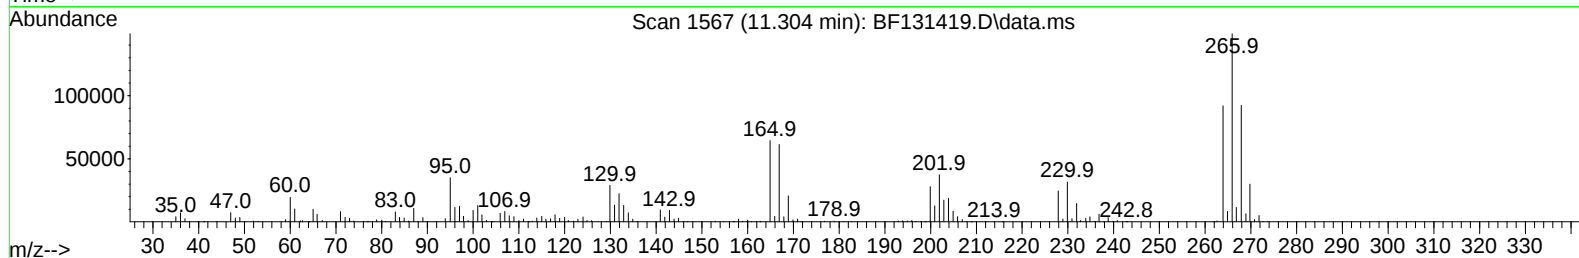


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112822\
Data File : BF131419.D
Acq On : 28 Nov 2022 09:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 05:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 00:18:36 2022
Response via : Initial Calibration

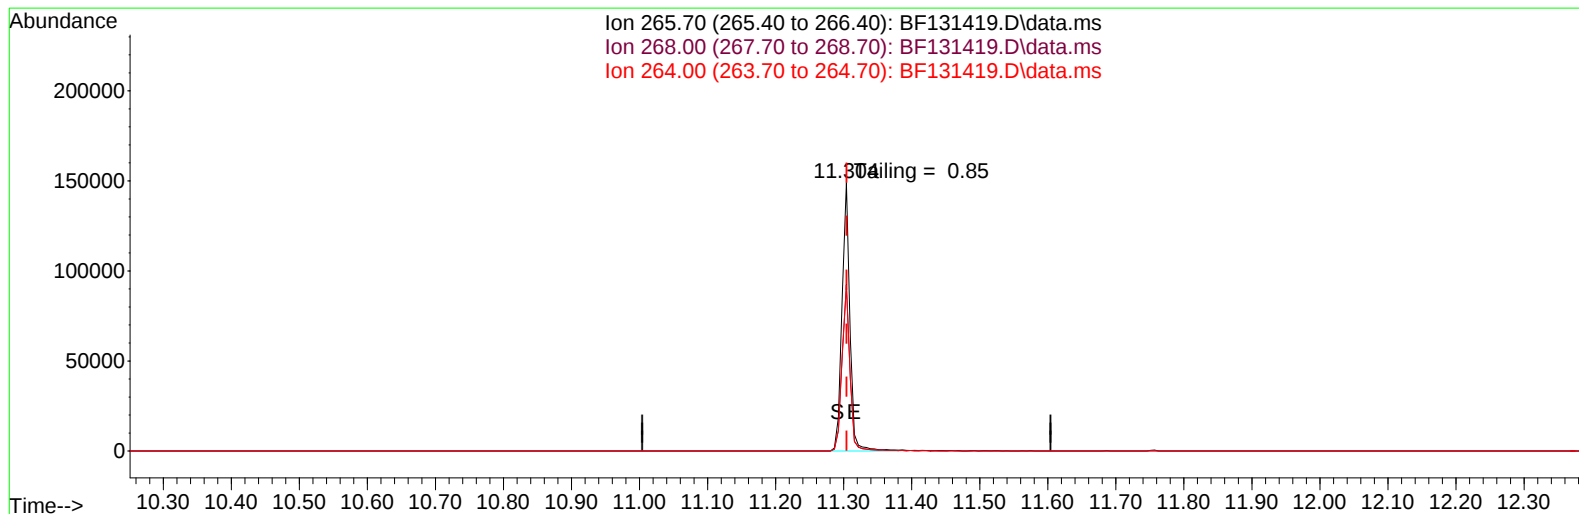

TIC: BF131419.D\data.ms

(70) Pentachlorophenol (C)




11.304min (0.000) 23375.97 ng

response 120775

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	61.92
264.00	63.00	61.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112822\
Data File : BF131419.D
Acq On : 28 Nov 2022 09:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Nov 29 05:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 00:18:36 2022
Response via : Initial Calibration

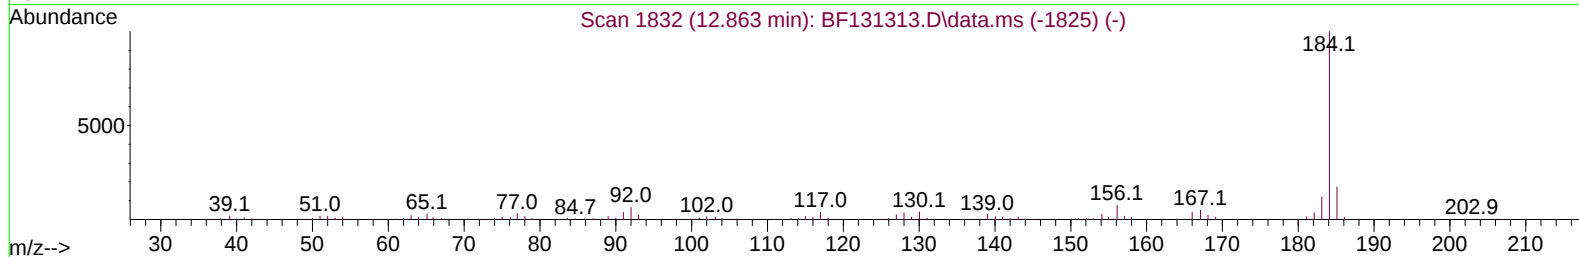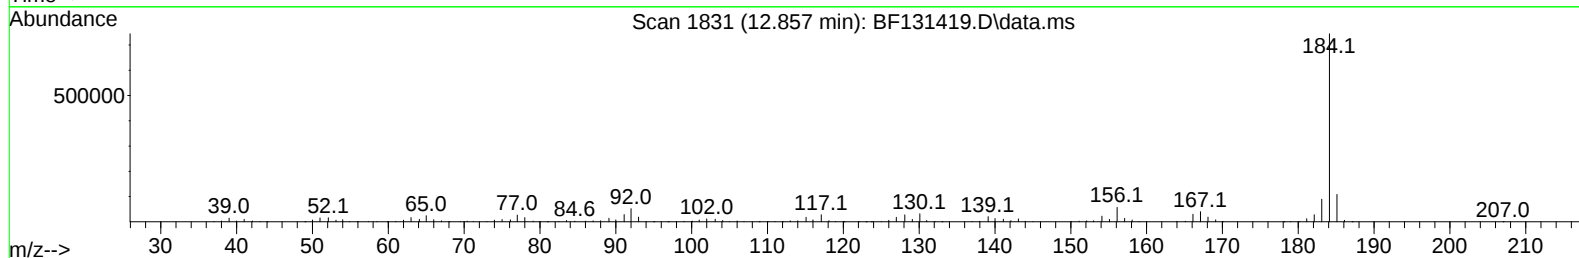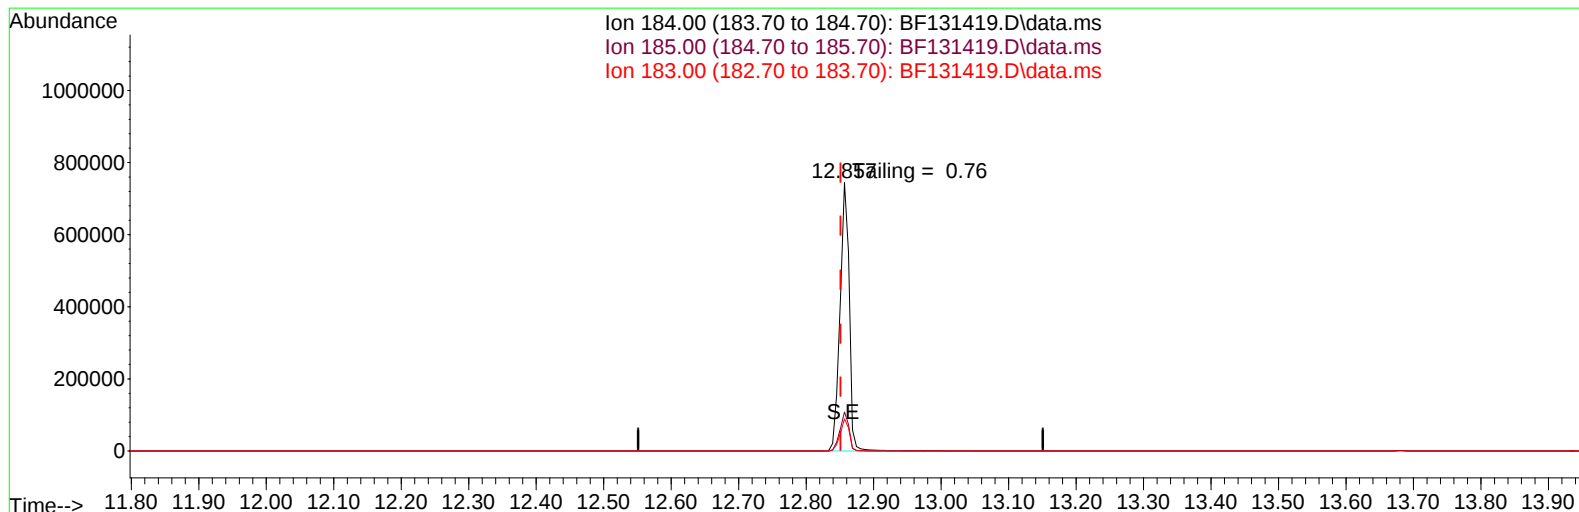

TIC: BF131419.D\data.ms

(77) Benzidine

12.857min (+ 0.006) 0.00 ng

response 709137

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.58
183.00	12.00	12.01
0.00	0.00	0.00