
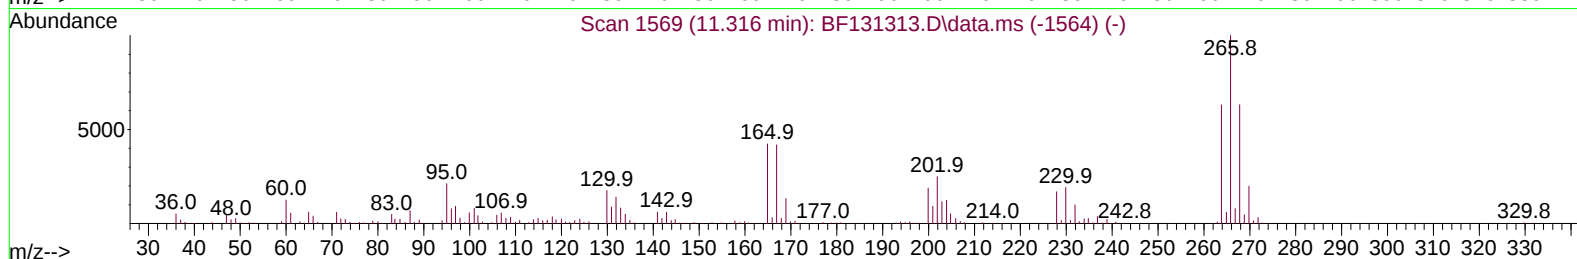
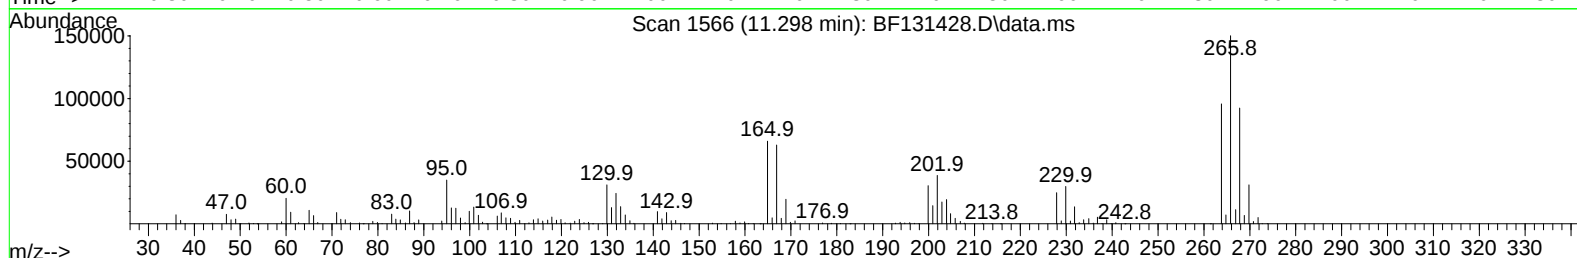


Quant Time: Nov 29 05:20:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 00:18:36 2022
Response via : Initial Calibration

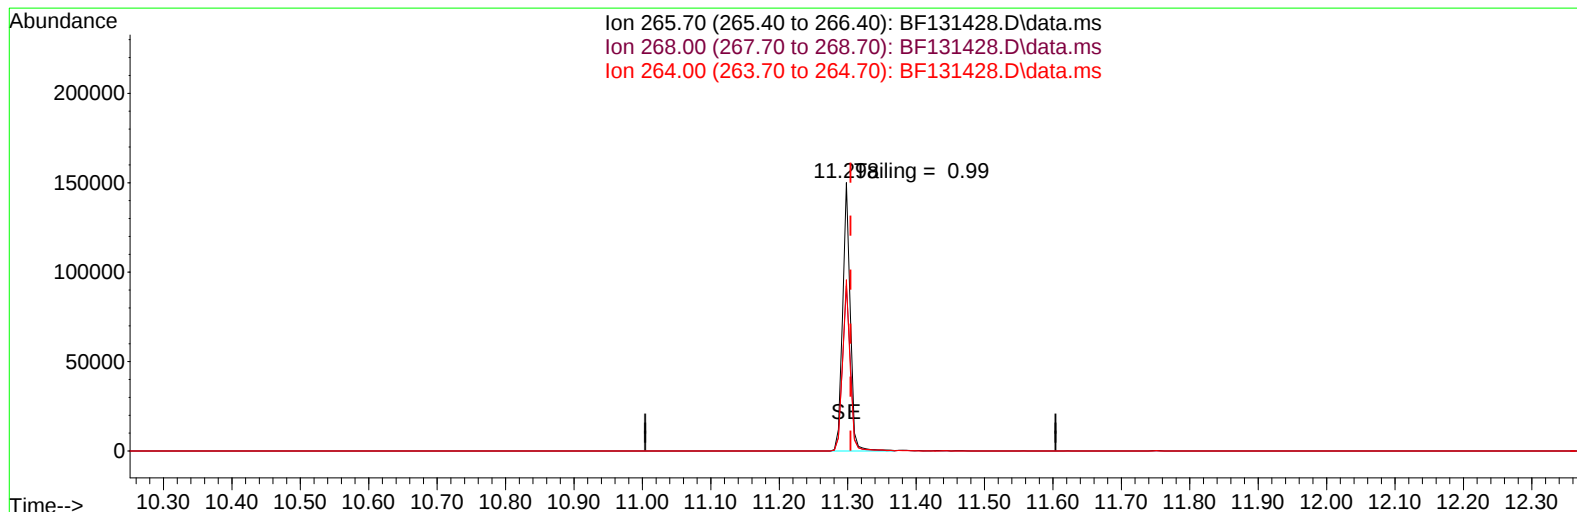

TIC: BF131428.D\data.ms

(70) Pentachlorophenol (C)




11.298min (-0.006) 250991.93 ng

response **117177**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	61.56
264.00	63.00	63.82
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112822\  
Data File : BF131428.D  
Acq On    : 28 Nov 2022  14:21  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Nov 29 05:20:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 00:18:36 2022
Response via : Initial Calibration

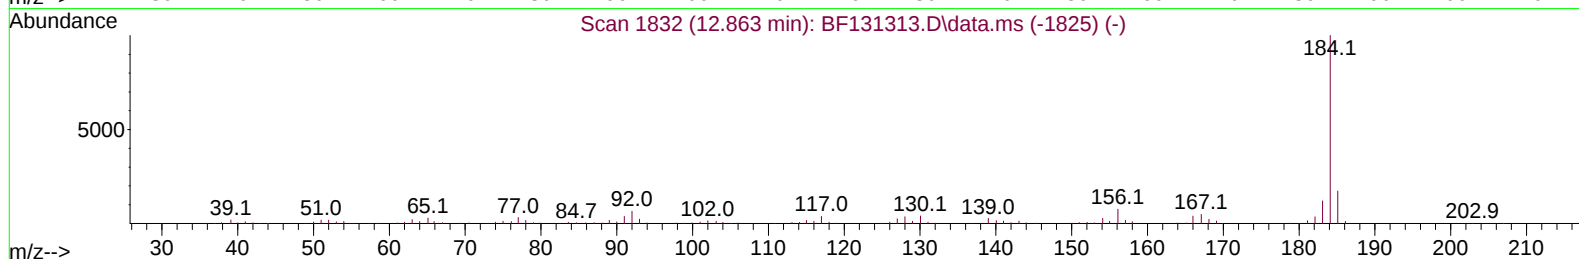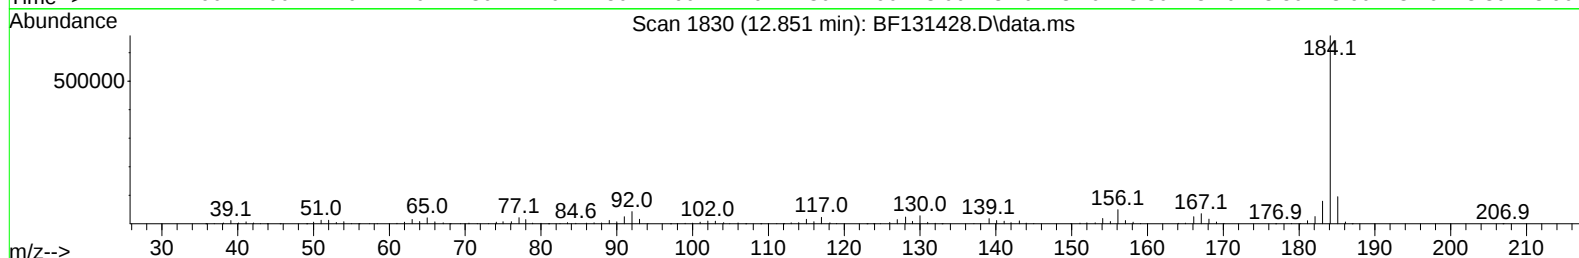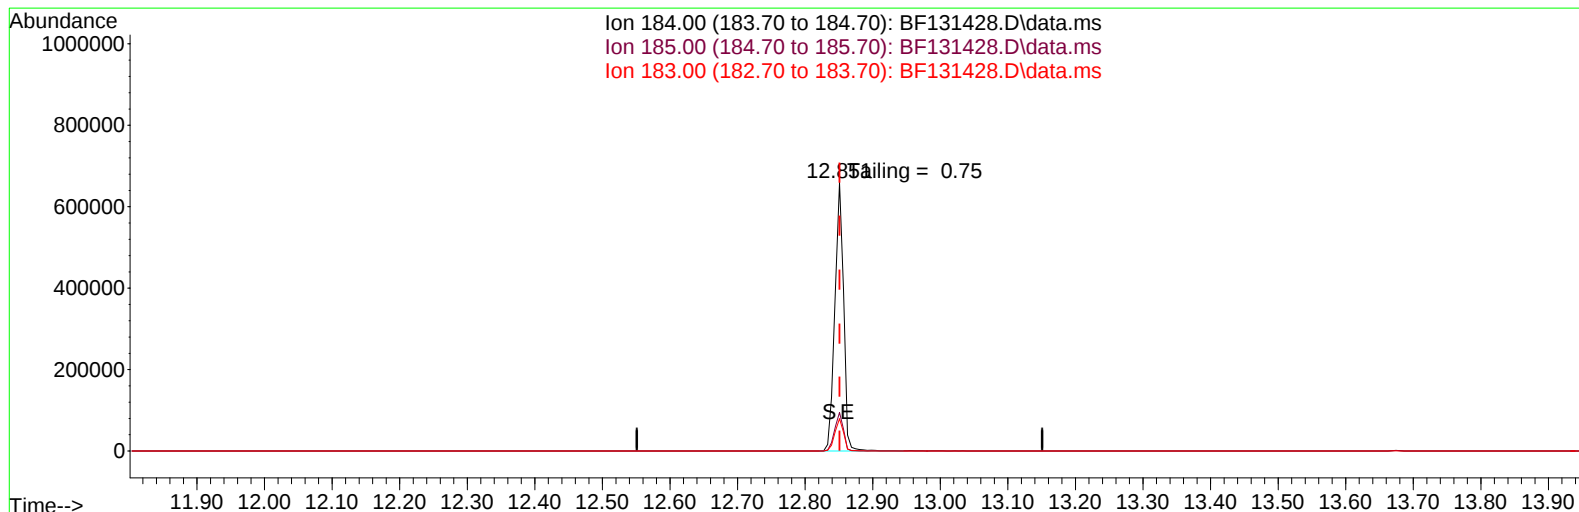

TIC: BF131428.D\data.ms

(77) Benzidine

12.851min (-0.000) 0.00 ng

response **592249**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.37
183.00	12.00	12.05
0.00	0.00	0.00