
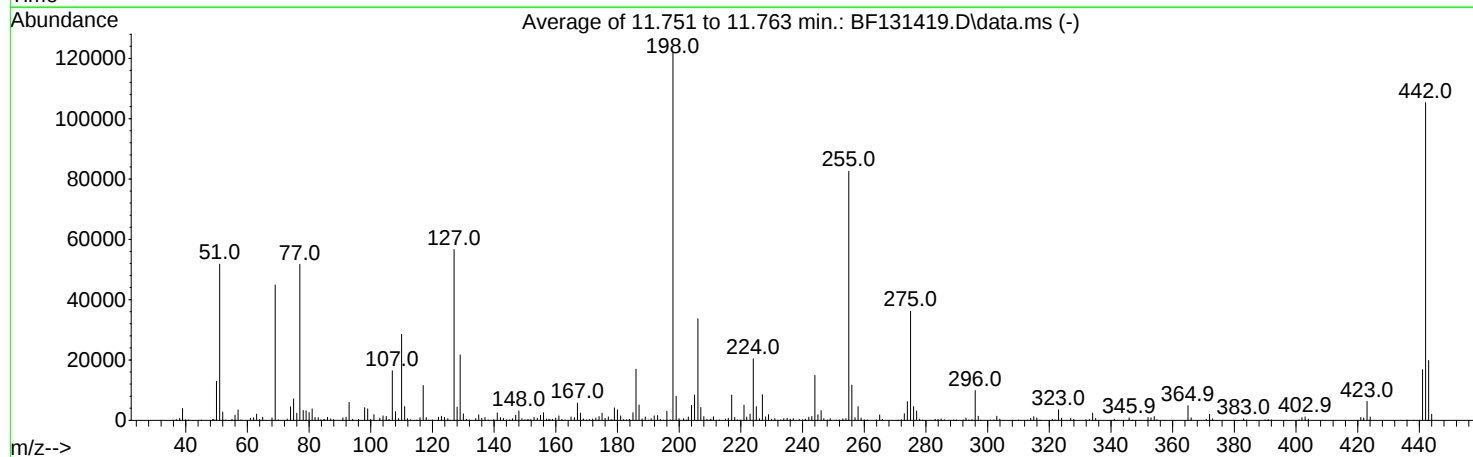


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112822\
 Data File : BF131419.D
 Acq On : 28 Nov 2022 09:01
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 01 12:46:17 2022

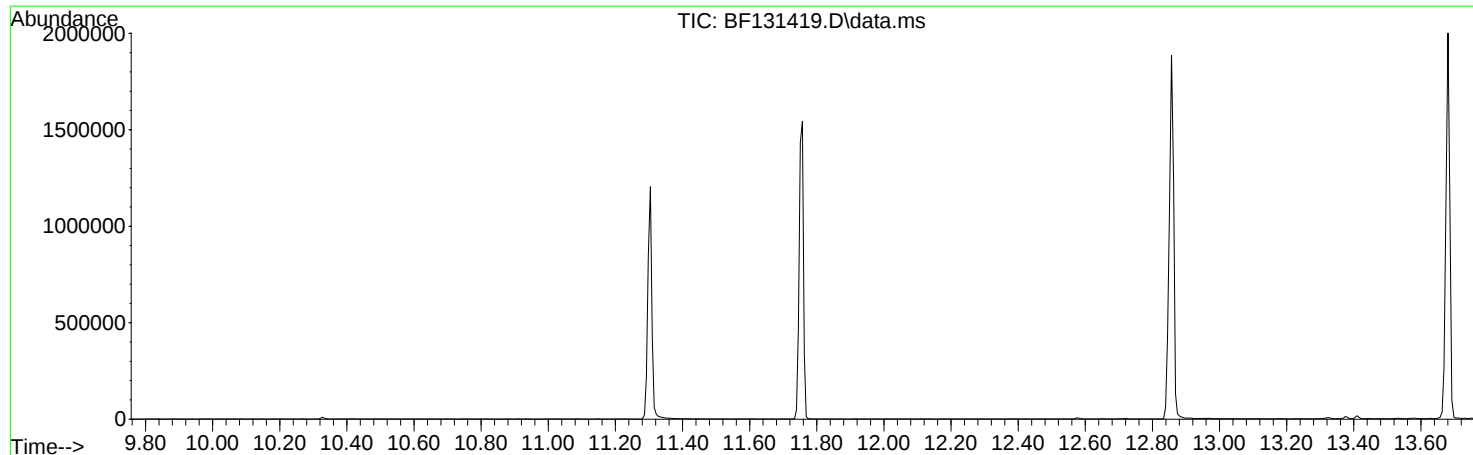




AutoFind: Scans 1643, 1644, 1645; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.4	51746	PASS
68	69	0.00	2	1.8	800	PASS
69	198	0.00	100	36.8	44886	PASS
70	69	0.00	2	0.5	209	PASS
127	198	10	80	46.4	56644	PASS
197	198	0.00	2	0.1	145	PASS
198	198	100	100	100.0	121968	PASS
199	198	5	9	6.5	7965	PASS
275	198	10	60	29.7	36175	PASS
365	198	1	100	4.0	4862	PASS
441	198	0.01	100	13.8	16804	PASS
442	442	50	100	100.0	105320	PASS
443	442	15	24	18.8	19839	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112822\
Data File : BF131419.D
Acq On : 28 Nov 2022 09:01
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 29 05:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 00:18:36 2022
Response via : Initial Calibration

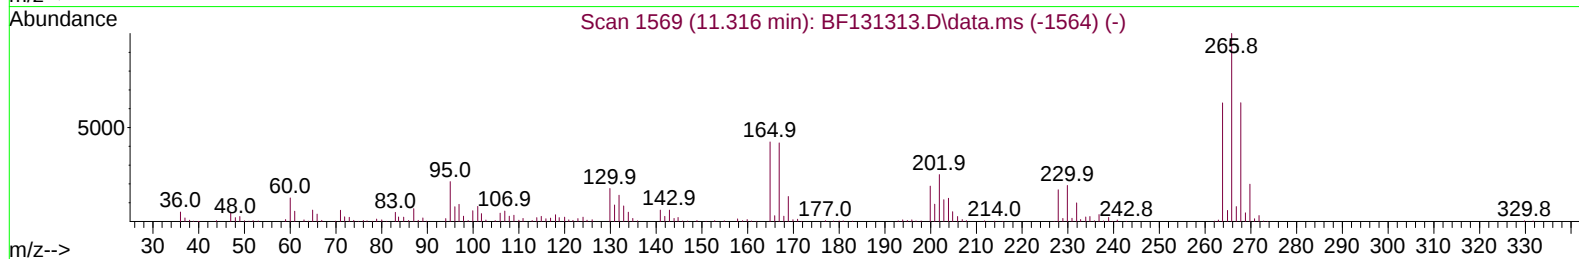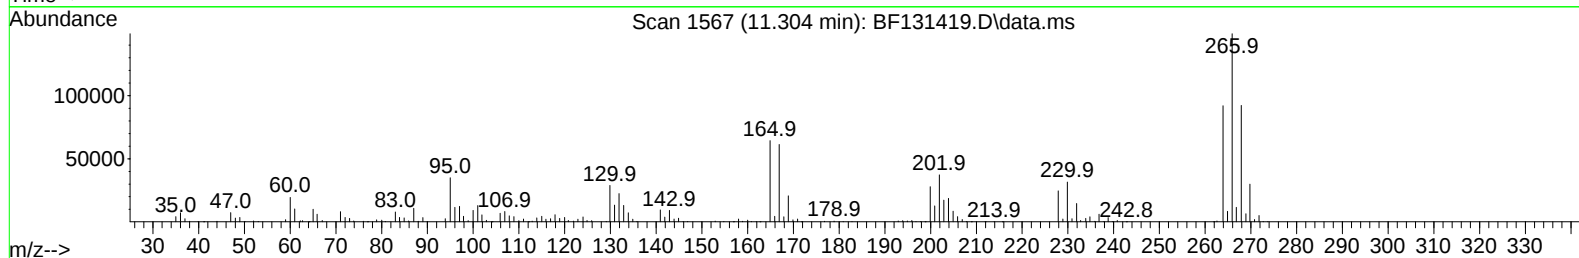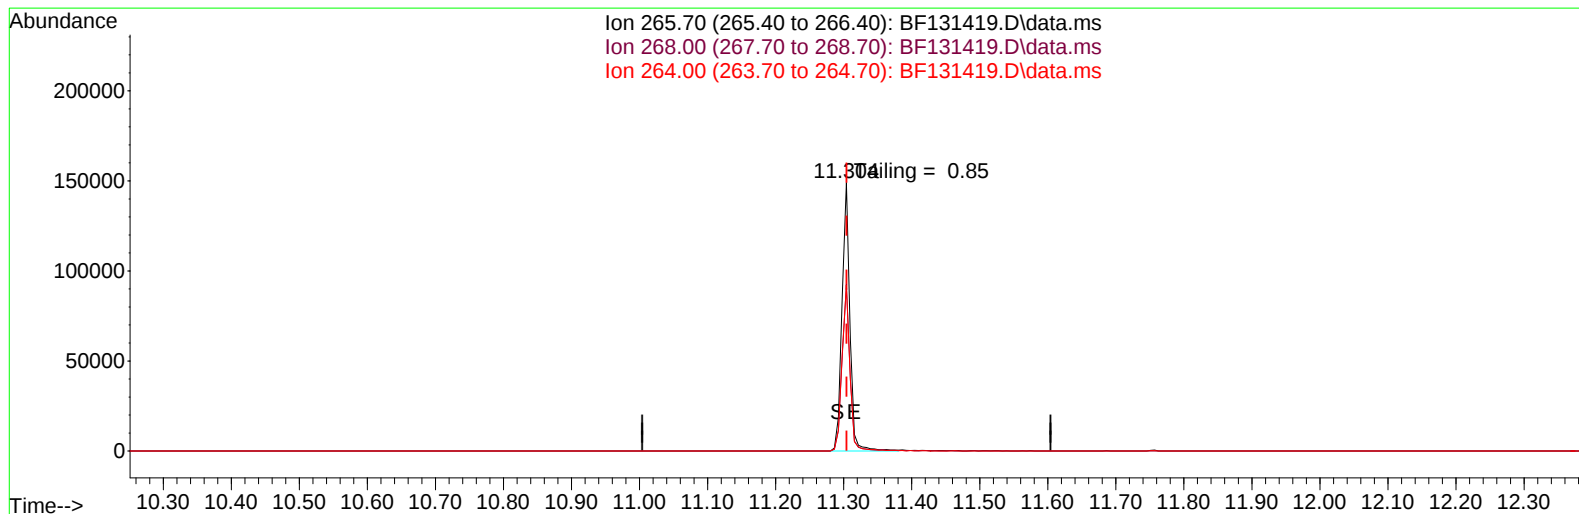

TIC: BF131419.D\data.ms

(70) Pentachlorophenol (C)

11.304min (0.000) 23375.97 ng




response 120775

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	61.92
264.00	63.00	61.76
0.00	0.00	0.00

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112822\  
Data File : BF131419.D  
Acq On    : 28 Nov 2022  09:01  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 29 05:18:07 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 00:18:36 2022
Response via : Initial Calibration

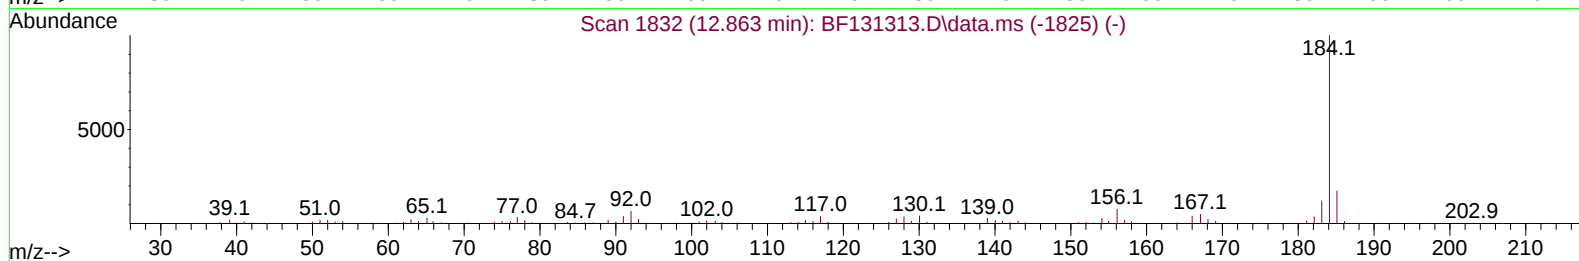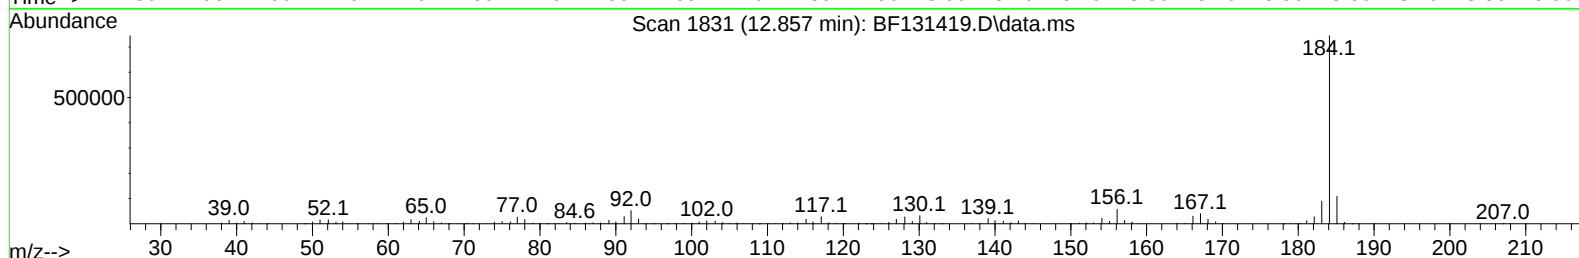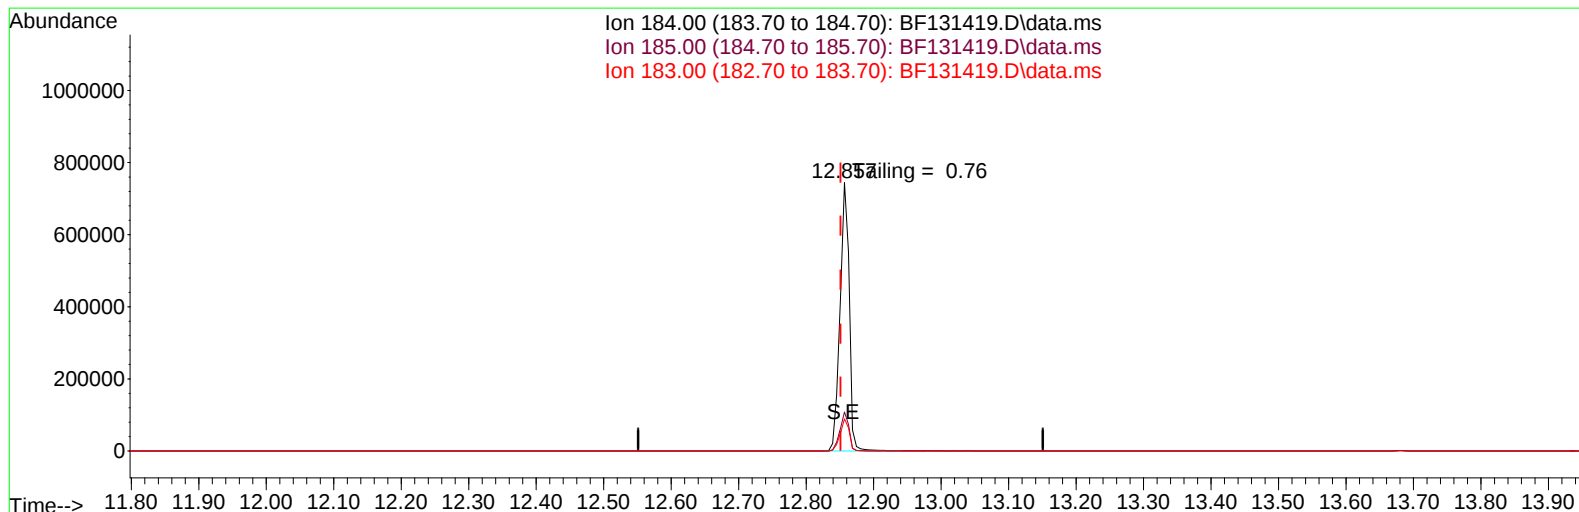

TIC: BF131419.D\data.ms

(77) Benzidine

12.857min (+ 0.006) 0.00 ng

response 709137

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.58
183.00	12.00	12.01
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/28/2022	BNA_F	<u>BF131419.D</u>
Compound Name	Response	Retention Time
DDT	315613	13.68
DDD	5215	13.374
DDE	215	13.039
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5430	321043	1.69

Instrument :
BNA_F
ClientSampleId :
DFTPP