


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112822\
 Data File : BF131428.D
 Acq On : 28 Nov 2022 14:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 01 12:46:17 2022

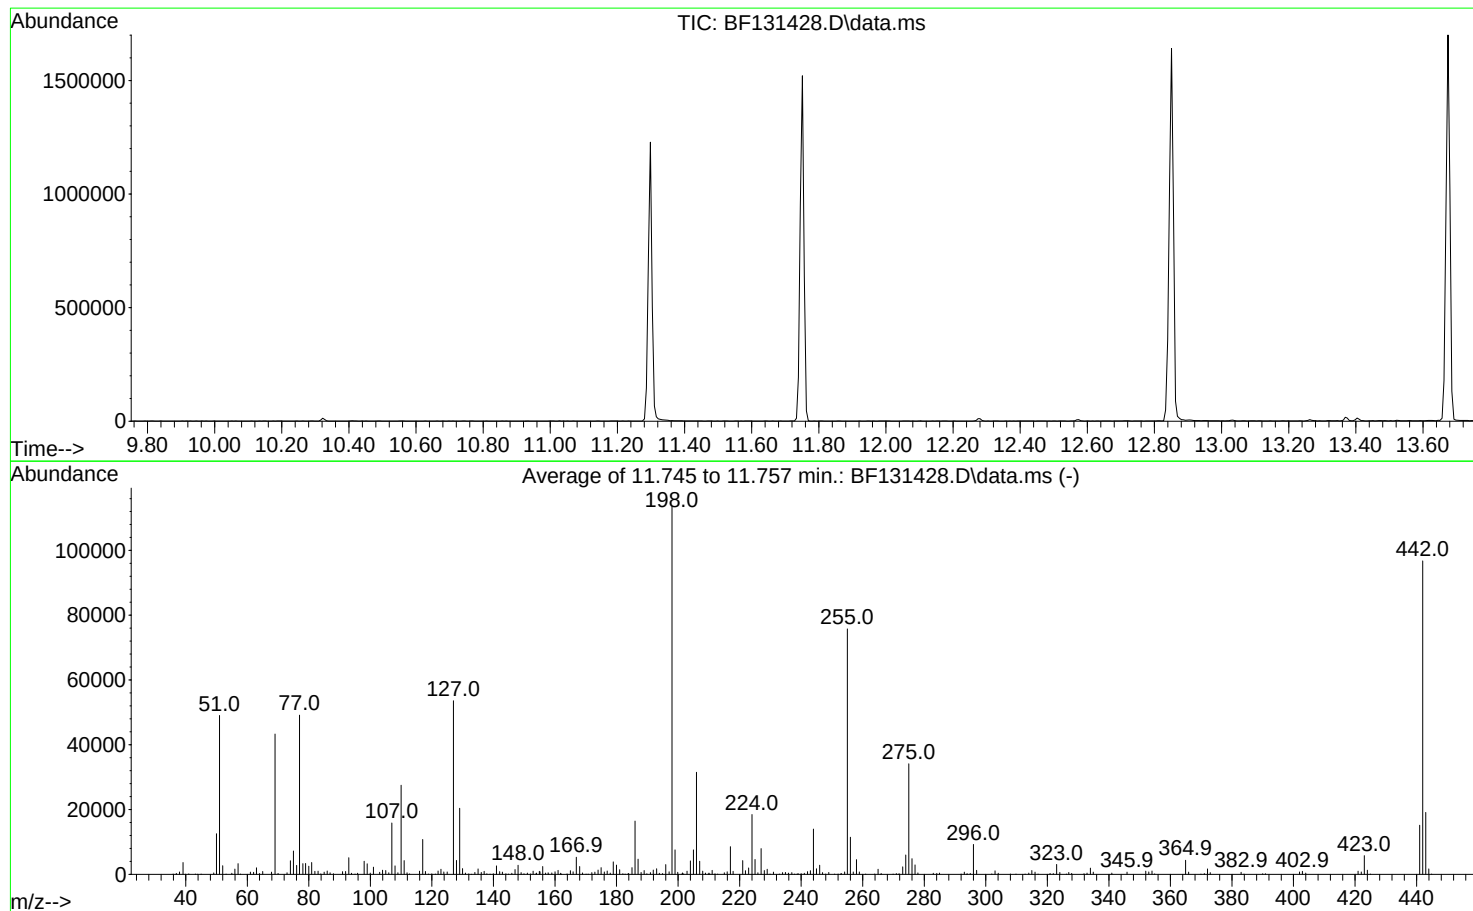




AutoFind: Scans 1642, 1643, 1644; Background Corrected with Scan 1637

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.2	49016	PASS
68	69	0.00	2	1.5	654	PASS
69	198	0.00	100	38.1	43285	PASS
70	69	0.00	2	0.6	280	PASS
127	198	10	80	47.2	53592	PASS
197	198	0.00	2	0.7	747	PASS
198	198	100	100	100.0	113581	PASS
199	198	5	9	6.6	7528	PASS
275	198	10	60	30.0	34107	PASS
365	198	1	100	3.8	4322	PASS
441	198	0.01	100	13.3	15147	PASS
442	442	50	100	100.0	96781	PASS
443	442	15	24	19.8	19116	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112822\
Data File : BF131428.D
Acq On : 28 Nov 2022 14:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 29 05:20:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 00:18:36 2022
Response via : Initial Calibration

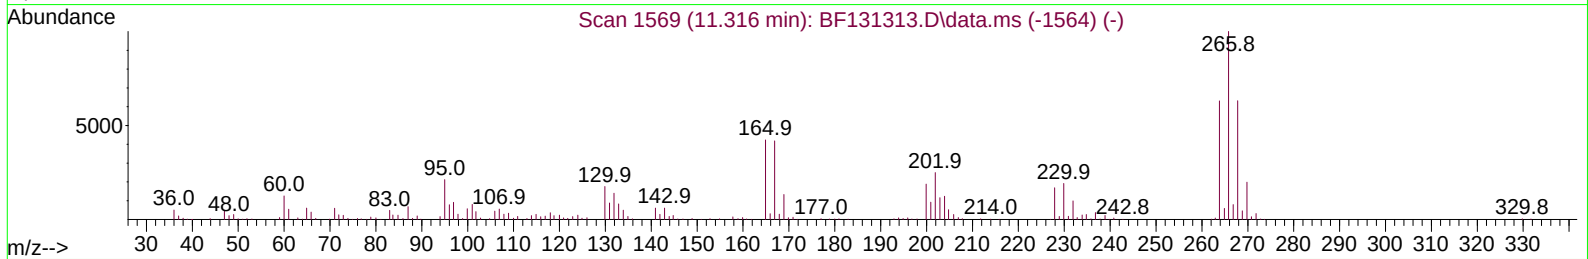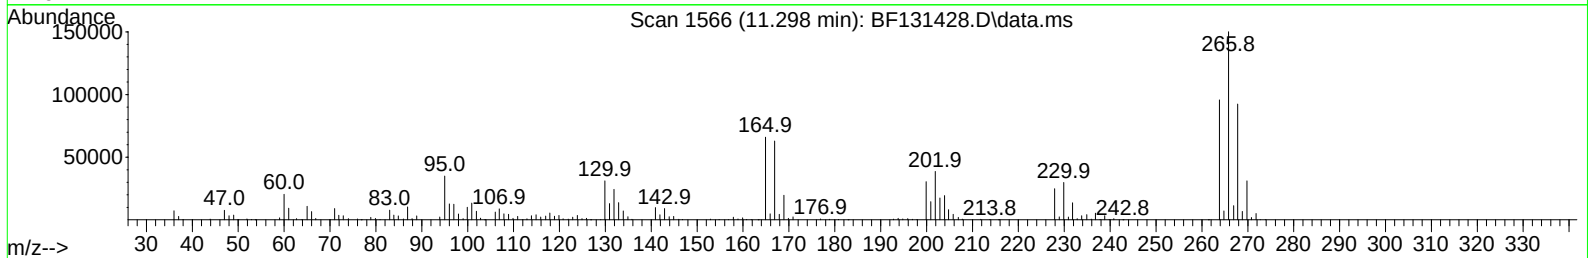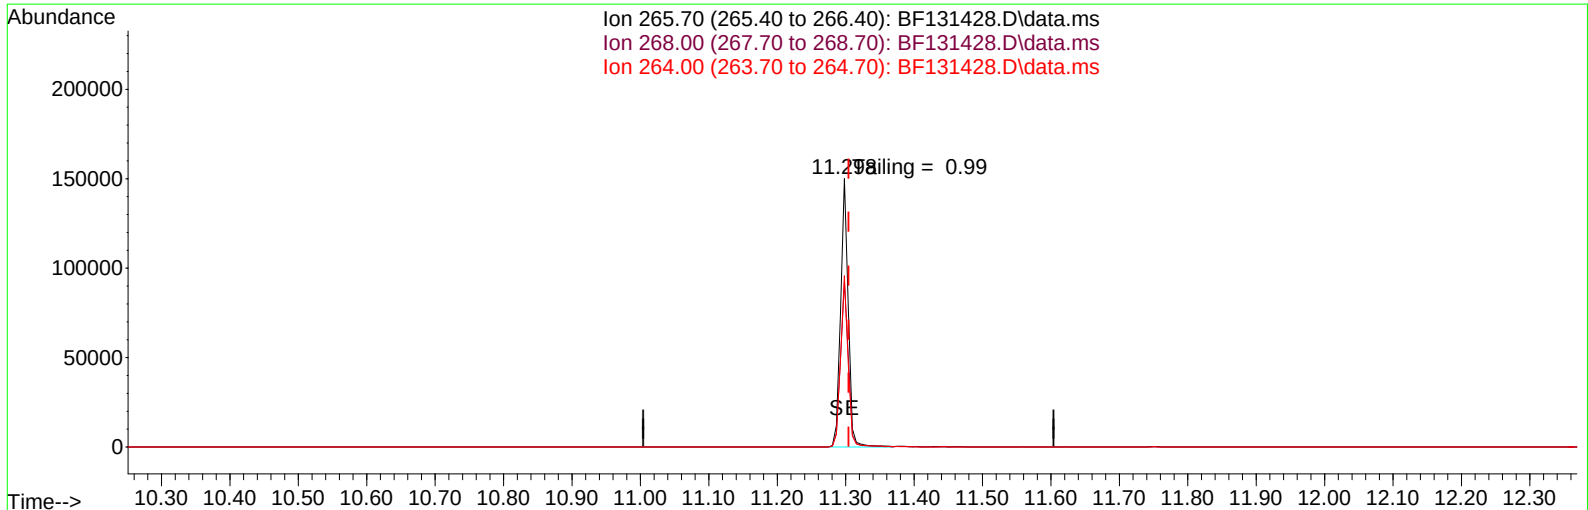

TIC: BF131428.D\data.ms

(70) Pentachlorophenol (C)

11.298min (-0.006) 250991.93 ng




response 117177

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.20	61.56
264.00	63.00	63.82
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF112822\
Data File : BF131428.D
Acq On : 28 Nov 2022 14:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Nov 29 05:20:46 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF112122.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Nov 29 00:18:36 2022
Response via : Initial Calibration

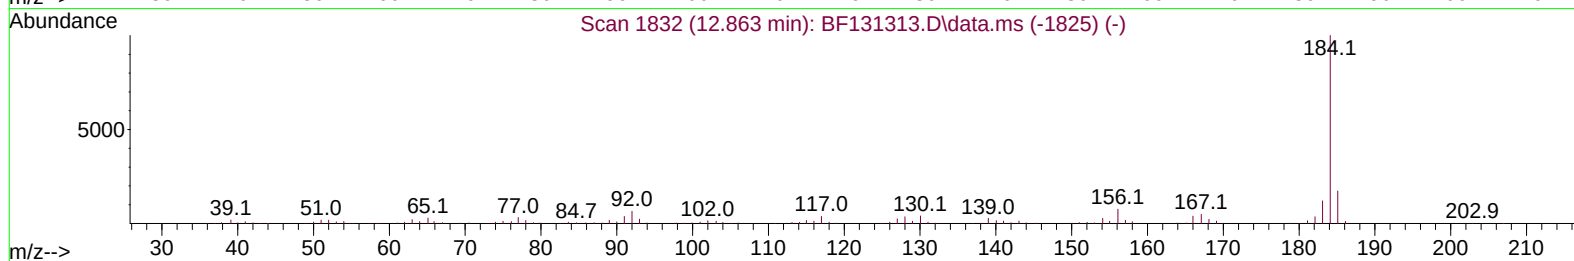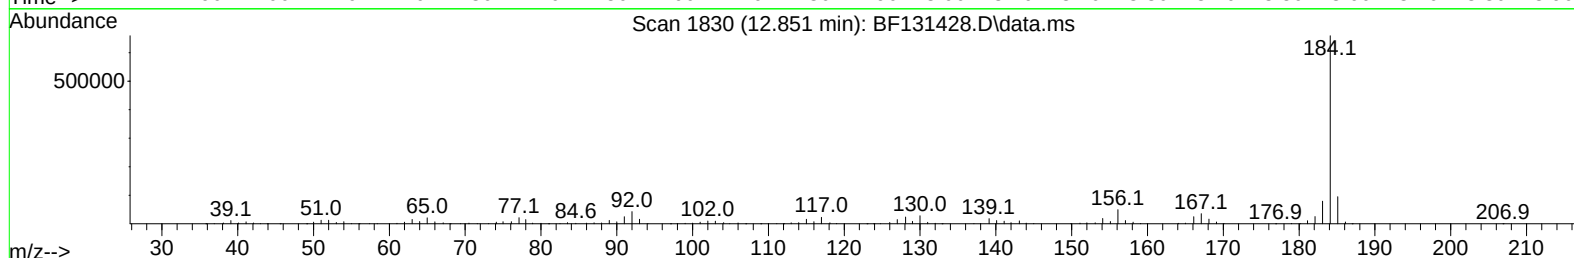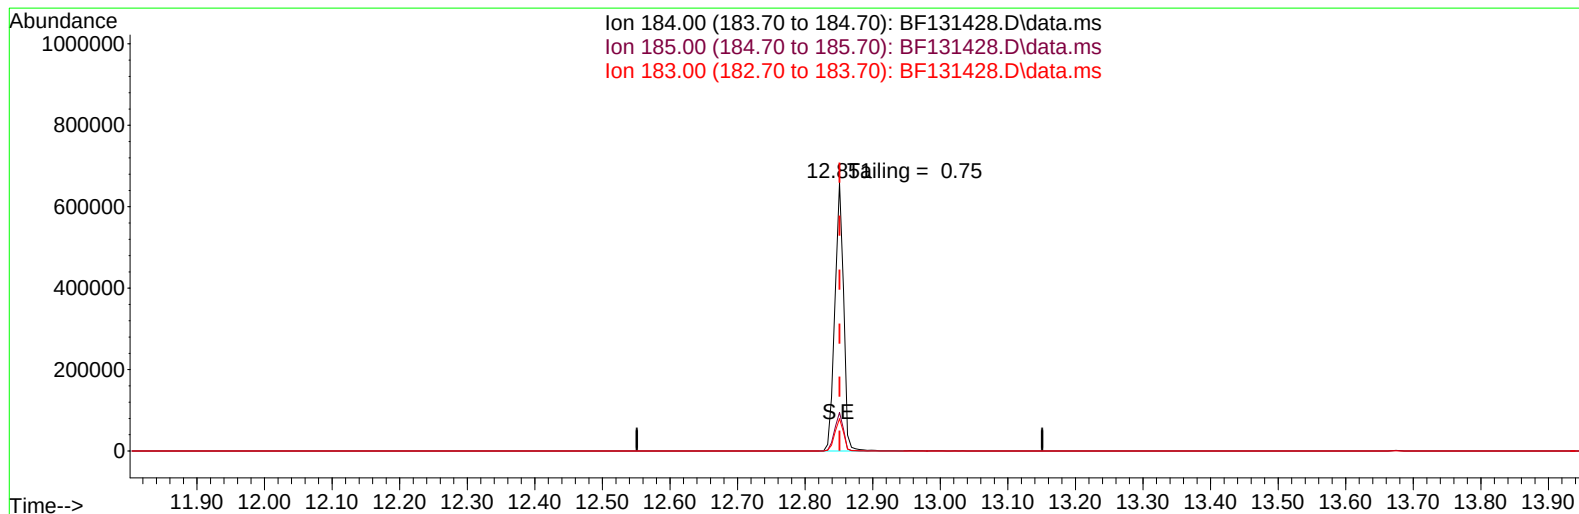

TIC: BF131428.D\data.ms

(77) Benzidine

12.851min (-0.000) 0.00 ng

response 592249

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	17.30	14.37
183.00	12.00	12.05
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
11/28/2022	BNA_F	<u>BF131428.D</u>
Compound Name	Response	Retention Time
DDT	277688	13.674
DDD	5443	13.369
DDE	698	13.033
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6141	283829	2.16

Instrument :
BNA_F
ClientSampleId :
DFTPP