


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120320\
 Data File : BF122529.D
 Acq On : 3 Dec 2020 9:57
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF110920.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 04 12:52:10 2020

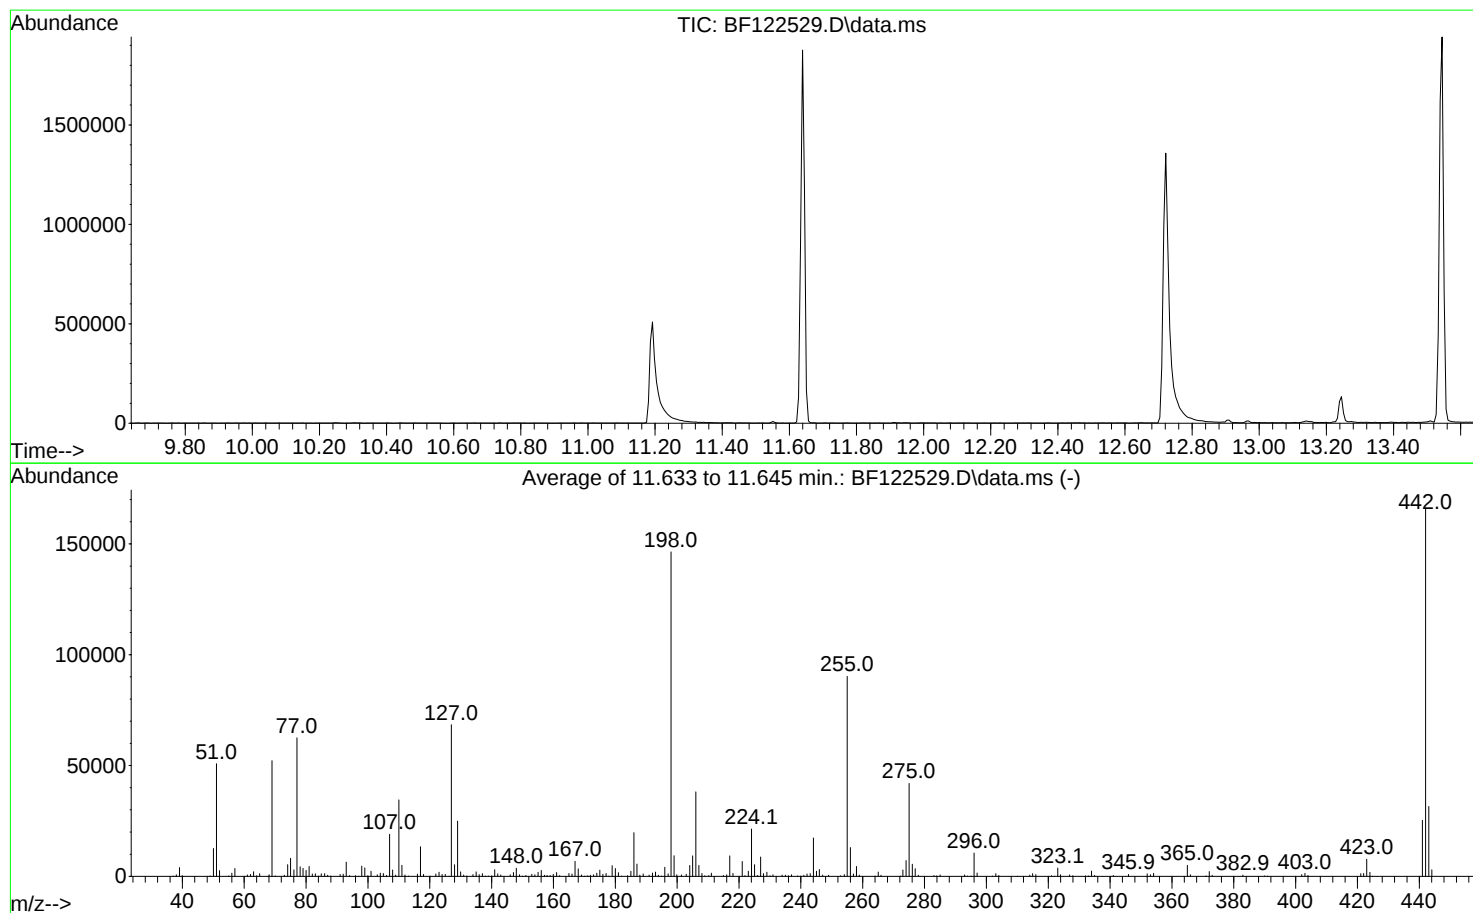

AutoFind: Scans 1623, 1624, 1625; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.7	50843	PASS
68	69	0.00	2	1.4	738	PASS
69	198	0.00	100	35.6	52197	PASS
70	69	0.00	2	0.4	187	PASS
127	198	10	80	46.8	68475	PASS
197	198	0.00	2	0.8	1183	PASS
198	198	100	100	100.0	146432	PASS
199	198	5	9	6.4	9304	PASS
275	198	10	60	28.6	41947	PASS
365	198	1	100	3.4	5014	PASS
441	198	0.01	100	17.3	25318	PASS
442	442	100	100	100.0	165968	PASS
443	442	15	24	19.0	31537	PASS