
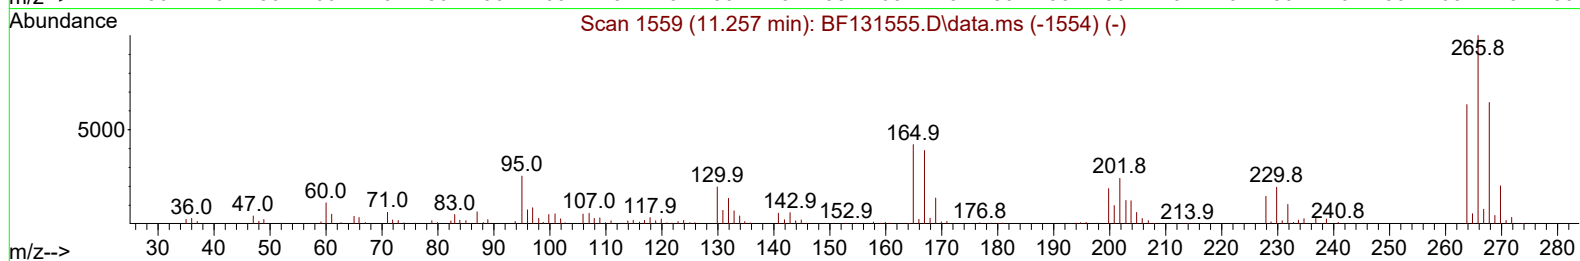
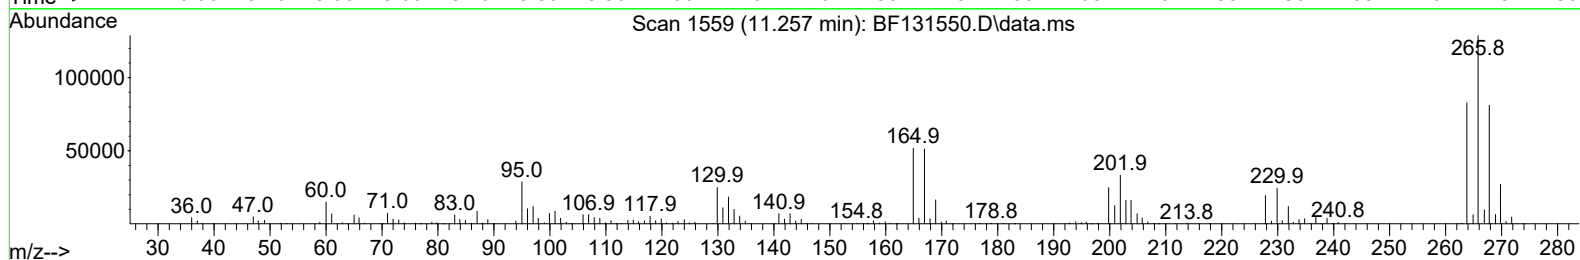


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120822\
Data File : BF131550.D
Acq On : 08 Dec 2022 11:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 09:23:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 06:08:27 2022
Response via : Initial Calibration

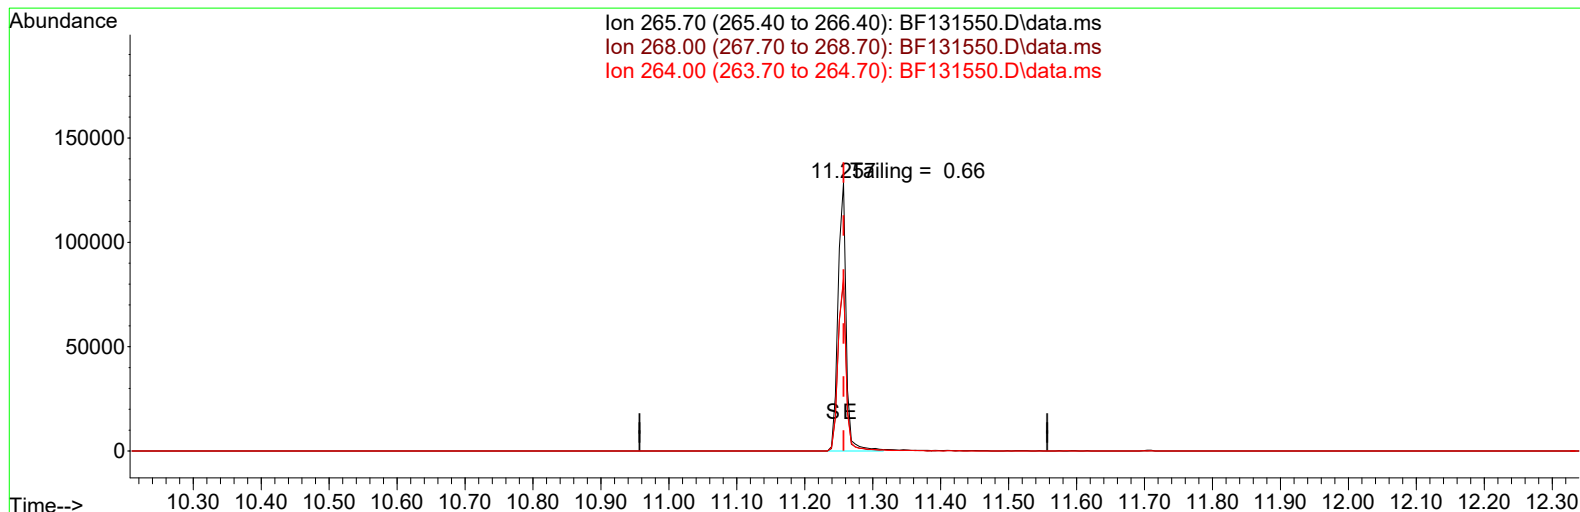

TIC: BF131550.D\data.ms

(70) Pentachlorophenol (C)




11.257min (-0.000) 23941.32 ng

response 107018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	63.00
264.00	63.40	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120822\
 Data File : BF131550.D
 Acq On : 08 Dec 2022 11:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 09 09:23:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 09 06:08:27 2022
 Response via : Initial Calibration

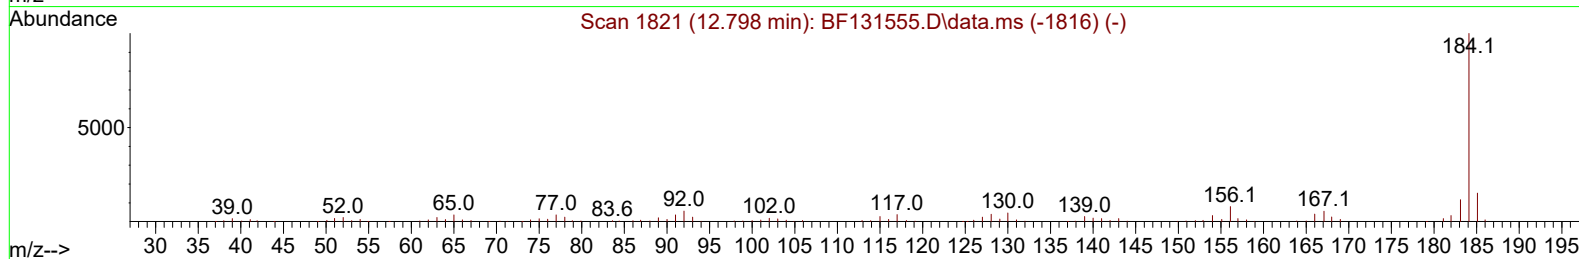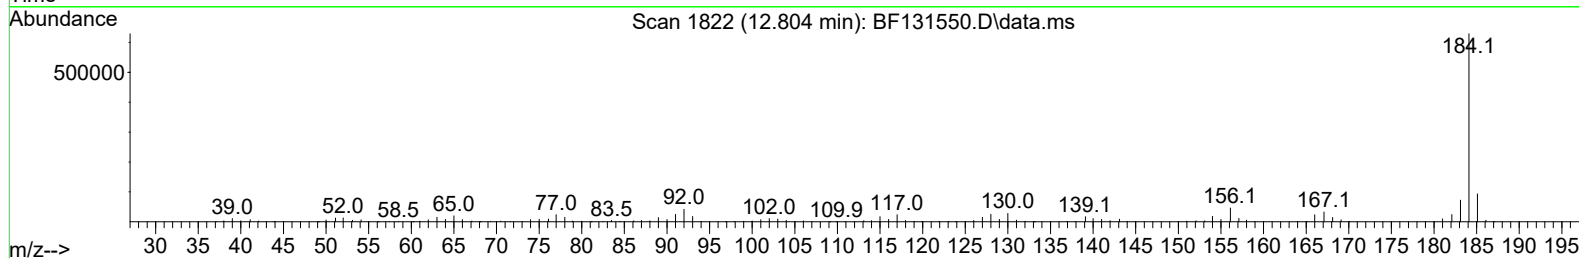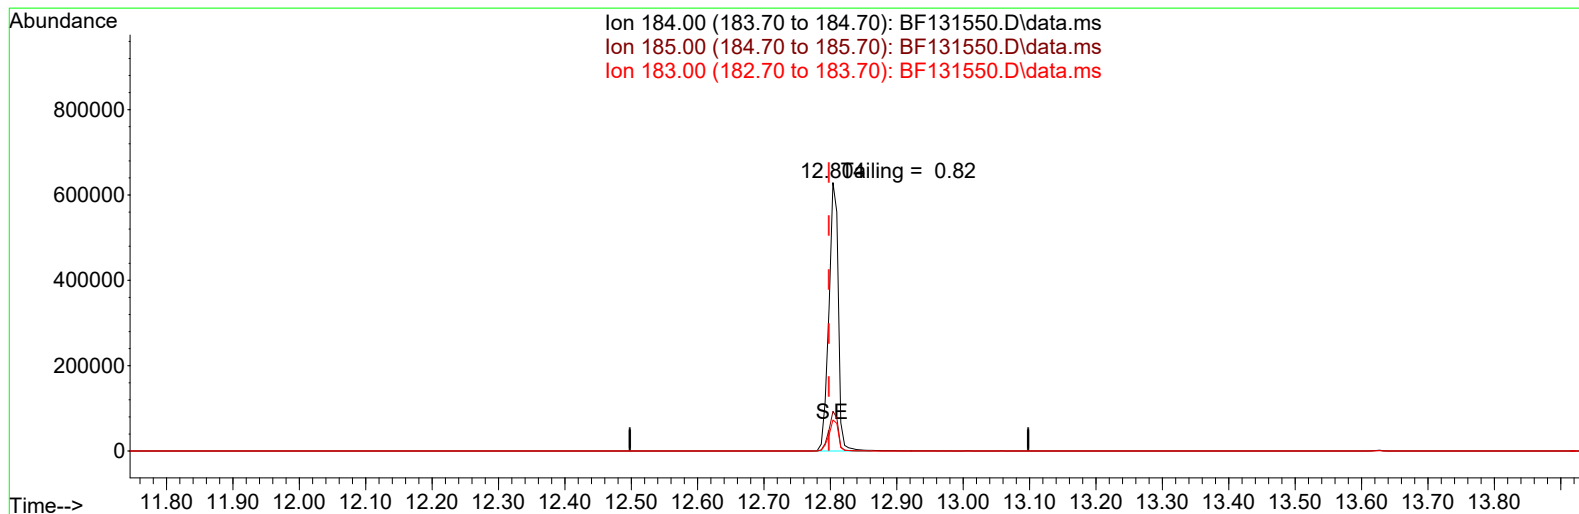

TIC: BF131550.D\data.ms

(77) Benzidine

12.804min (+ 0.006) 0.00 ng

response 624769

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.80
183.00	11.60	11.56
0.00	0.00	0.00