
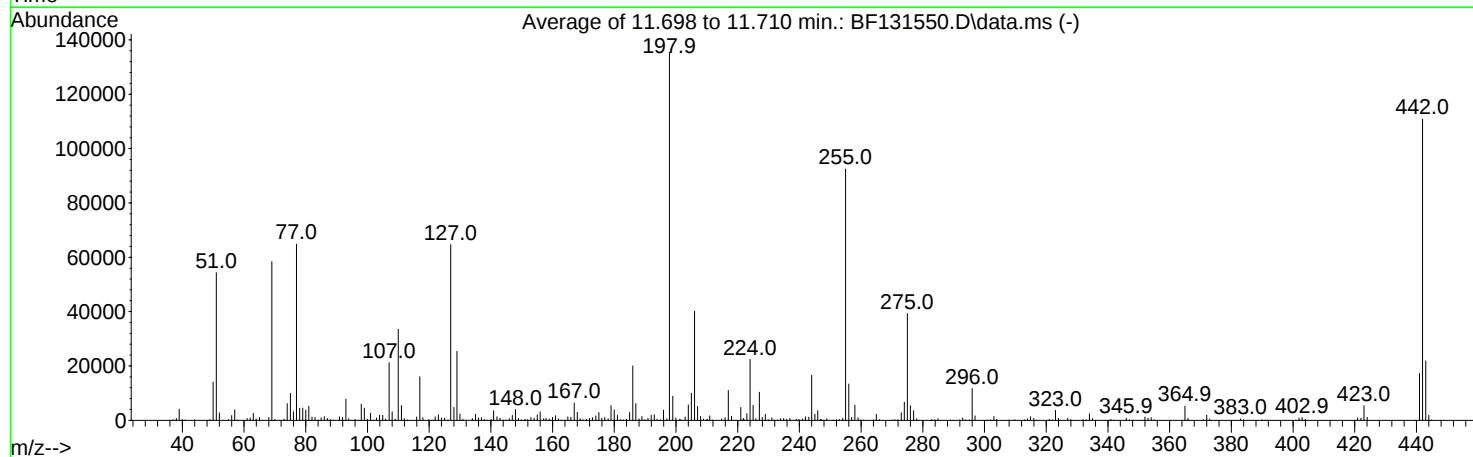


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120822\
Data File : BF131550.D
Acq On : 08 Dec 2022 11:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Dec 09 06:08:27 2022

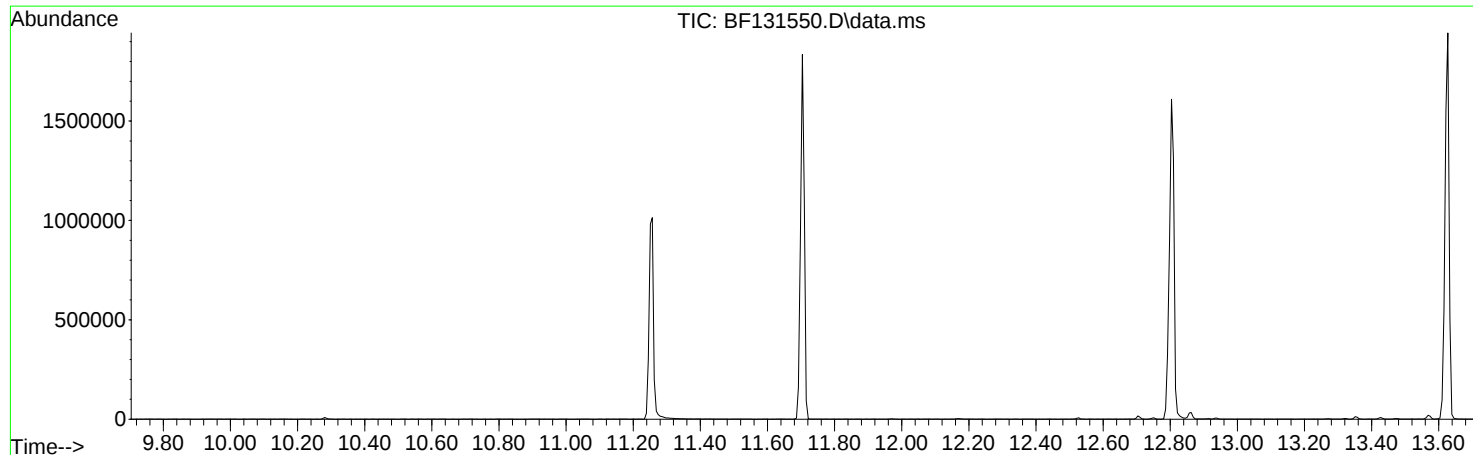




AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.1	54309	PASS
68	69	0.00	2	1.8	1073	PASS
69	198	0.00	100	43.1	58416	PASS
70	69	0.00	2	0.6	345	PASS
127	198	10	80	47.8	64651	PASS
197	198	0.00	2	0.4	564	PASS
198	198	100	100	100.0	135392	PASS
199	198	5	9	6.5	8866	PASS
275	198	10	60	29.0	39323	PASS
365	198	1	100	3.8	5210	PASS
441	198	0.01	100	12.7	17230	PASS
442	442	50	100	100.0	110837	PASS
443	442	15	24	19.8	21891	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120822\
Data File : BF131550.D
Acq On : 08 Dec 2022 11:09
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 09 09:23:04 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 06:08:27 2022
Response via : Initial Calibration

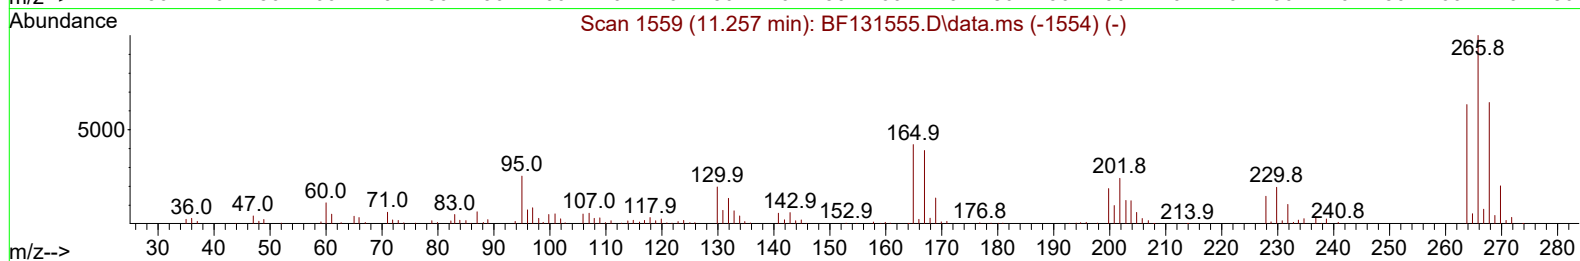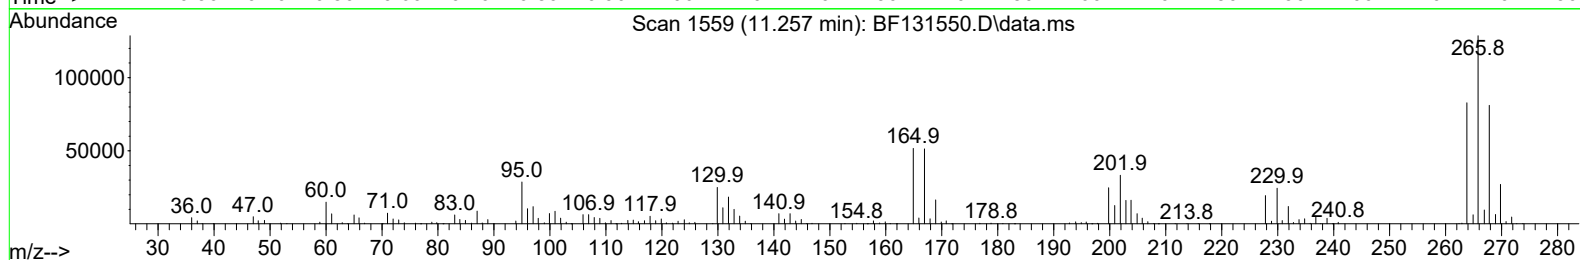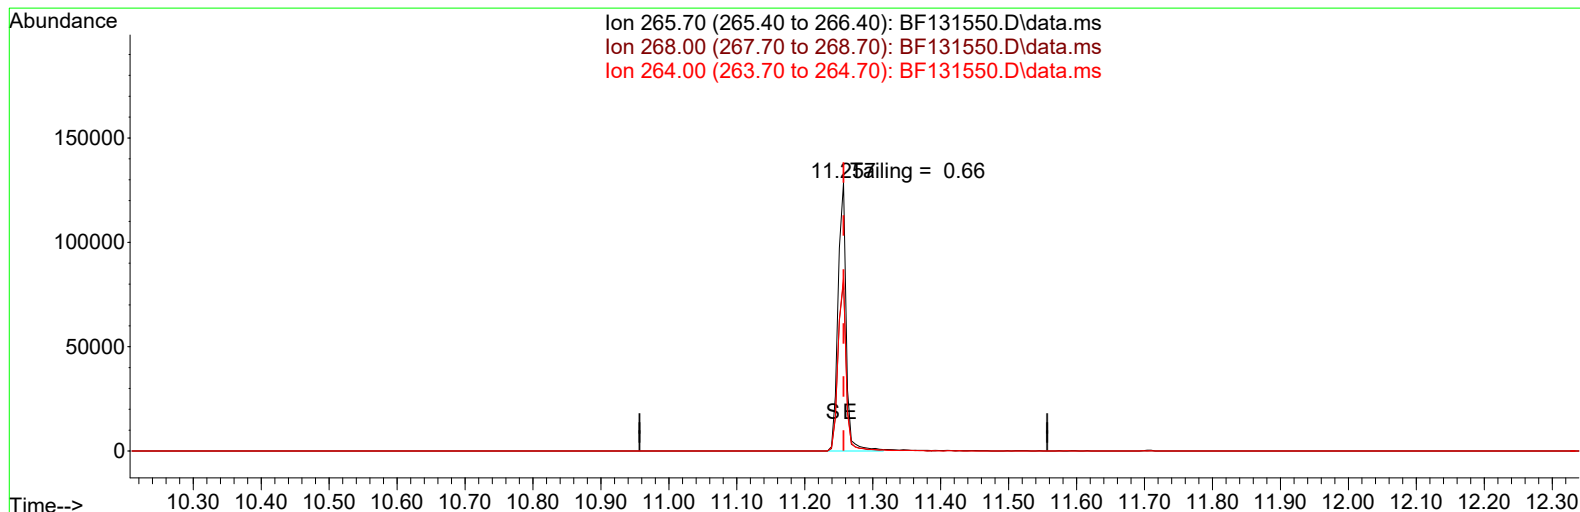

TIC: BF131550.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.000) 23941.32 ng




response 107018

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	63.00
264.00	63.40	64.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120822\
 Data File : BF131550.D
 Acq On : 08 Dec 2022 11:09
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 09 09:23:04 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 09 06:08:27 2022
 Response via : Initial Calibration

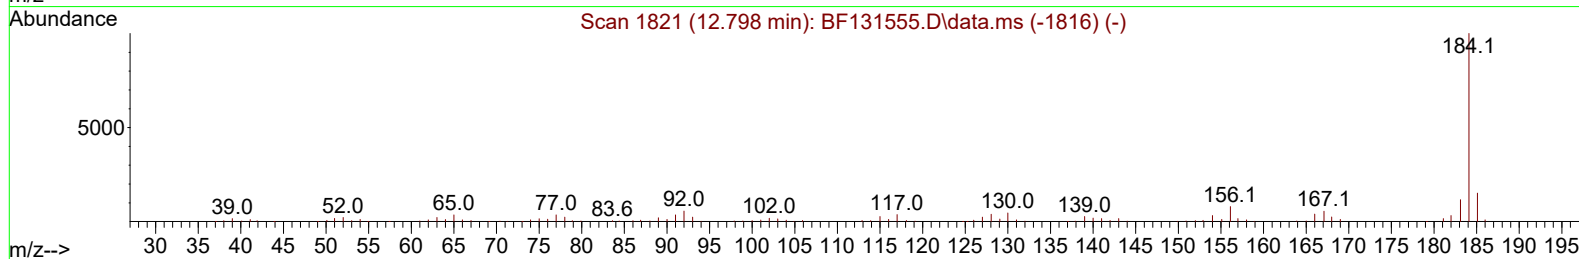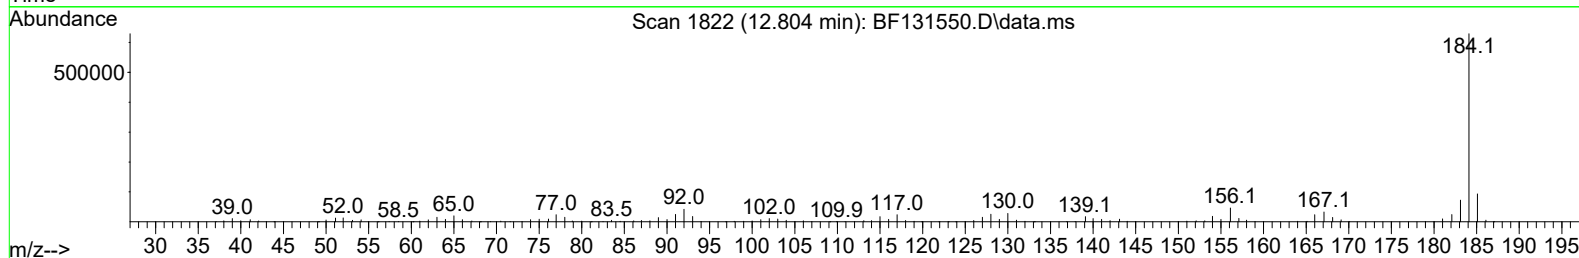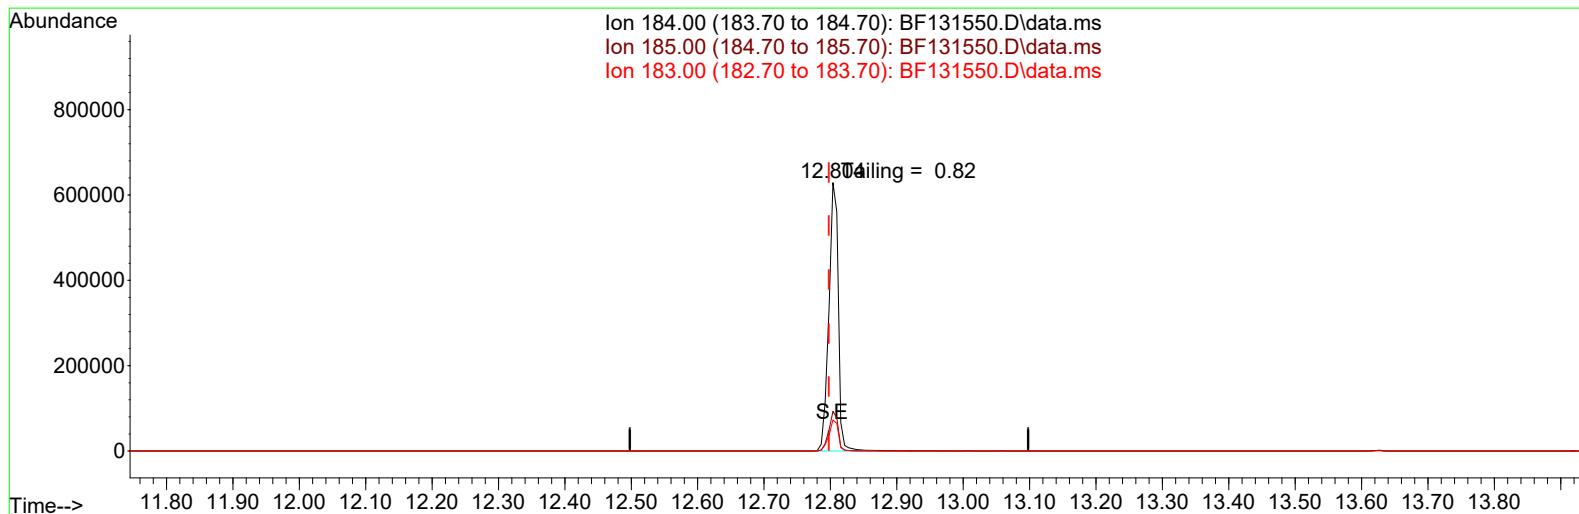

TIC: BF131550.D\data.ms

(77) Benzidine

12.804min (+ 0.006) 0.00 ng

response 624769

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.80
183.00	11.60	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/8/2022	BNA_F	<u>BF131550.D</u>
Compound Name	Response	Retention Time
DDT	312589	13.627
DDD	3178	13.351
DDE	0	12.998
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3178	315767	1.01

Instrument :
BNA_F
ClientSampleId :
DFTPP