
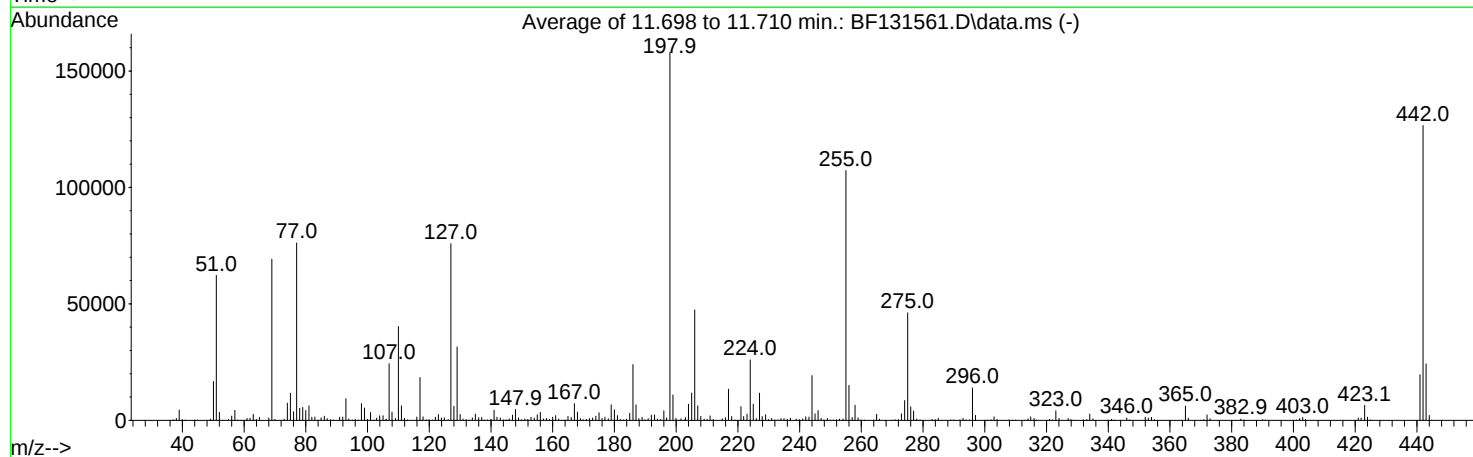


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120922\
 Data File : BF131561.D
 Acq On : 09 Dec 2022 11:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Dec 09 06:08:27 2022

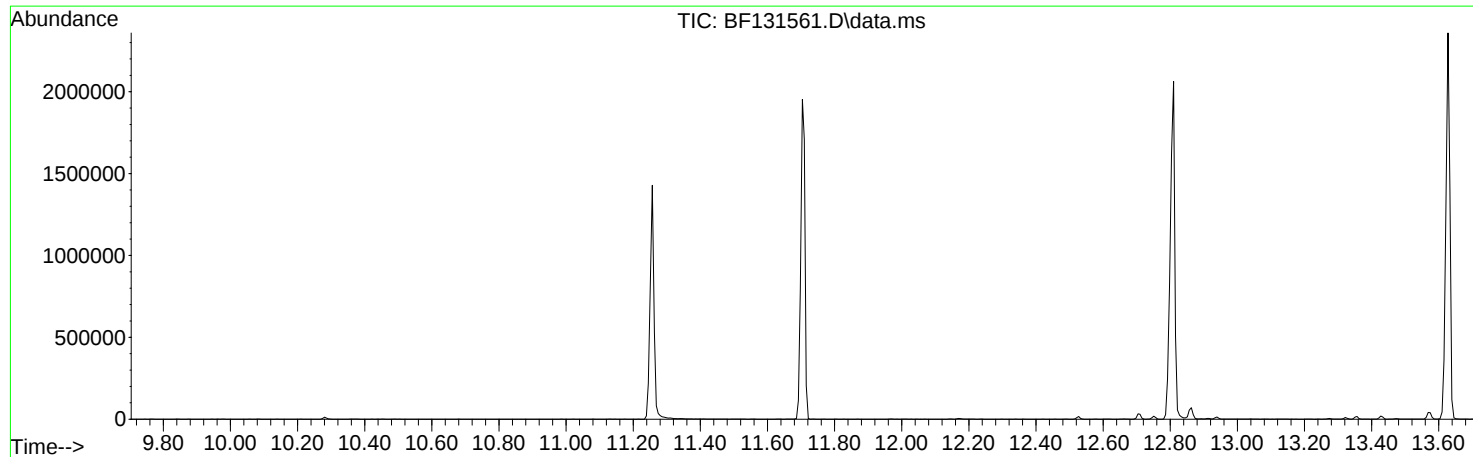




AutoFind: Scans 1634, 1635, 1636; Background Corrected with Scan 1629

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.4	62229	PASS
68	69	0.00	2	1.4	984	PASS
69	198	0.00	100	43.8	69171	PASS
70	69	0.00	2	0.5	379	PASS
127	198	10	80	48.0	75835	PASS
197	198	0.00	2	0.6	999	PASS
198	198	100	100	100.0	158000	PASS
199	198	5	9	6.9	10864	PASS
275	198	10	60	29.2	46123	PASS
365	198	1	100	3.9	6098	PASS
441	198	0.01	100	12.4	19636	PASS
442	442	50	100	100.0	126645	PASS
443	442	15	24	19.1	24219	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120922\
Data File : BF131561.D
Acq On : 09 Dec 2022 11:24
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 10 07:57:23 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Dec 09 06:08:27 2022
Response via : Initial Calibration

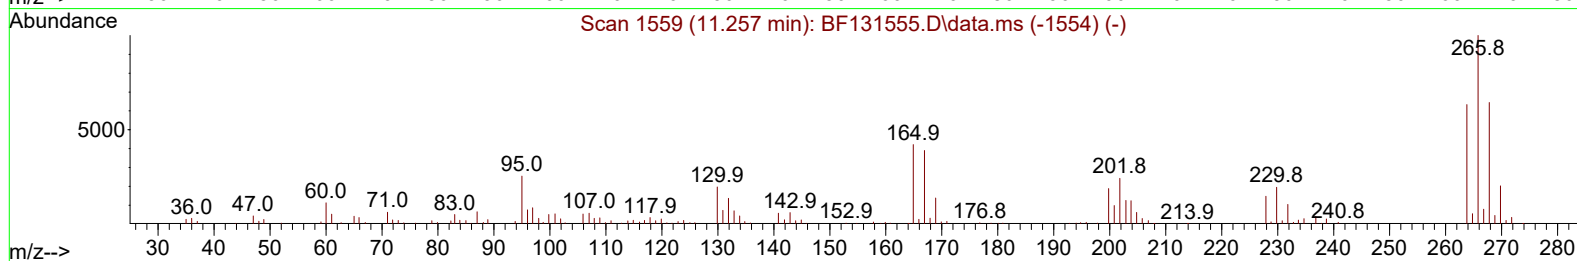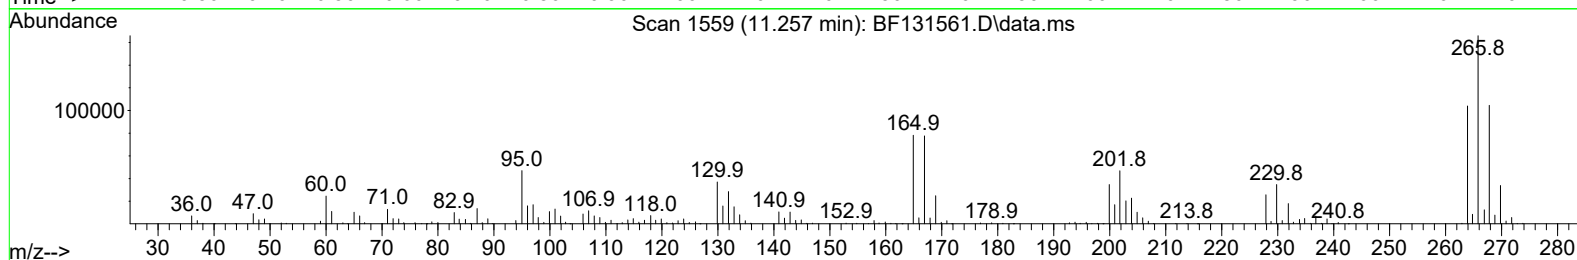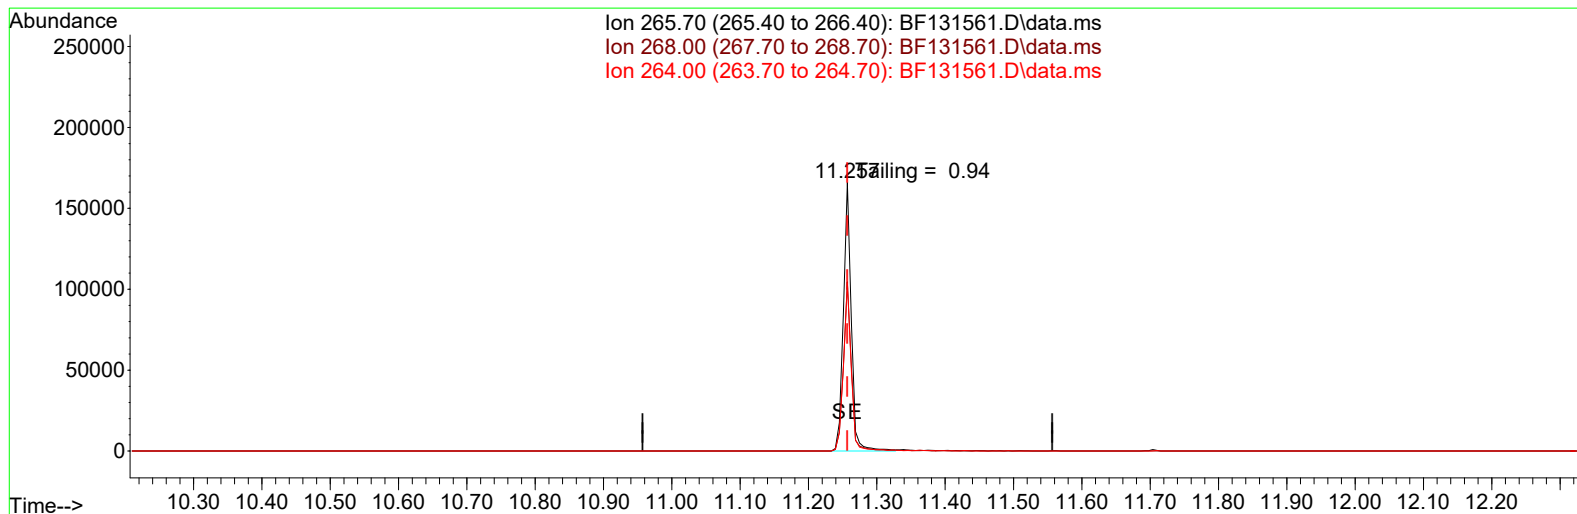

TIC: BF131561.D\data.ms

(70) Pentachlorophenol (C)

11.257min (-0.000) 24640.80 ng




response 132915

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.40	62.98
264.00	63.40	62.72
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF120922\
 Data File : BF131561.D
 Acq On : 09 Dec 2022 11:24
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 10 07:57:23 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF120822.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Dec 09 06:08:27 2022
 Response via : Initial Calibration

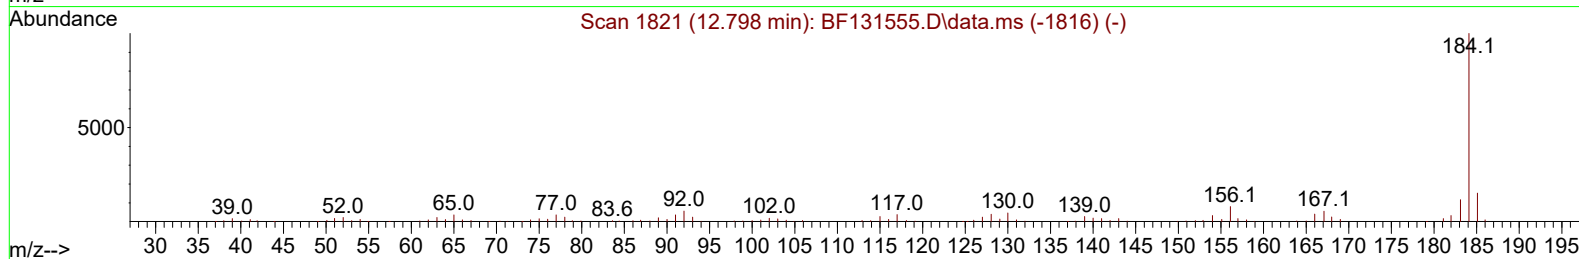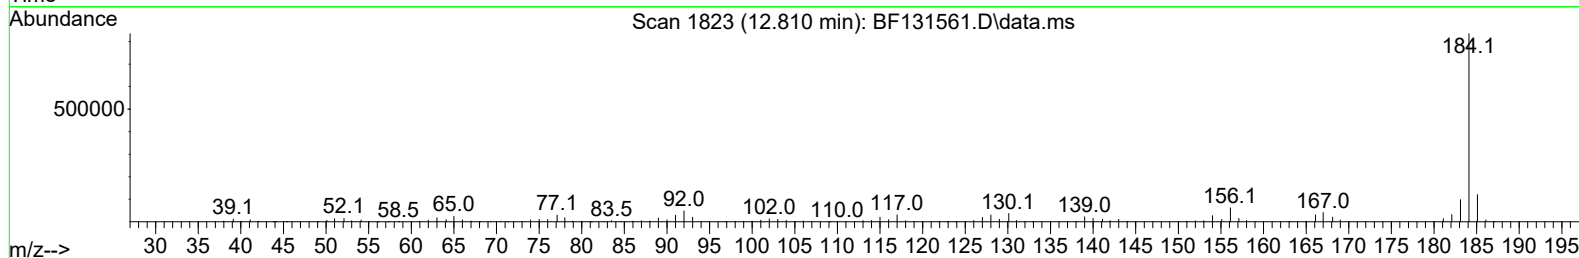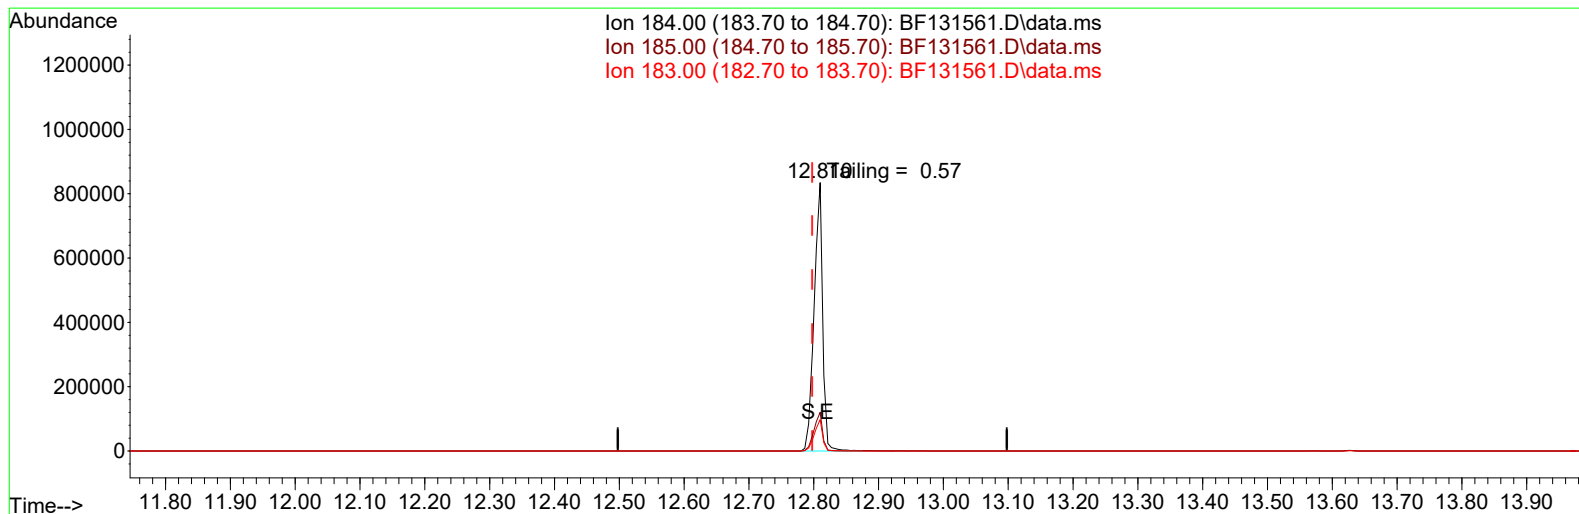

TIC: BF131561.D\data.ms

(77) Benzidine

12.810min (+ 0.012) 0.00 ng

response 768075

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	15.20	14.47
183.00	11.60	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/9/2022	BNA_F	<u>BF131561.D</u>
Compound Name	Response	Retention Time
DDT	370811	13.627
DDD	5052	13.357
DDE	56	12.98
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5108	375919	1.36

Instrument :
BNA_F
ClientSampleId :
DFTPP