
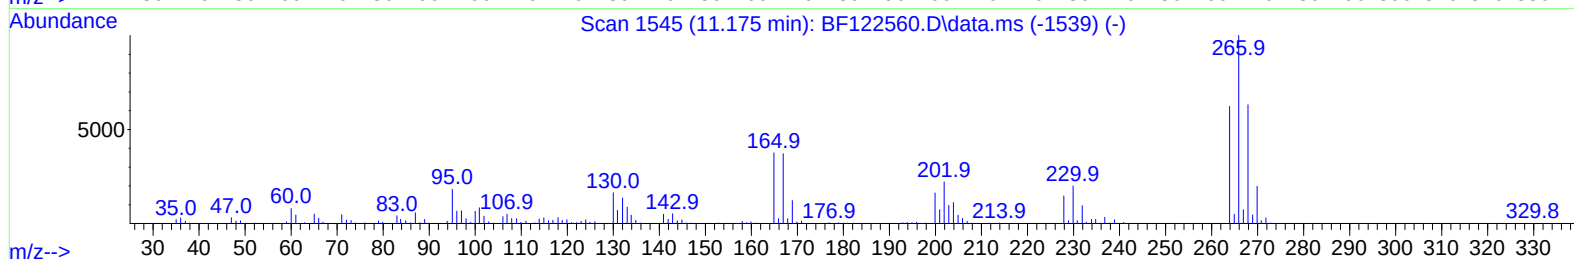
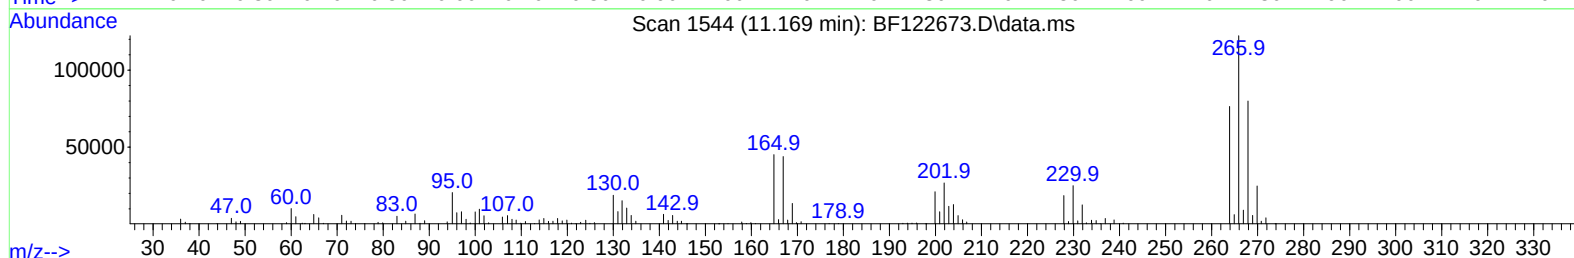


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\  
Data File : BF122673.D  
Acq On    : 12 Dec 2020  11:42  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 15 08:45:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

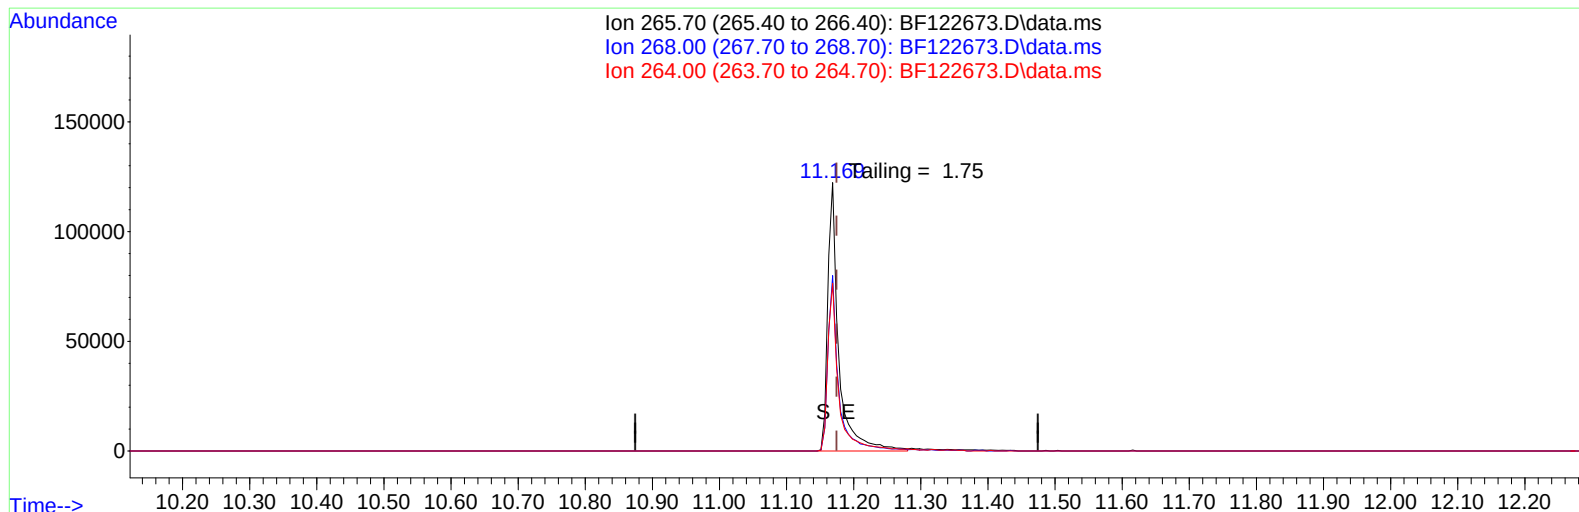

TIC: BF122673.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.006) 55218.05 ng

response 140240

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	63.10	65.36
--------	-------	-------

264.00	62.30	62.49
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
Data File : BF122673.D
Acq On : 12 Dec 2020 11:42
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 15 08:45:17 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Dec 07 12:08:49 2020
Response via : Initial Calibration

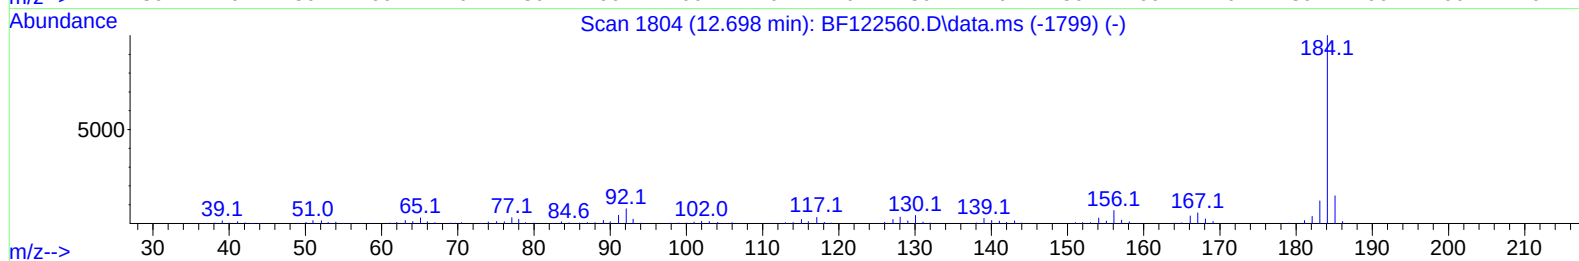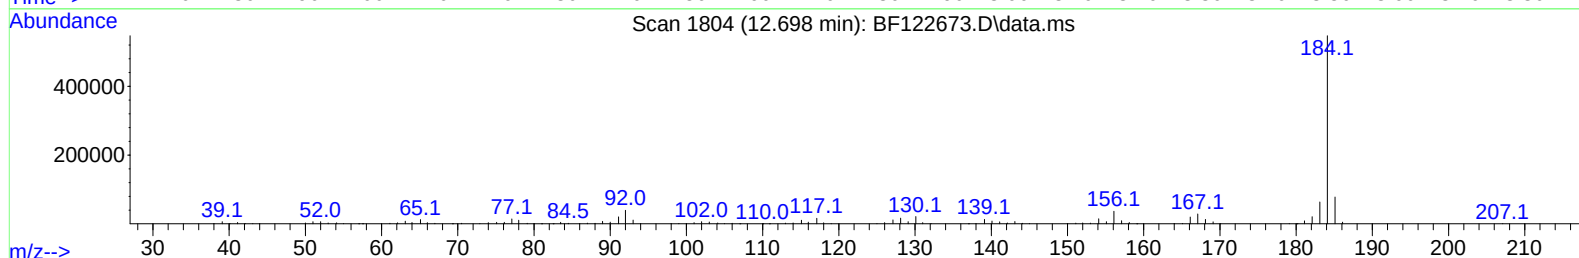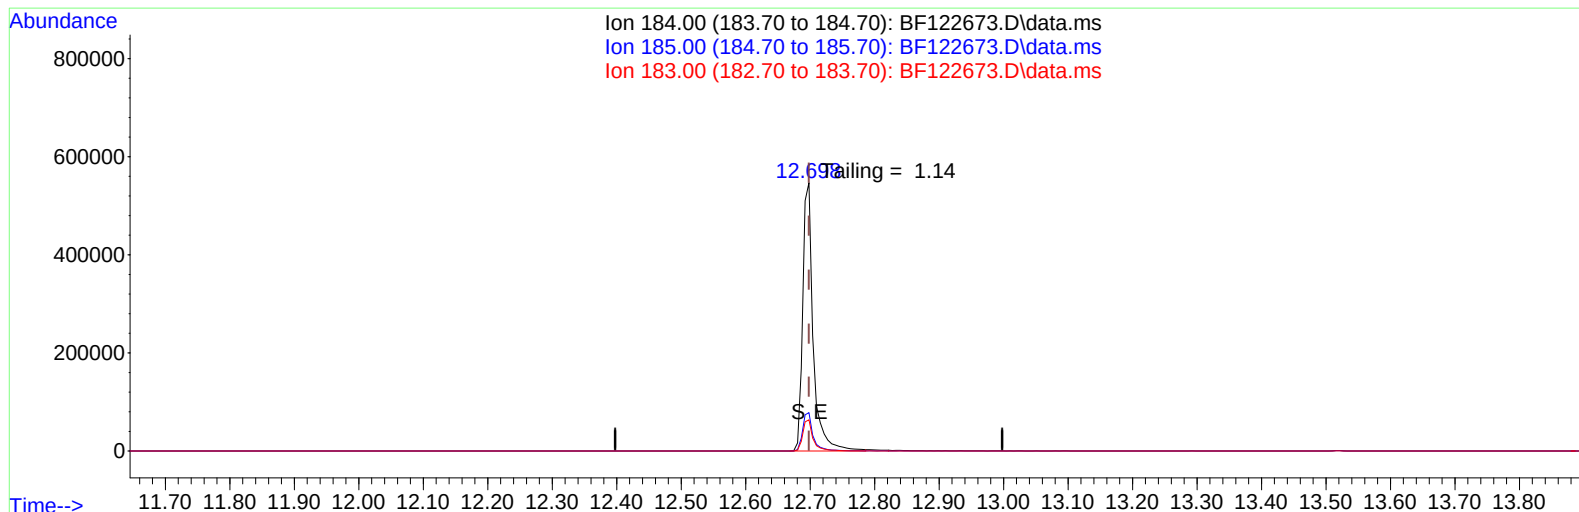

TIC: BF122673.D\data.ms

(77) Benzidine

12.698min (+ 0.000) 0.00 ng

response 627353

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.30
183.00	12.10	11.61
0.00	0.00	0.00