

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
 Data File : BF122680.D
 Acq On : 12 Dec 2020 16:08
 Operator : JU/CG
 Sample : L5043-02
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KENS-SS1-121020-0-7

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122680.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.122	3	6	11	rVB	35363	44311	1.38%	0.199%
2	5.457	568	573	576	rBV	2829366	2590384	80.90%	11.620%
3	6.469	740	745	761	rBV	2565242	2831175	88.42%	12.700%
4	6.669	776	779	792	rBV	22084	34003	1.06%	0.153%
5	6.834	804	807	811	rBV	977072	771178	24.09%	3.459%
6	7.398	898	903	906	rBV	1895264	1721014	53.75%	7.720%
7	8.122	1021	1026	1041	rBV	1009356	1020997	31.89%	4.580%
8	9.192	1204	1208	1219	rBV	3191676	3201852	100.00%	14.363%
9	9.586	1272	1275	1285	rBV	222795	219448	6.85%	0.984%
10	9.875	1319	1324	1334	rVB	1392690	1201461	37.52%	5.389%
11	10.663	1454	1458	1469	rBV	1871548	1739051	54.31%	7.801%
12	11.357	1572	1576	1588	rBV	1275472	1239124	38.70%	5.558%
13	11.886	1658	1666	1670	rBV3	22599	36859	1.15%	0.165%
14	12.674	1795	1800	1807	rBV	52629	91444	2.86%	0.410%
15	12.945	1841	1846	1849	rBV	3423681	3074528	96.02%	13.792%
16	13.421	1919	1927	1932	rBV	104711	176396	5.51%	0.791%
17	13.857	1996	2001	2002	rBV	34235	33483	1.05%	0.150%
18	13.874	2002	2004	2019	rVV6	40780	118436	3.70%	0.531%
19	13.998	2021	2025	2035	rVB	1198738	1126104	35.17%	5.051%
20	14.751	2150	2153	2160	rBV3	62897	90826	2.84%	0.407%
21	15.462	2268	2274	2281	rBV	685470	930756	29.07%	4.175%

Sum of corrected areas: 22292830

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
Data File : BF122680.D
Acq On : 12 Dec 2020 16:08
Operator : JU/CG
Sample : L5043-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KENS-SS1-121020-0-7










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 9-Octadecenamide, (Z)- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.421	3.13 ng	176396	Chrysene-d12	13.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			9-Octadecenamide, (Z)-	281	C18H35NO	000301-02-0	98
2			7-Nonenamide	155	C9H17NO	090949-53-4	64
3			Hexadecanamide	255	C16H33NO	000629-54-9	64
4			Octanamide	143	C8H17NO	000629-01-6	53
5			Benzeneethanamine, 2-fluoro-.bet...	229	C11H16FN03	061338-98-5	53

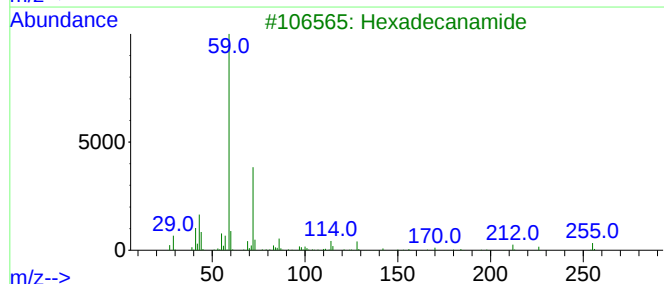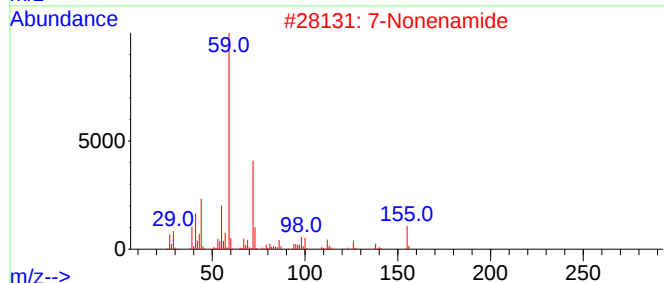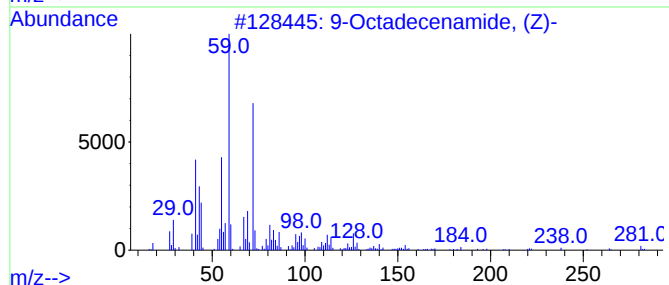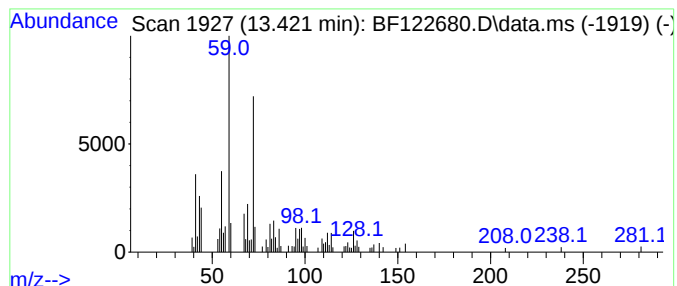

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
Data File : BF122680.D
Acq On : 12 Dec 2020 16:08
Operator : JU/CG
Sample : L5043-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KENS-SS1-121020-0-7










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 unknown13.874 Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.874	2.10 ng	118436	Chrysene-d12	13.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Sulfurous acid, butyl tridecyl e...	320	C17H36O3S	1000309-18-0	35
2			Decyl trifluoroacetate	254	C12H21F3O2	000333-88-0	27
3			Sulfurous acid, butyl dodecyl ester	306	C16H34O3S	1000309-17-9	25
4			n-Nonadecanol-1	284	C19H40O	001454-84-8	22
5			1-Hexadecanol	242	C16H34O	036653-82-4	22

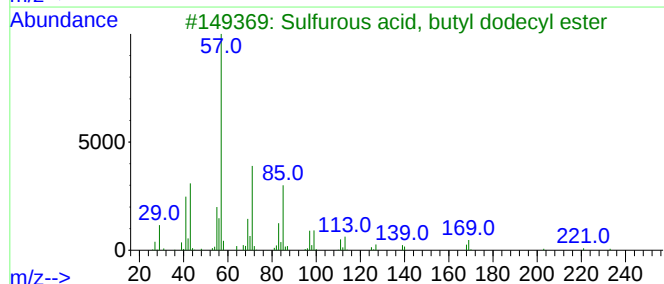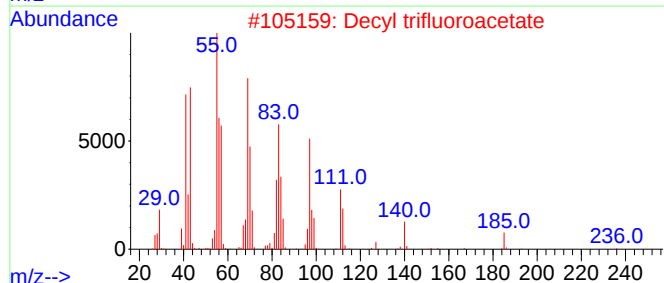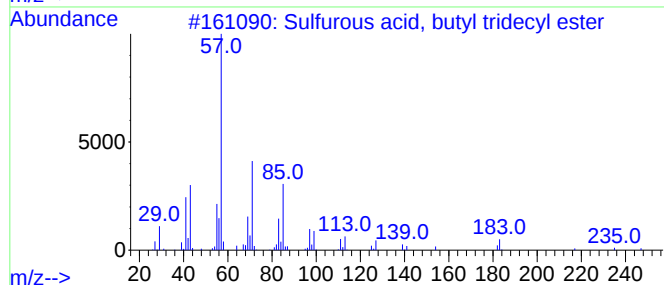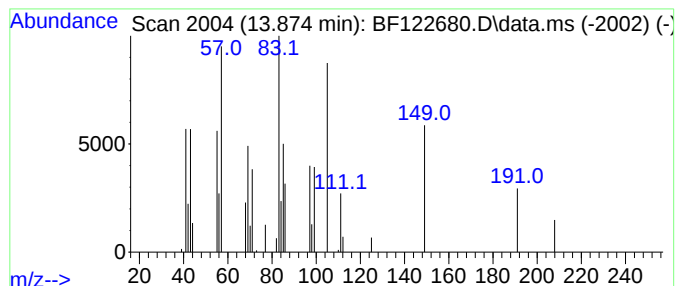

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
Data File : BF122680.D
Acq On : 12 Dec 2020 16:08
Operator : JU/CG
Sample : L5043-02
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KENS-SS1-121020-0-7

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
9-Octadecenamid...	13.421	3.1	ng	176396	5	13.998	1126100	20.0
unknown13.874	13.874	2.1	ng	118436	5	13.998	1126100	20.0