

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
 Data File : BF122684.D
 Acq On : 12 Dec 2020 18:12
 Operator : JU/CG
 Sample : L5043-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 KENS-SS-121020-BD

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF122684.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.134	4	8	14	rVB	60098	82469	1.77%	0.264%
2	5.463	568	574	577	rBV	3571860	3779829	81.27%	12.120%
3	6.469	739	745	762	rBV	3321264	4151949	89.27%	13.313%
4	6.669	776	779	792	rBV	55154	78190	1.68%	0.251%
5	6.834	804	807	811	rBV	1102003	865776	18.61%	2.776%
6	7.398	898	903	906	rBV	2426017	2541176	54.64%	8.148%
7	8.116	1021	1025	1043	rVB	1159689	1145740	24.63%	3.674%
8	9.198	1203	1209	1212	rBV	4195414	4411991	94.86%	14.147%
9	9.586	1271	1275	1285	rBV	264667	249410	5.36%	0.800%
10	9.875	1319	1324	1336	rVB	1487354	1364340	29.33%	4.375%
11	10.663	1453	1458	1469	rBV	3035767	3003693	64.58%	9.631%
12	11.357	1572	1576	1585	rBV	1507673	1427877	30.70%	4.578%
13	11.886	1662	1666	1670	rBV	41365	52421	1.13%	0.168%
14	12.674	1795	1800	1813	rBV3	48269	87528	1.88%	0.281%
15	12.945	1841	1846	1850	rBV	4500608	4651022	100.00%	14.913%
16	13.421	1923	1927	1939	rBV	85842	115753	2.49%	0.371%
17	13.857	1995	2001	2014	rBV2	198987	690199	14.84%	2.213%
18	13.998	2021	2025	2032	rVB	1449262	1317746	28.33%	4.225%
19	15.462	2268	2274	2285	rBV	848216	1110899	23.89%	3.562%
20	16.033	2363	2371	2374	rBV7	23432	59086	1.27%	0.189%




Sum of corrected areas: 31187094

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
Data File : BF122684.D
Acq On : 12 Dec 2020 18:12
Operator : JU/CG
Sample : L5043-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KENS-SS-121020-BD

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

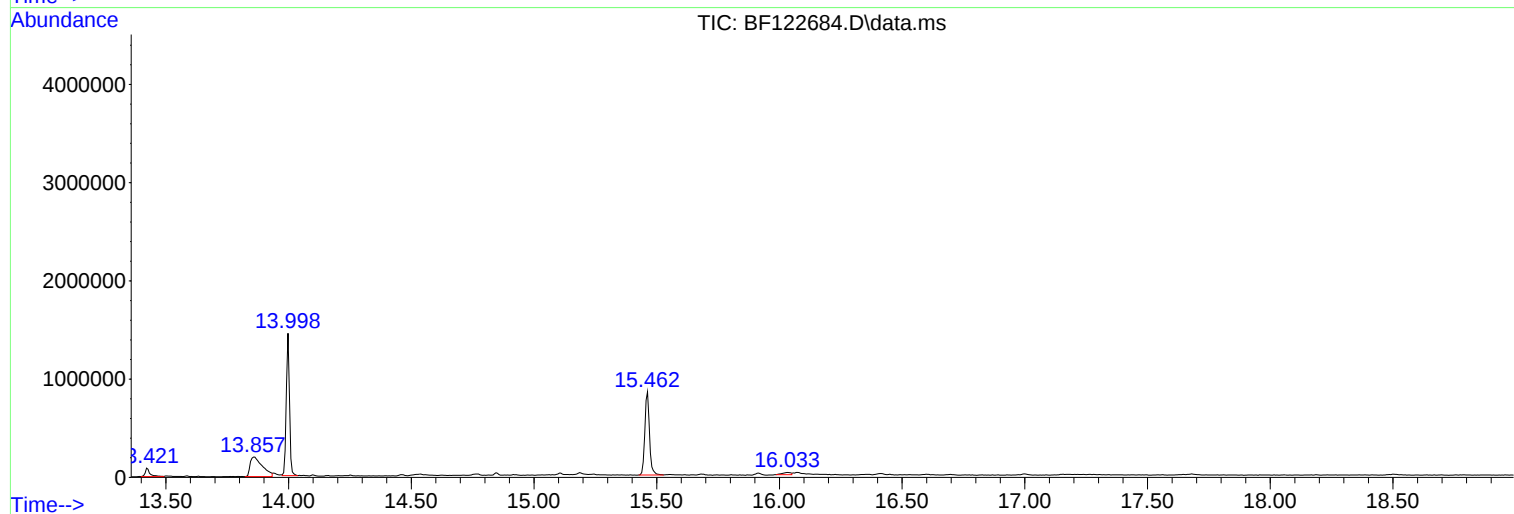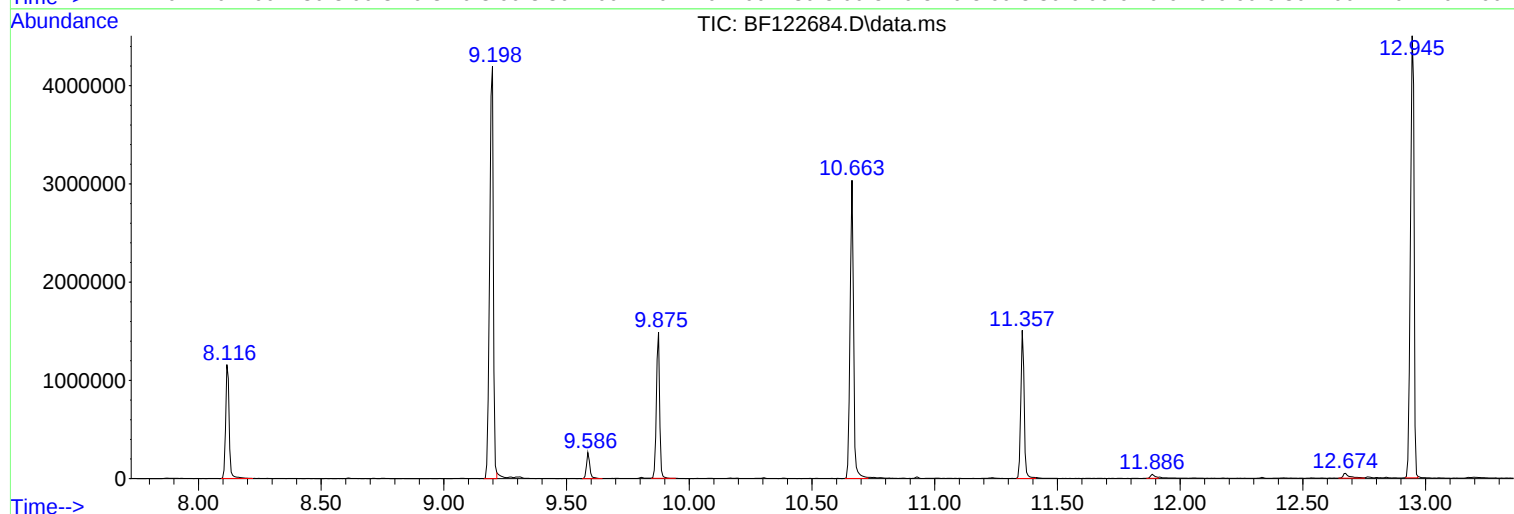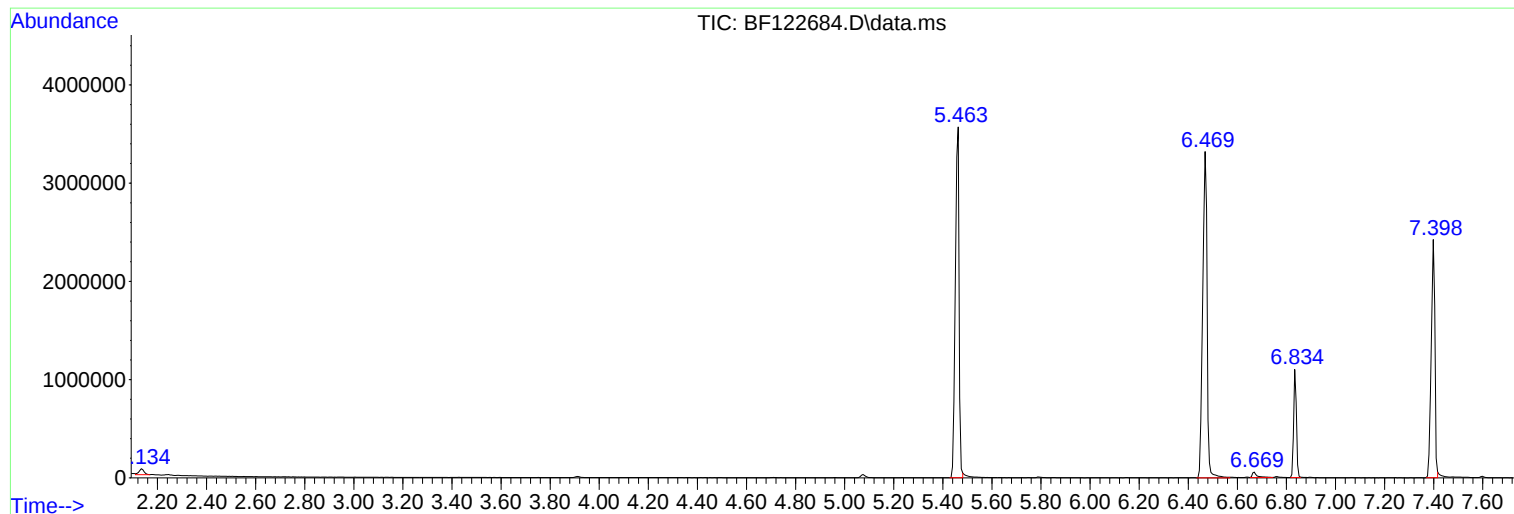

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
Data File : BF122684.D
Acq On : 12 Dec 2020 18:12
Operator : JU/CG
Sample : L5043-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KENS-SS-121020-BD










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Dichloroacetic acid, heptad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.857	10.48 ng	690199	Chrysene-d12	13.998

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Dichloroacetic acid, heptadecyl ...	366	C19H36Cl2O2	1000282-98-2	95
2			n-Nonadecanol-1	284	C19H40O	001454-84-8	95
3			1-Heneicosanol	312	C21H44O	015594-90-8	95
4			Behenic alcohol	326	C22H46O	000661-19-8	95
5			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94

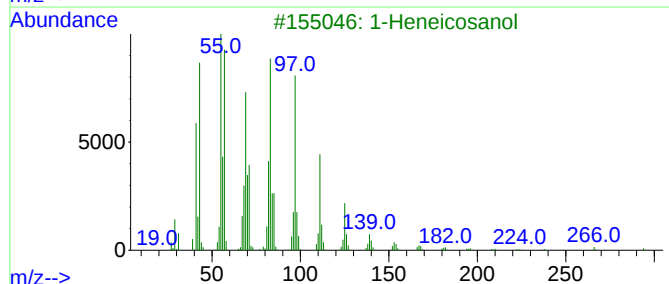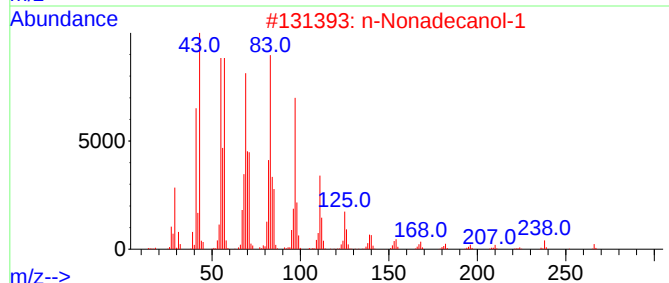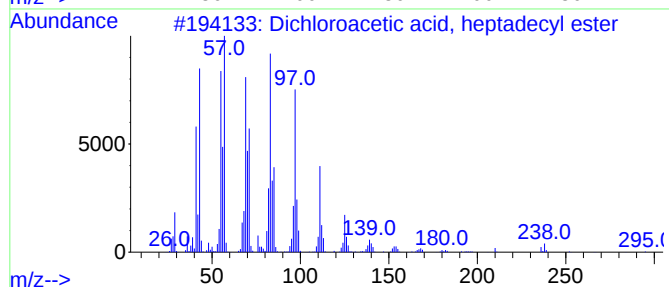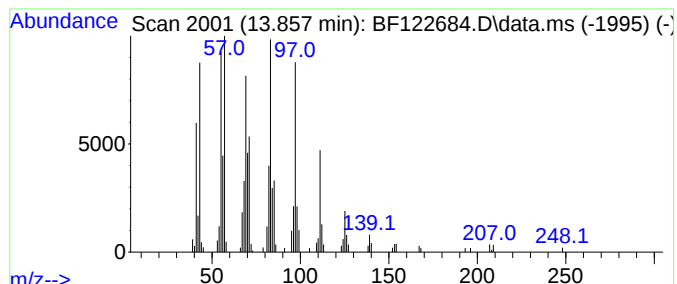

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
Data File : BF122684.D
Acq On : 12 Dec 2020 18:12
Operator : JU/CG
Sample : L5043-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
KENS-SS-121020-BD

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Dichloroacetic ...	13.857	10.5	ng	690199	5	13.998	1317750	20.0