


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121220\
 Data File : BF122673.D
 Acq On : 12 Dec 2020 11:42
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF120520.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Dec 15 18:14:23 2020

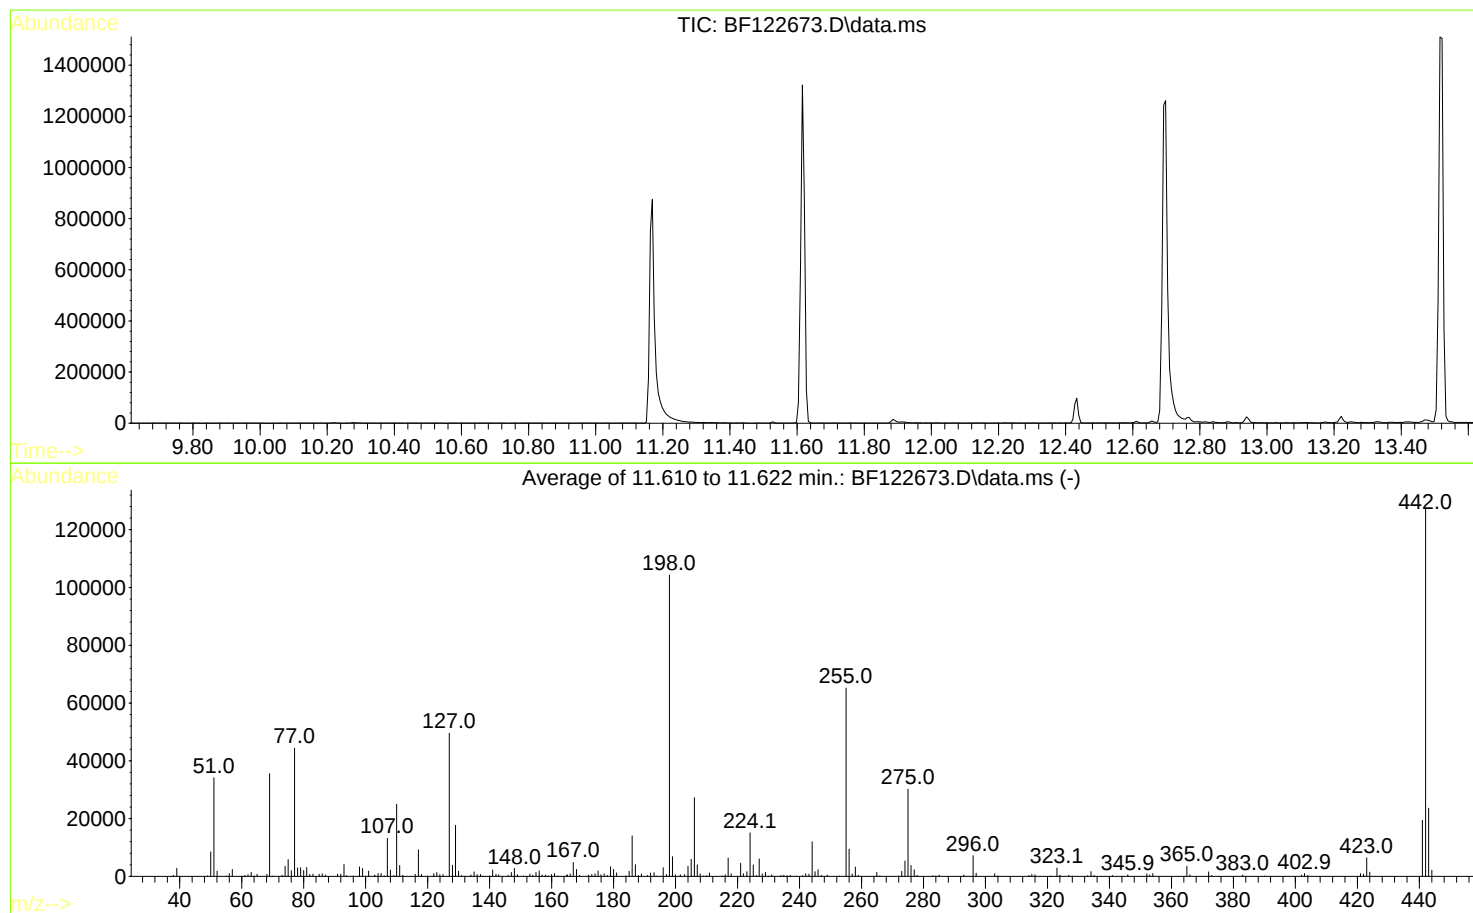

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.7	34096	PASS
68	69	0.00	2	2.0	710	PASS
69	198	0.00	100	34.1	35547	PASS
70	69	0.00	2	0.4	125	PASS
127	198	10	80	47.5	49573	PASS
197	198	0.00	2	0.6	595	PASS
198	198	100	100	100.0	104291	PASS
199	198	5	9	6.6	6839	PASS
275	198	10	60	28.9	30181	PASS
365	198	1	100	3.4	3509	PASS
441	198	0.01	100	18.7	19462	PASS
442	442	100	100	100.0	127339	PASS
443	442	15	24	18.5	23585	PASS