
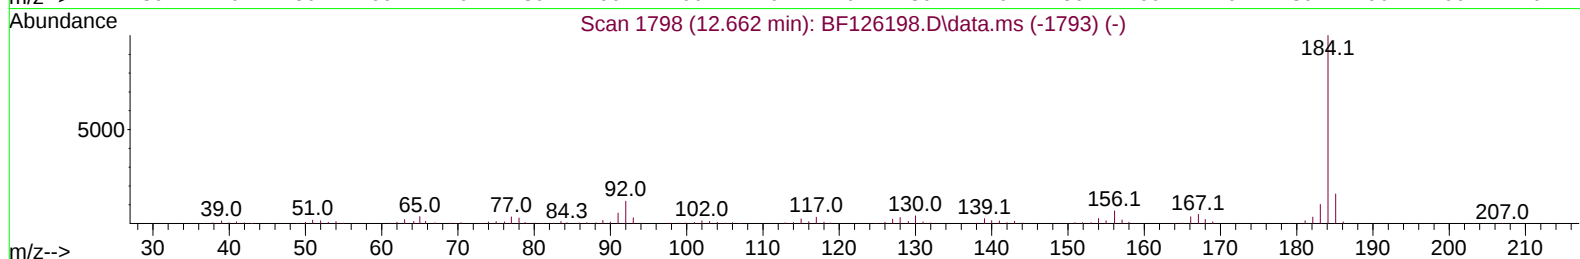
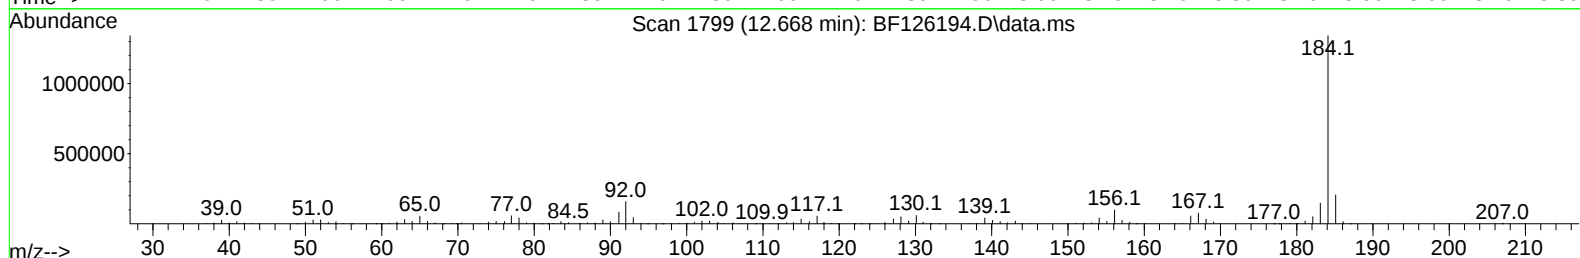


```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121521\  
Data File : BF126194.D  
Acq On    : 15 Dec 2021  14:38  
Operator  : JU/CG  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Quant Time: Dec 16 12:48:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

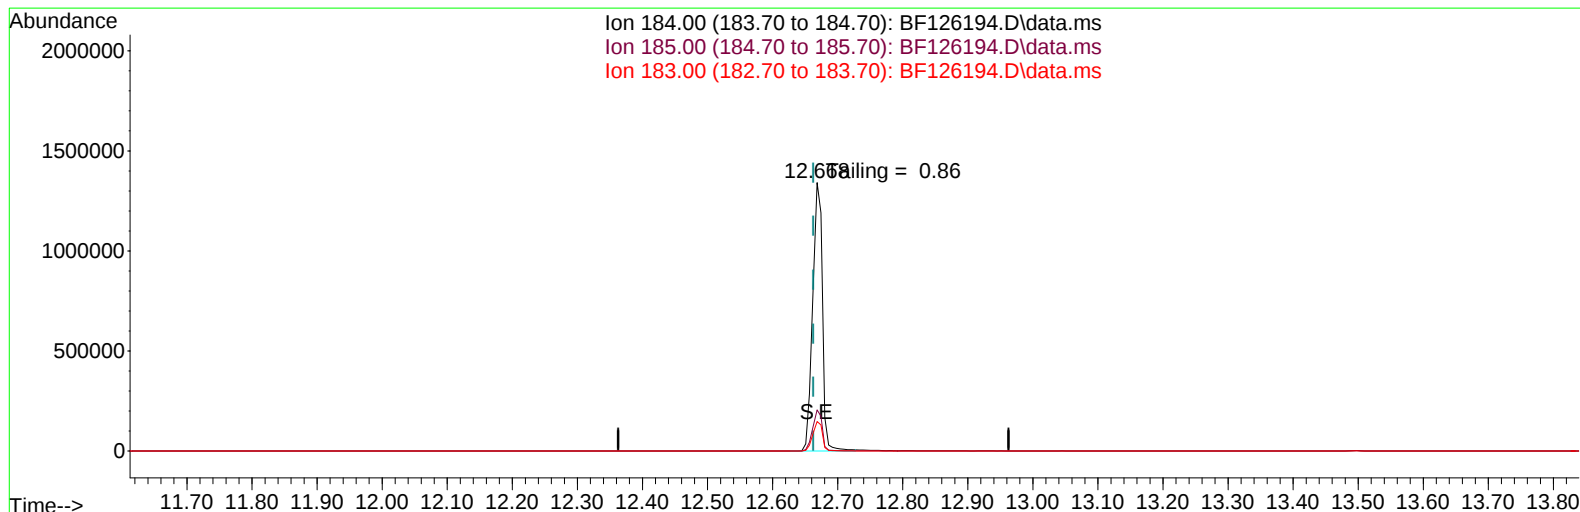

TIC: BF126194.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 0.00 ng

response **1412916**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	15.32
183.00	10.10	10.99
0.00	0.00	0.00