
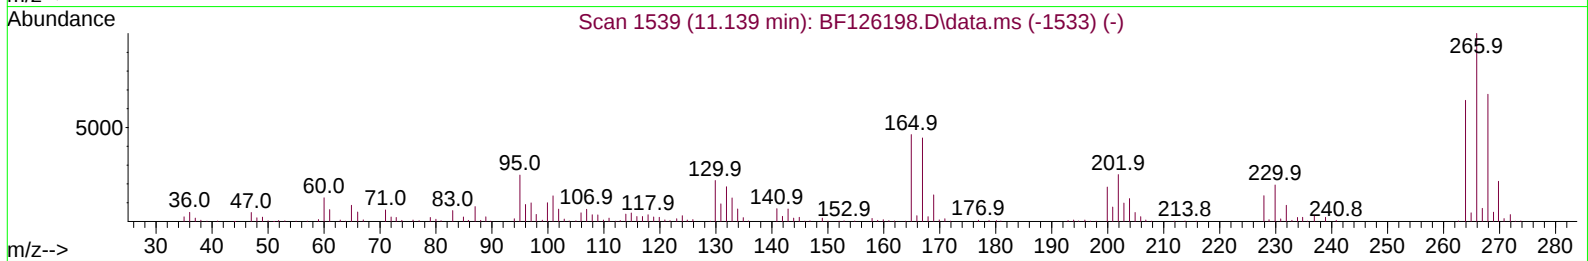
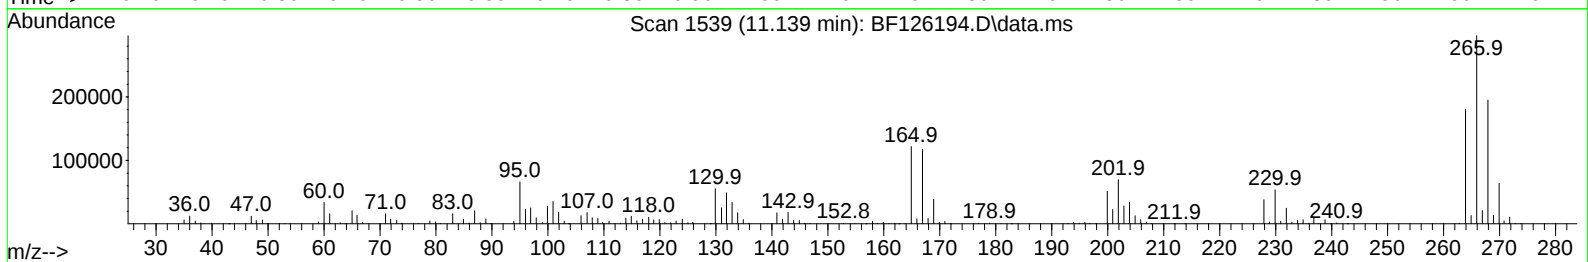


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121521\
 Data File : BF126194.D
 Acq On : 15 Dec 2021 14:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 12:48:06 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

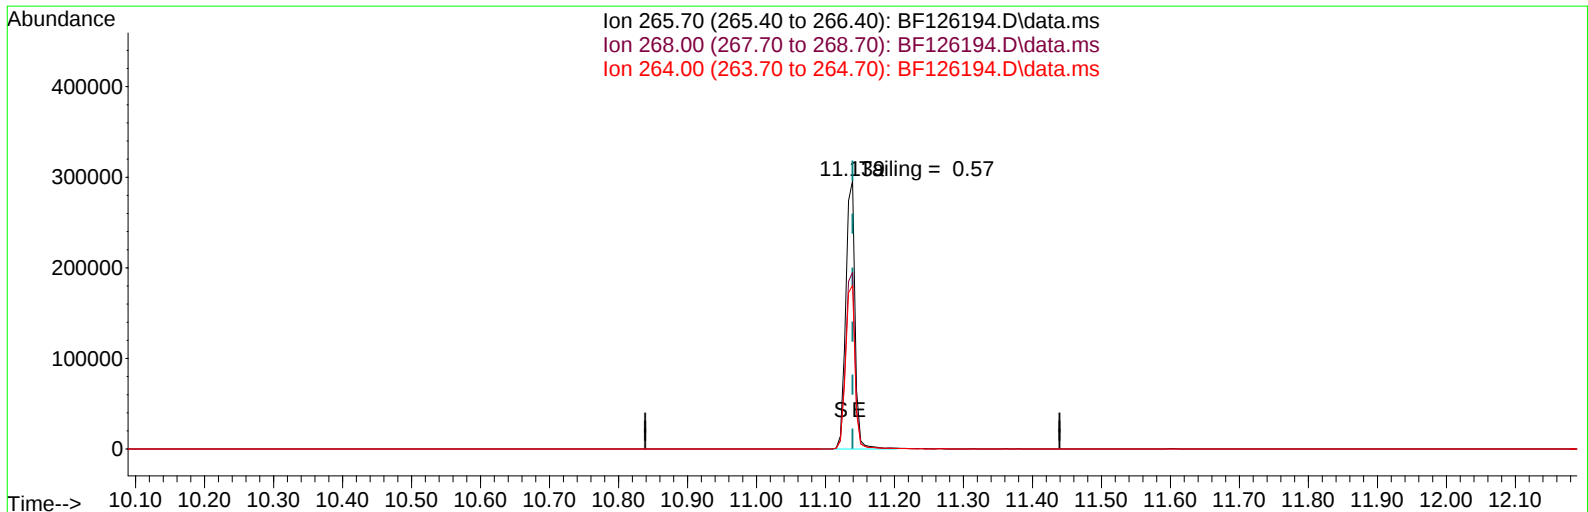

TIC: BF126194.D\data.ms

(70) Pentachlorophenol (C)




11.139min (+ 0.000) 41241.18 ng

response 275858

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.80
264.00	69.90	60.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121521\
 Data File : BF126194.D
 Acq On : 15 Dec 2021 14:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 12:48:06 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

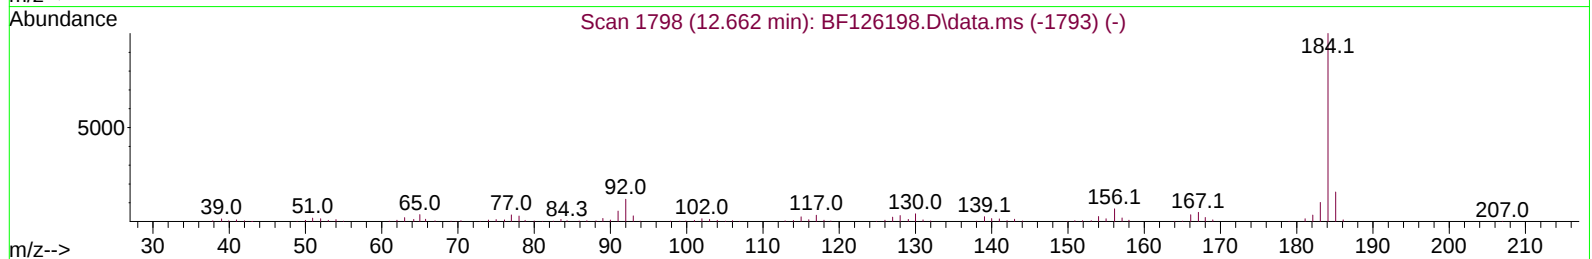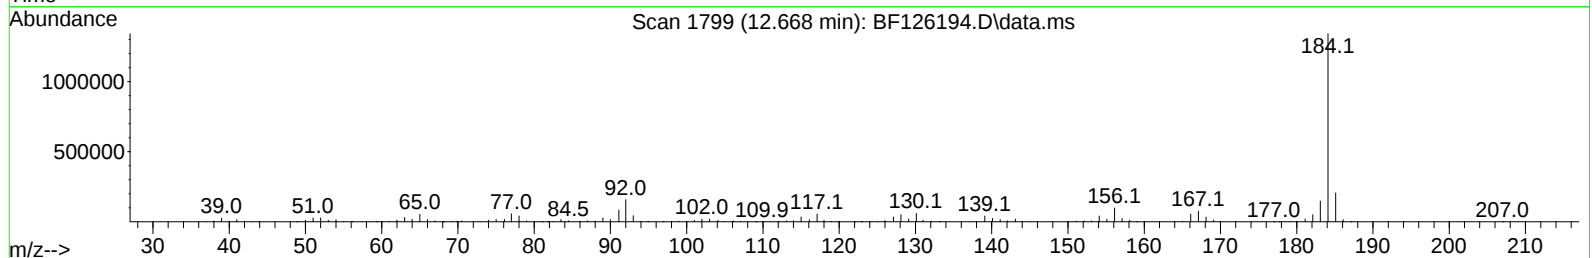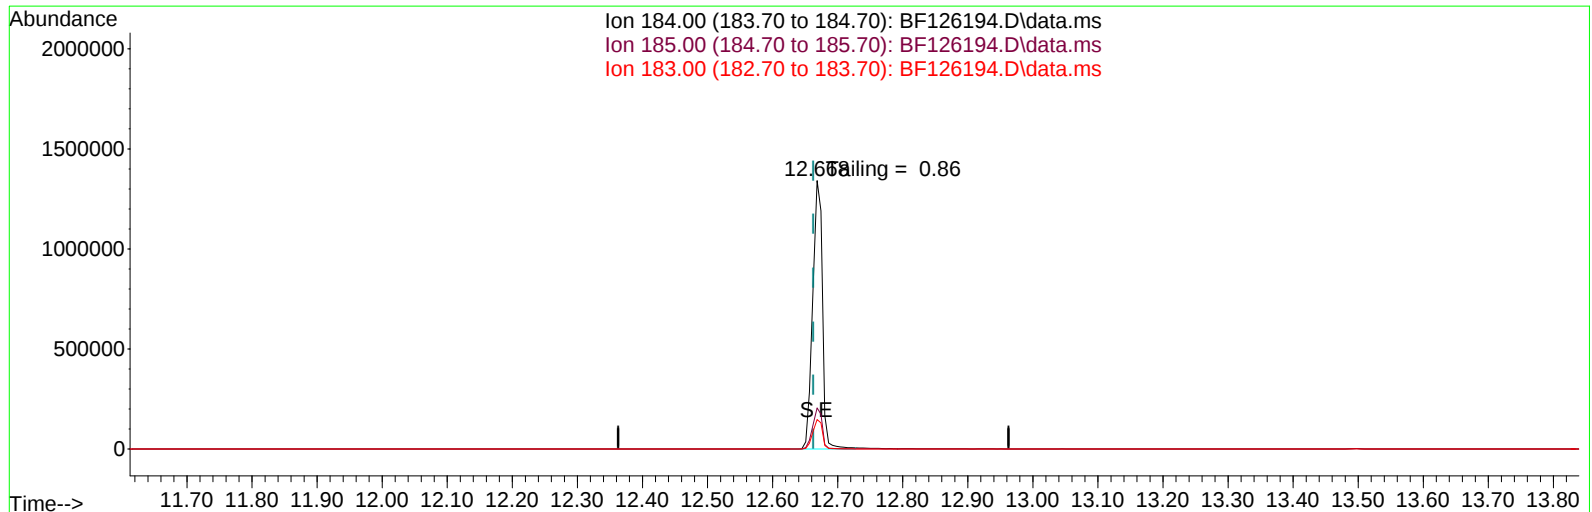

TIC: BF126194.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 0.00 ng

response 1412916

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	15.32
183.00	10.10	10.99
0.00	0.00	0.00