
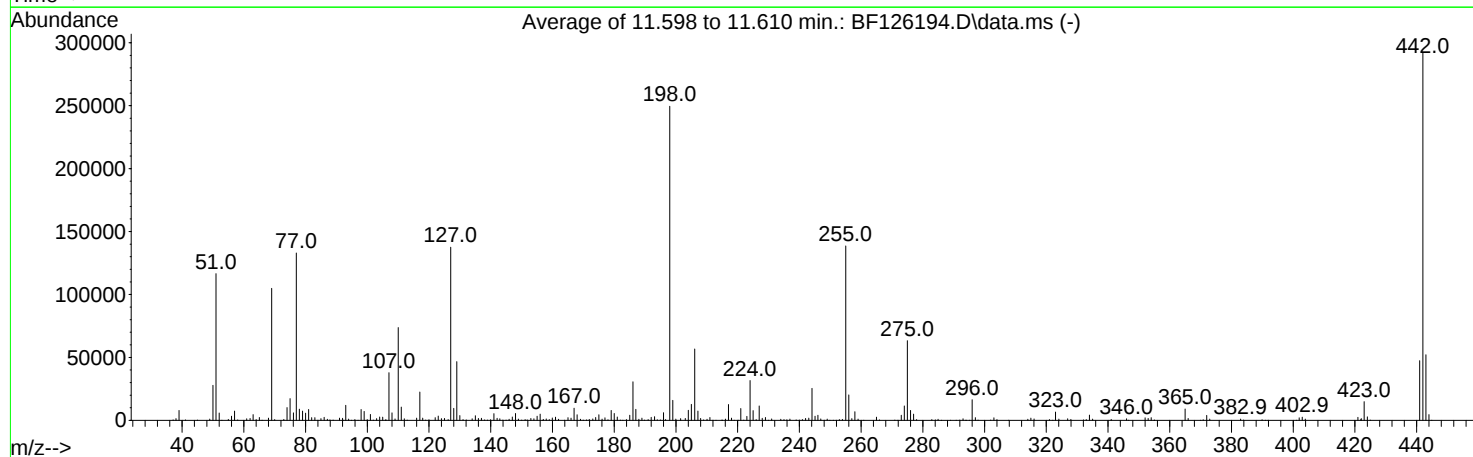


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121521\
 Data File : BF126194.D
 Acq On : 15 Dec 2021 14:38
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 16 12:22:48 2021

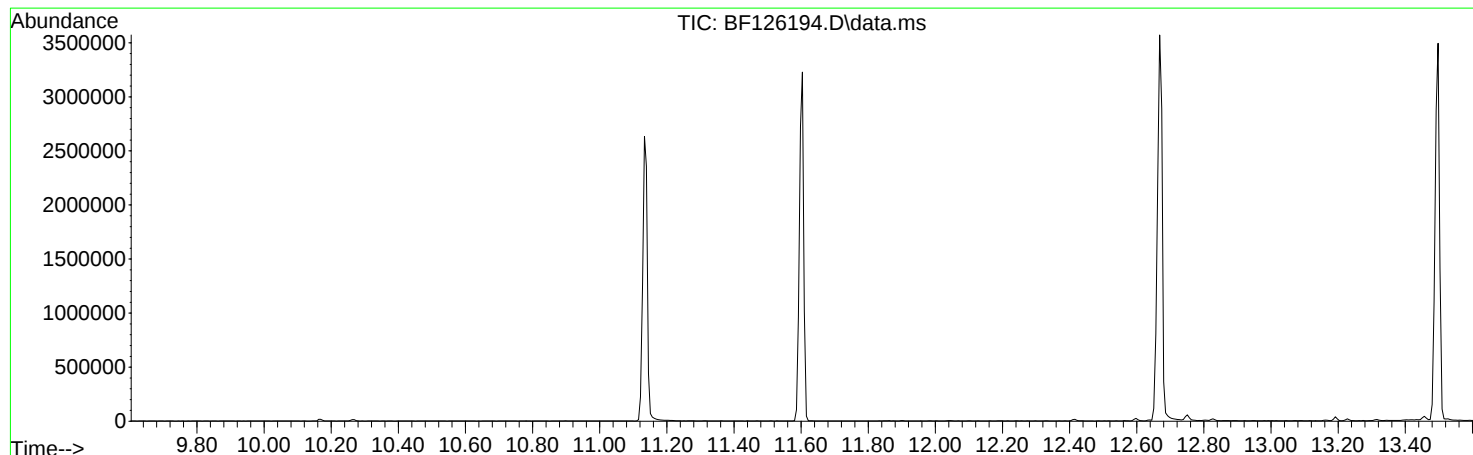




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.7	116581	PASS
68	69	0.00	2	1.7	1799	PASS
69	198	0.00	100	42.0	104923	PASS
70	69	0.00	2	0.6	658	PASS
127	198	10	80	55.1	137603	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	249571	PASS
199	198	5	9	6.4	15925	PASS
275	198	10	60	25.4	63320	PASS
365	198	1	100	3.6	9069	PASS
441	198	0.01	100	19.0	47453	PASS
442	442	50	100	100.0	292245	PASS
443	442	15	24	17.8	52080	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121521\
Data File : BF126194.D
Acq On : 15 Dec 2021 14:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 16 12:48:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

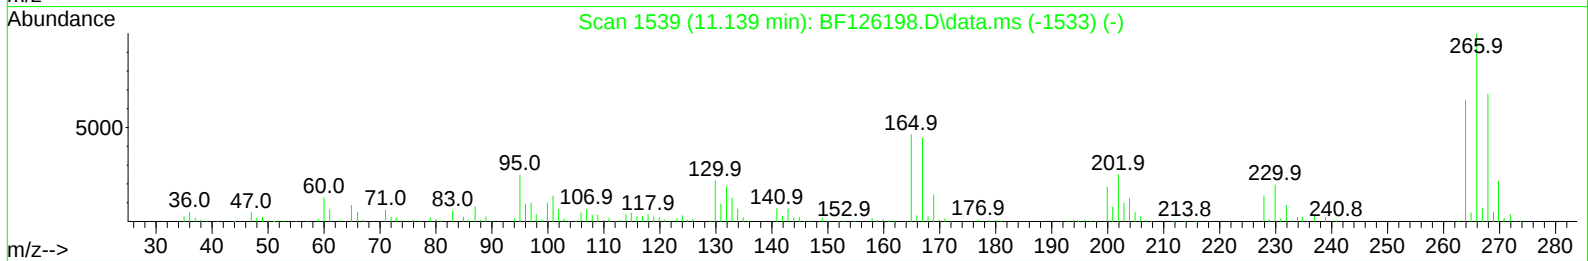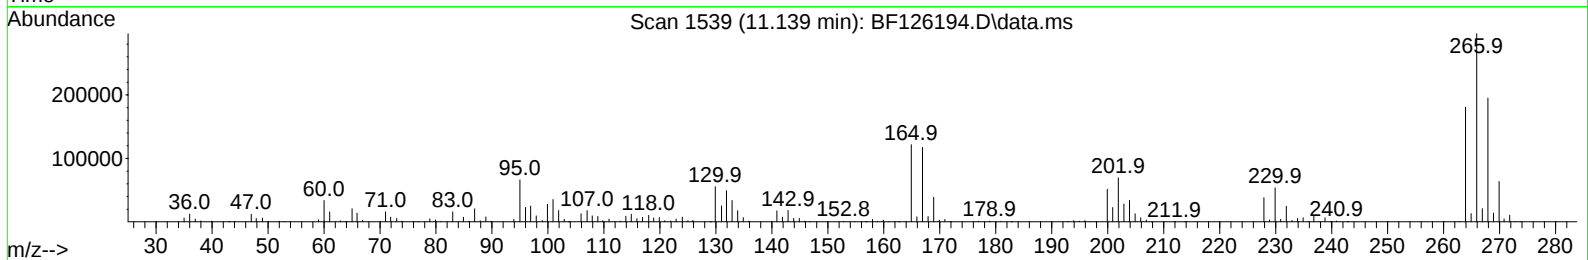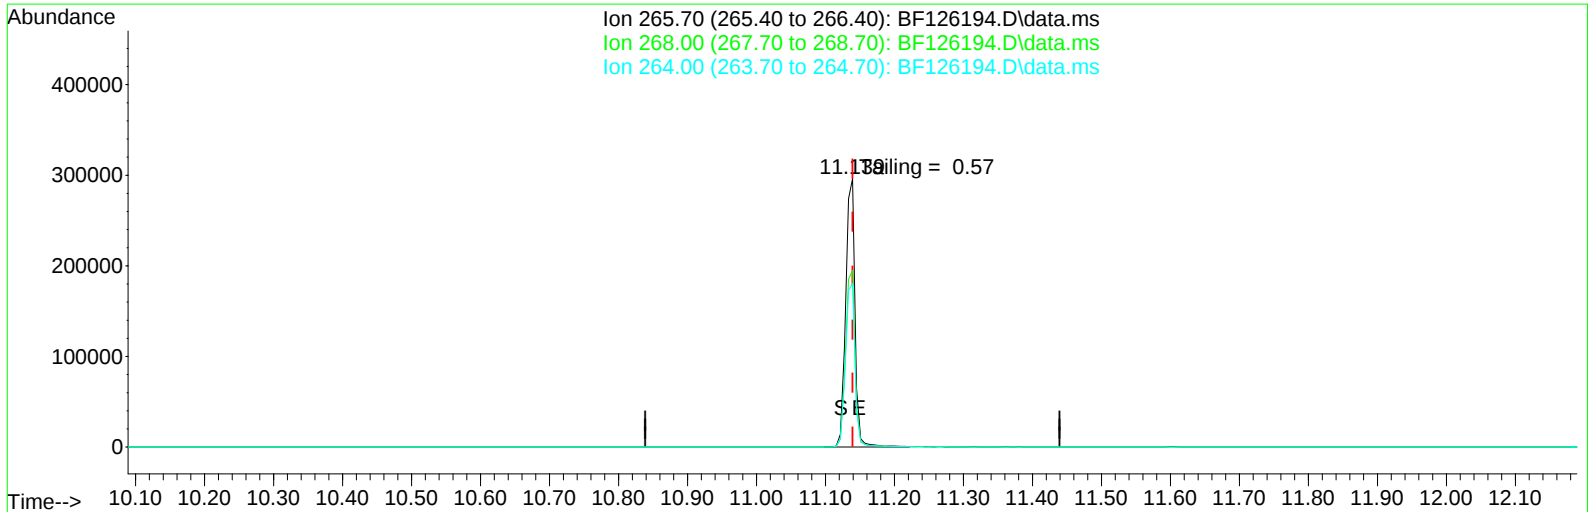

TIC: BF126194.D\data.ms

(70) Pentachlorophenol (C)

11.139min (+ 0.000) 41241.18 ng




response 275858

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	65.80
264.00	69.90	60.99
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121521\
Data File : BF126194.D
Acq On : 15 Dec 2021 14:38
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Dec 16 12:48:06 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Dec 16 12:22:48 2021
Response via : Initial Calibration

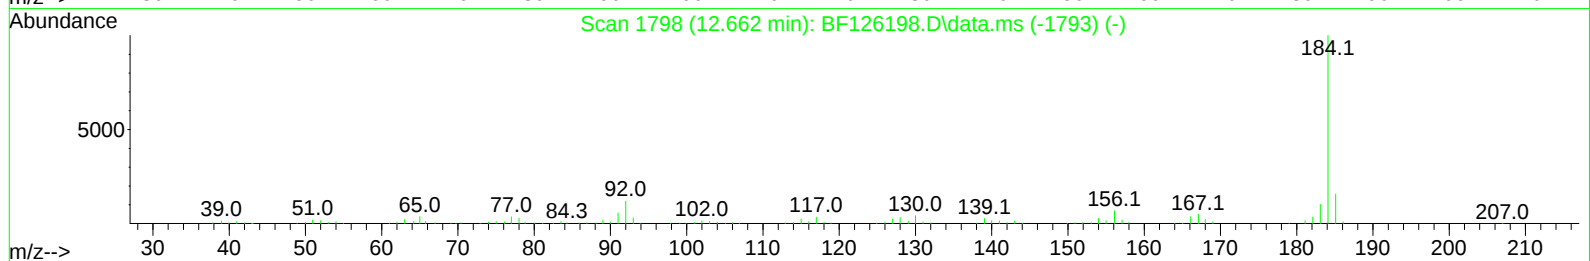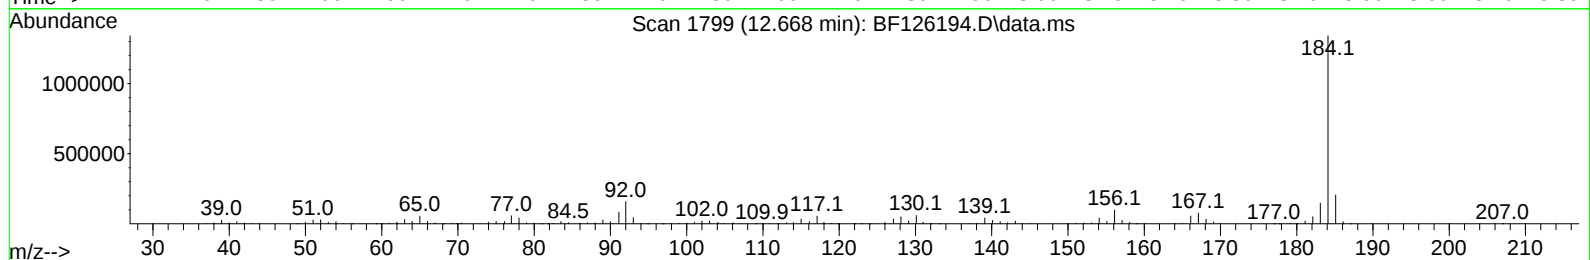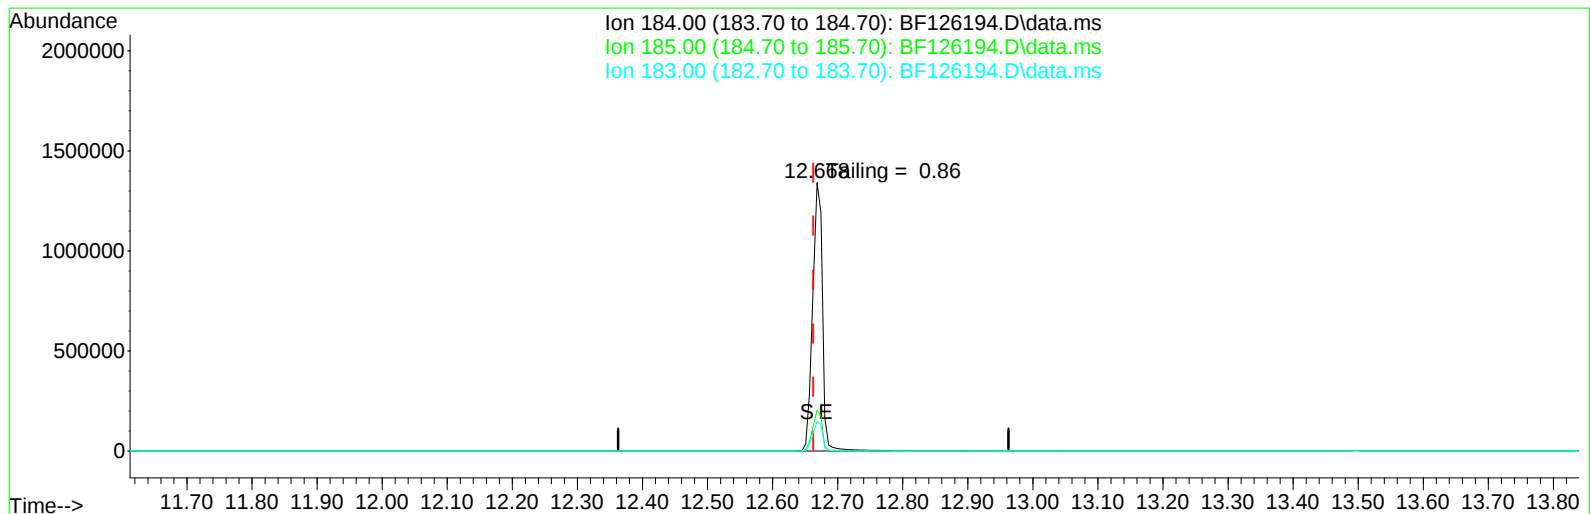

TIC: BF126194.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 0.00 ng

response 1412916

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	15.32
183.00	10.10	10.99
0.00	0.00	0.00

Instrument :
BNA_F
ClientSampleId :
DFTPP

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/15/2021	BNA_F	<u>BF126194.D</u>
Compound Name	Response	Retention Time
DDT	592528	13.49
DDD	4289	13.19
DDE	351	12.86
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4640	597168	0.78