
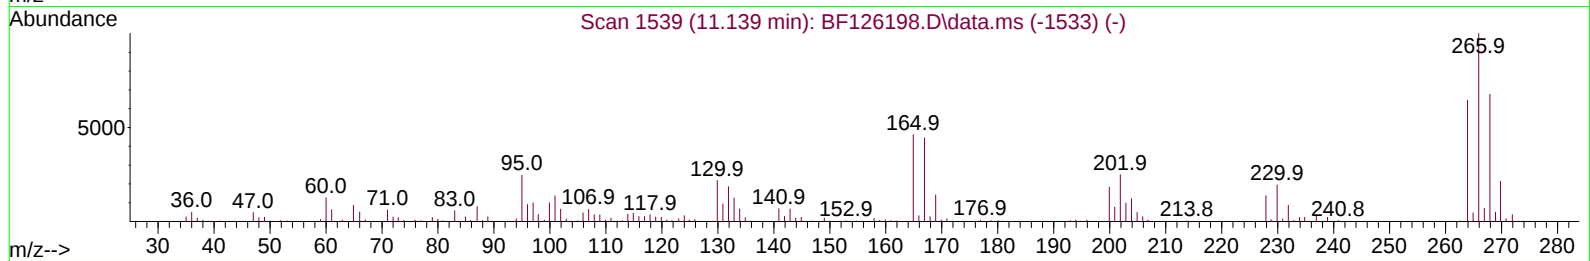
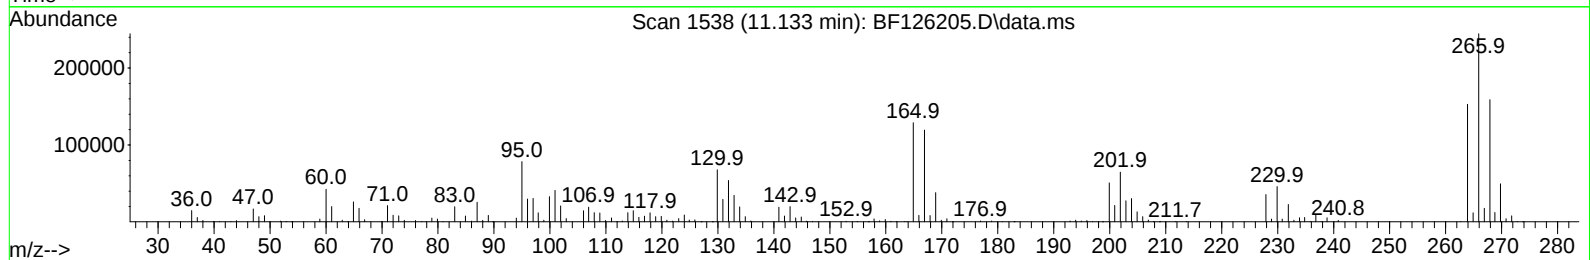


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121621\
 Data File : BF126205.D
 Acq On : 16 Dec 2021 10:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 13:48:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

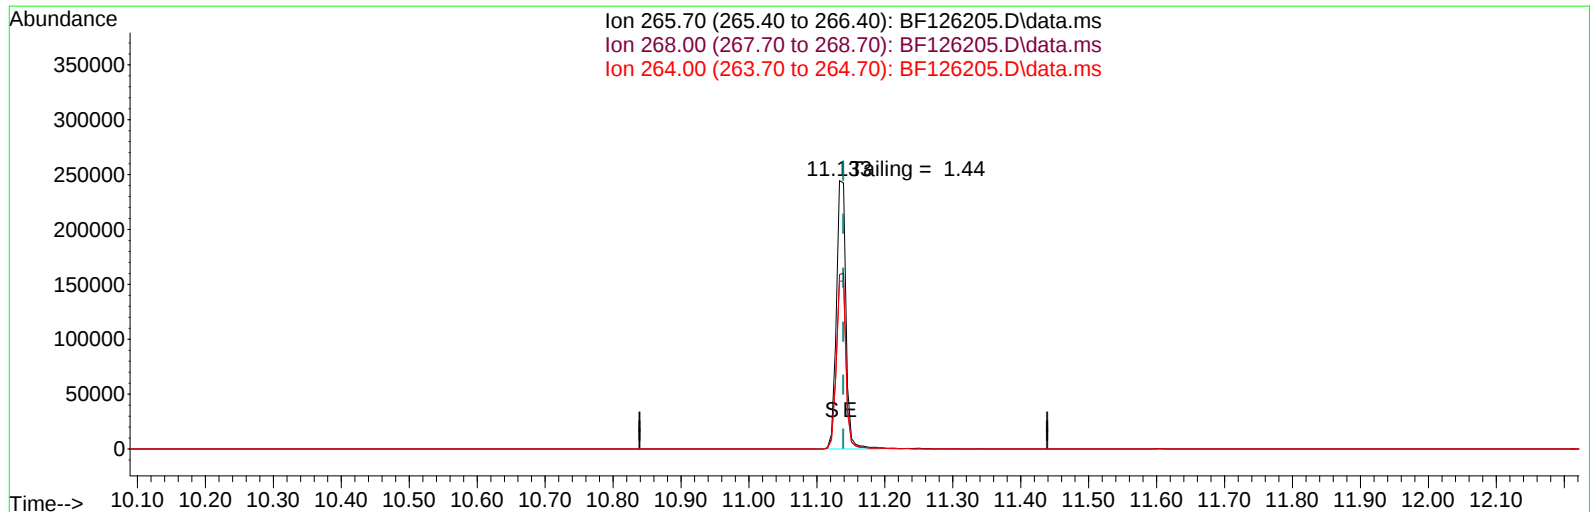

TIC: BF126205.D\data.ms

(70) Pentachlorophenol (C)




11.133min (-0.006) 102216.34 ng

response 241167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.98
264.00	69.90	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121621\
 Data File : BF126205.D
 Acq On : 16 Dec 2021 10:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 13:48:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

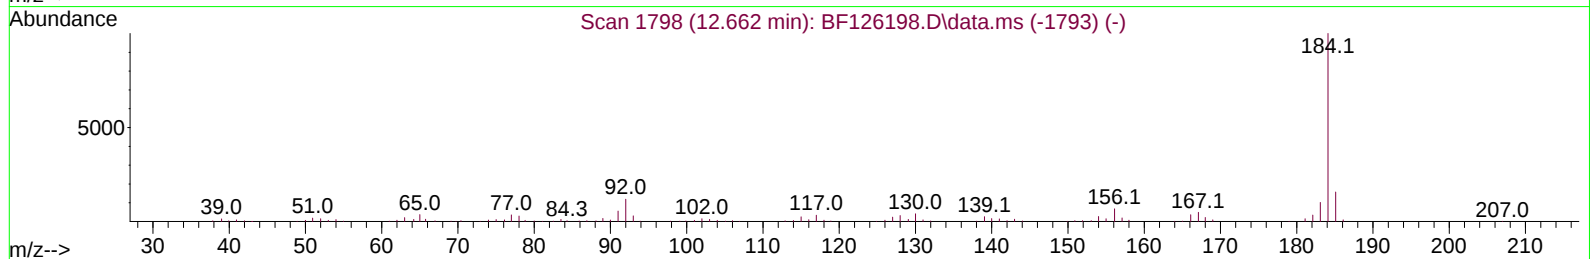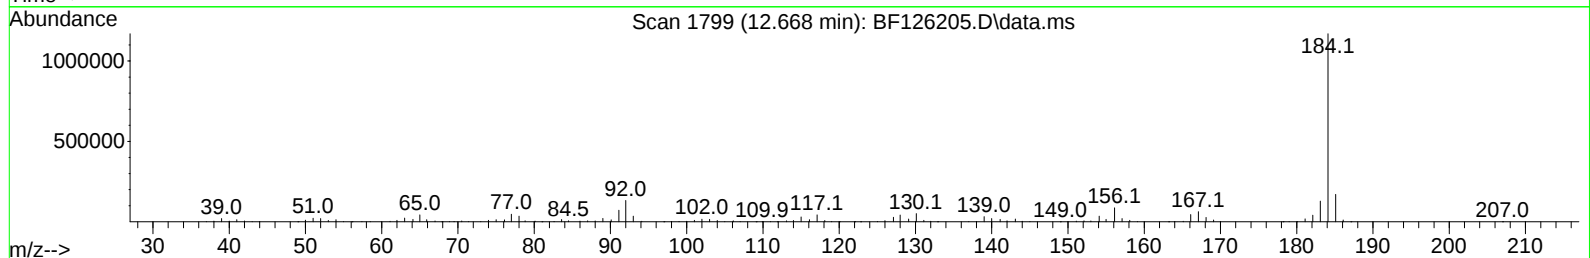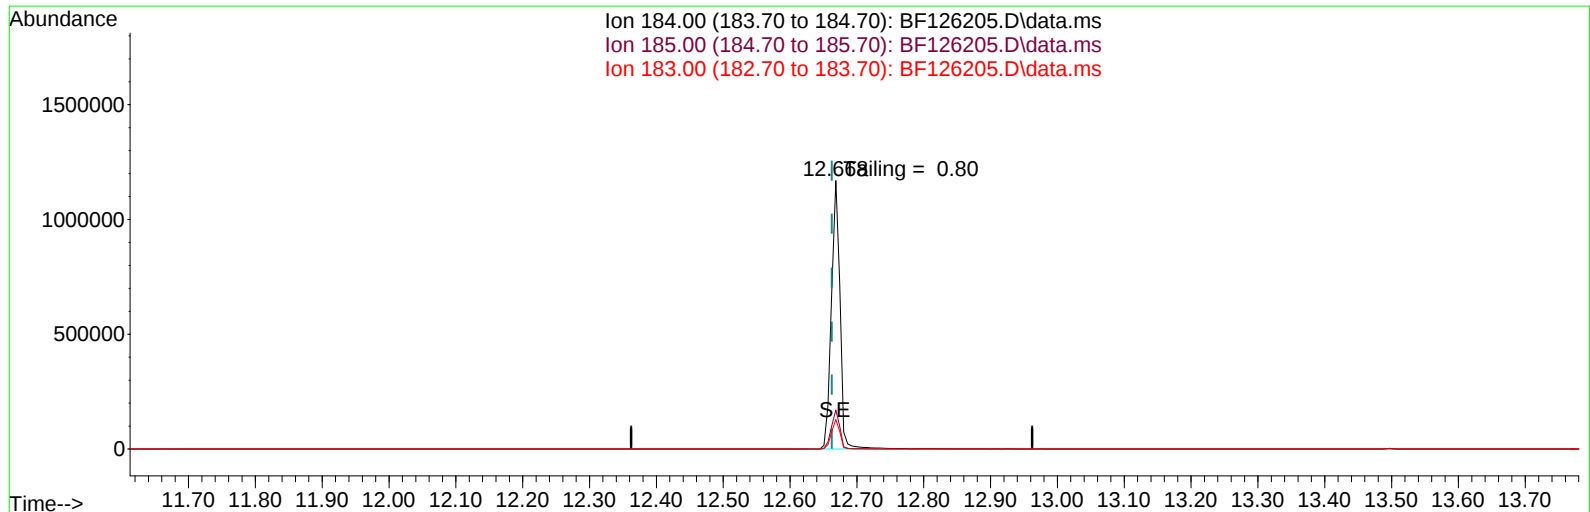

TIC: BF126205.D\data.ms

(77) Benzidine**12.668min (+ 0.006) 41871.97 ng****response 1051590**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.56
183.00	10.10	11.00
0.00	0.00	0.00