
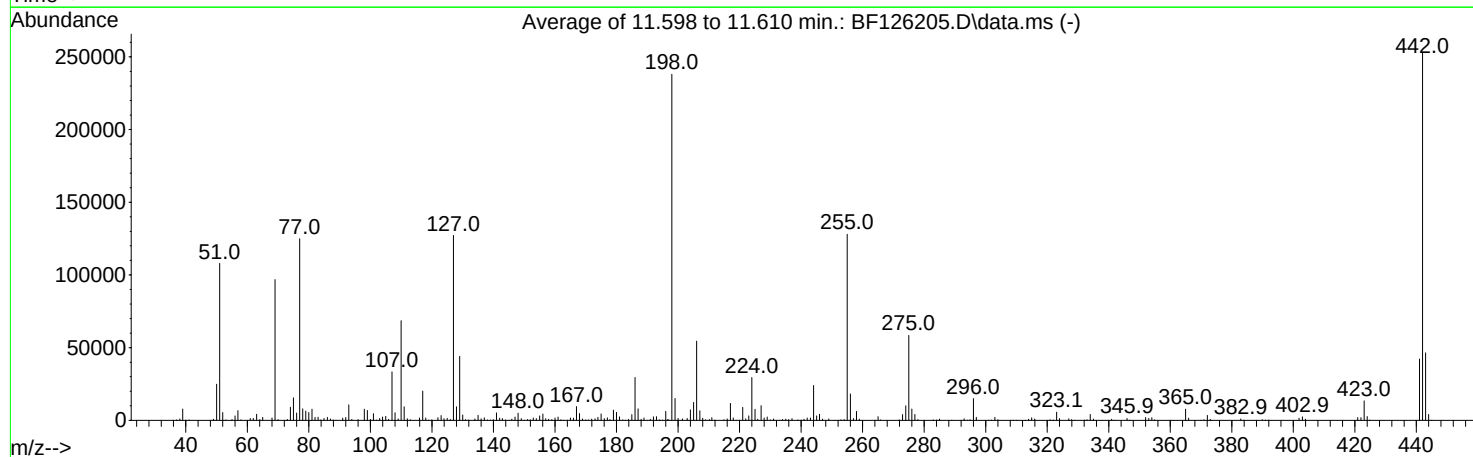


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121621\
 Data File : BF126205.D
 Acq On : 16 Dec 2021 10:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Dec 16 12:22:48 2021

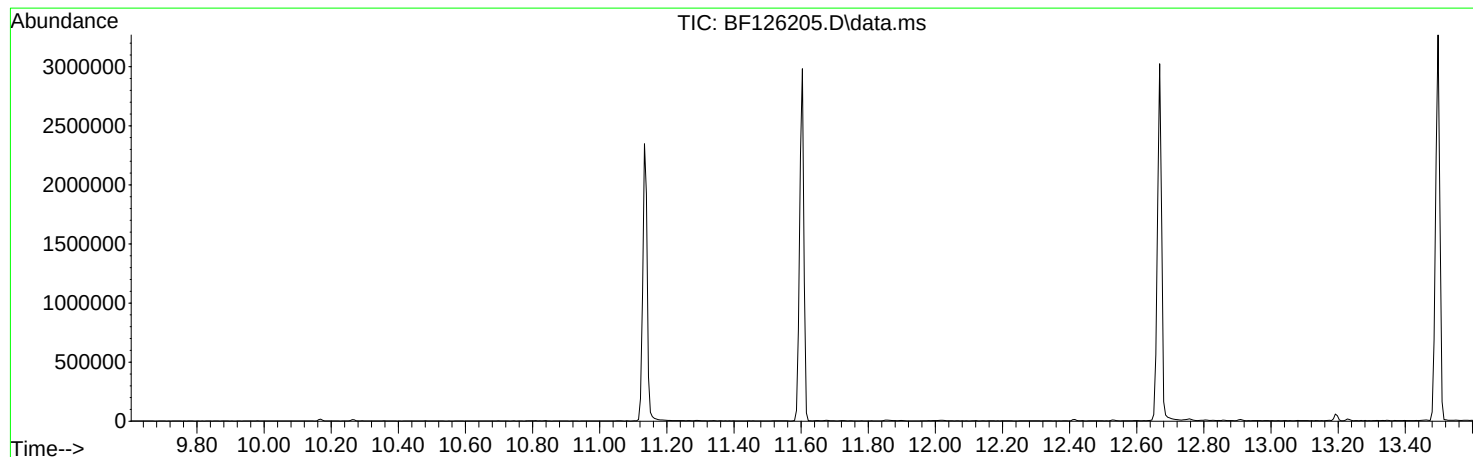




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1611

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.3	107931	PASS
68	69	0.00	2	1.7	1666	PASS
69	198	0.00	100	40.7	96864	PASS
70	69	0.00	2	0.6	562	PASS
127	198	10	80	53.4	127179	PASS
197	198	0.00	2	0.3	672	PASS
198	198	100	100	100.0	238021	PASS
199	198	5	9	6.3	15040	PASS
275	198	10	60	24.5	58432	PASS
365	198	1	100	3.3	7761	PASS
441	198	0.01	100	17.7	42101	PASS
442	442	50	100	100.0	252992	PASS
443	442	15	24	18.4	46477	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121621\
 Data File : BF126205.D
 Acq On : 16 Dec 2021 10:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 16 13:48:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

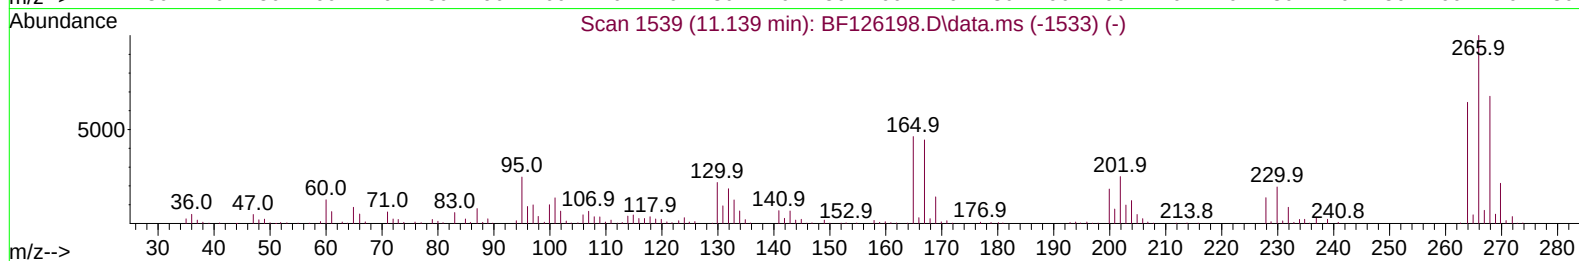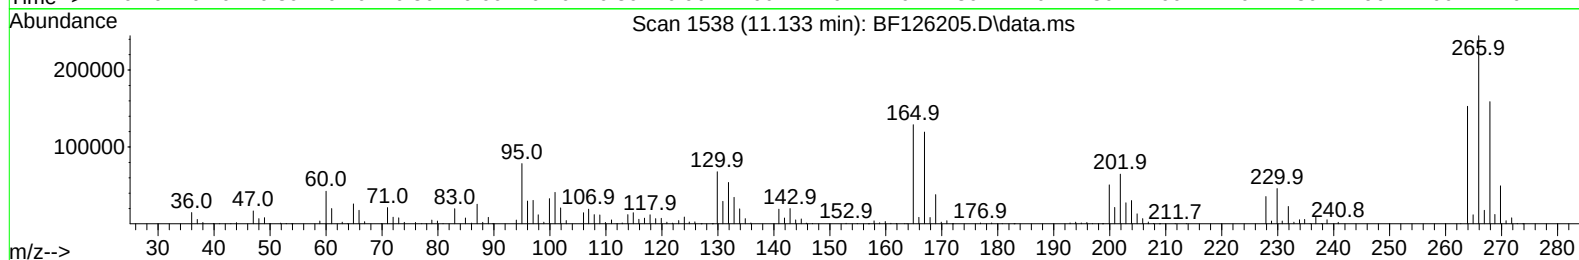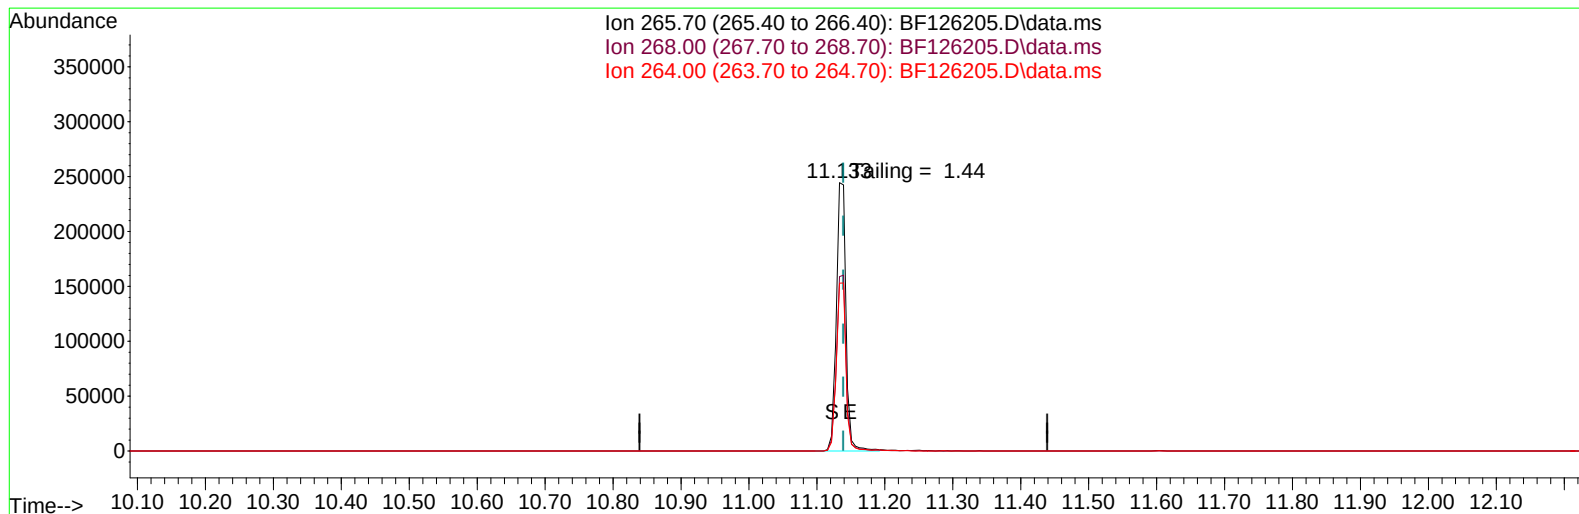

TIC: BF126205.D\data.ms

(70) Pentachlorophenol (C)

11.133min (-0.006) 102216.34 ng




response 241167

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.98
264.00	69.90	62.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121621\
 Data File : BF126205.D
 Acq On : 16 Dec 2021 10:48
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Dec 16 13:48:15 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121521.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Dec 16 12:22:48 2021
 Response via : Initial Calibration

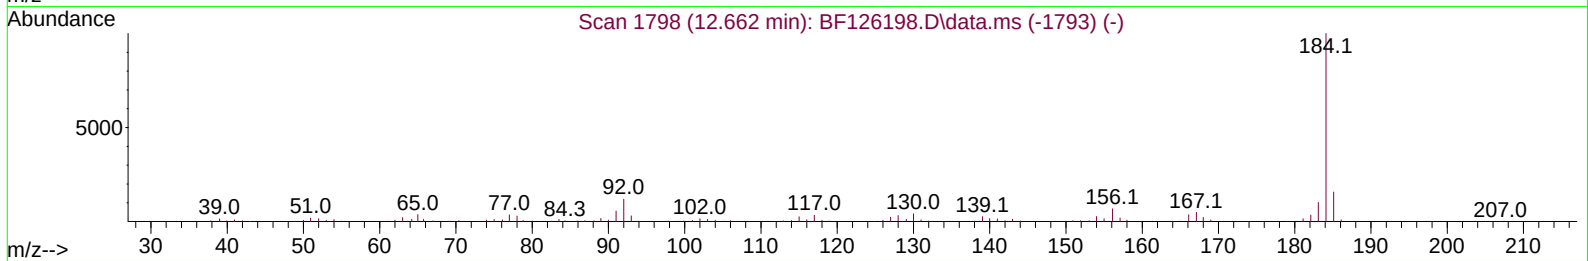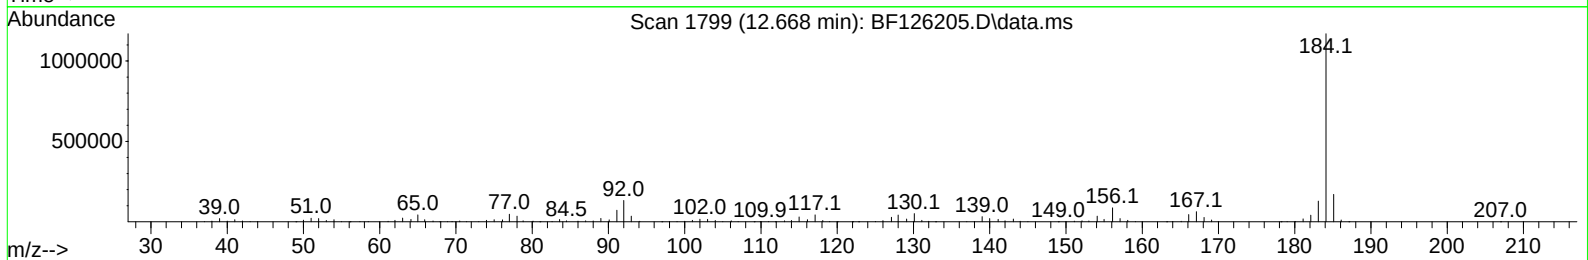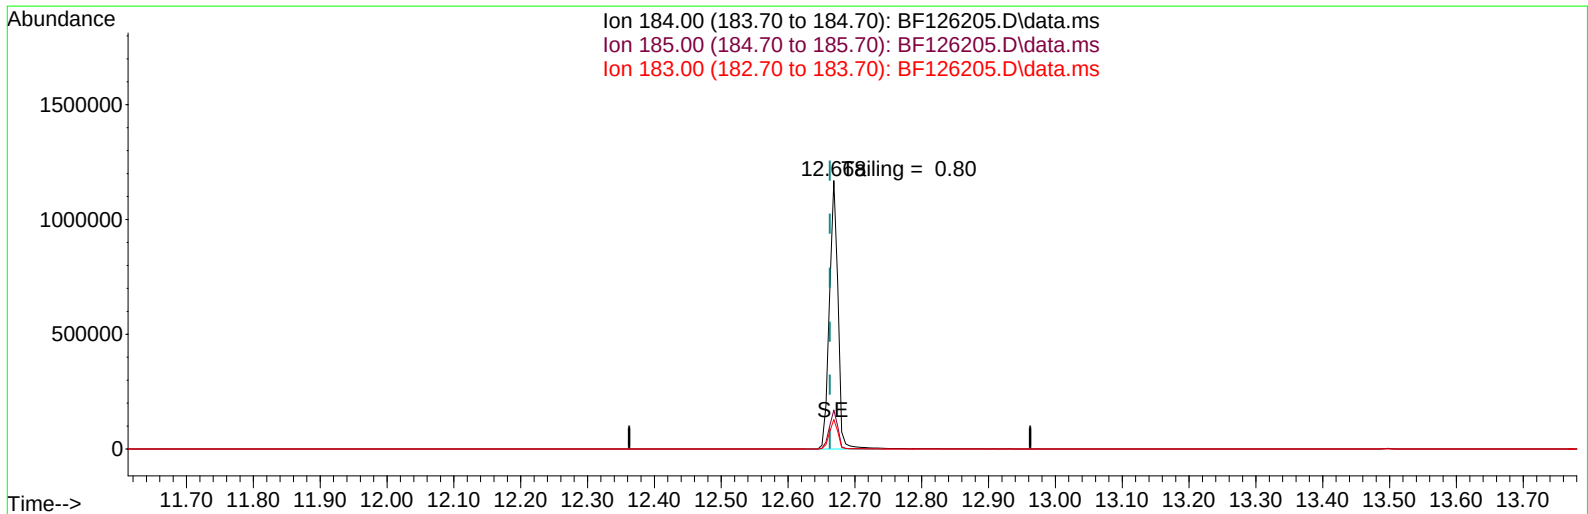

TIC: BF126205.D\data.ms

(77) Benzidine

12.668min (+ 0.006) 41871.97 ng

response 1051590

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.56
183.00	10.10	11.00
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
12/16/2021	BNA_F	<u>BF126205.D</u>
Compound Name	Response	Retention Time
DDT	540480	13.49
DDD	9407	13.19
DDE	770	12.85
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10177	550657	1.85

Instrument :
BNA_F
ClientSampleId :
DFTPP