
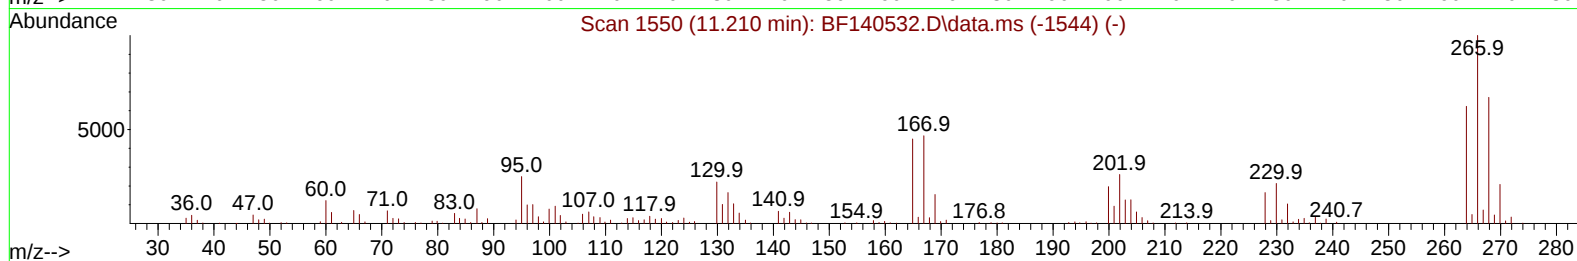
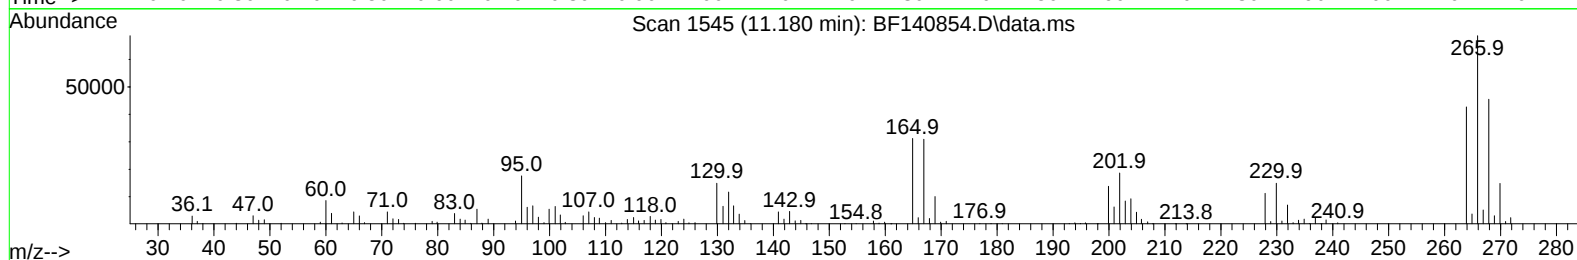


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121624\
Data File : BF140854.D
Acq On : 16 Dec 2024 11:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 12:02:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

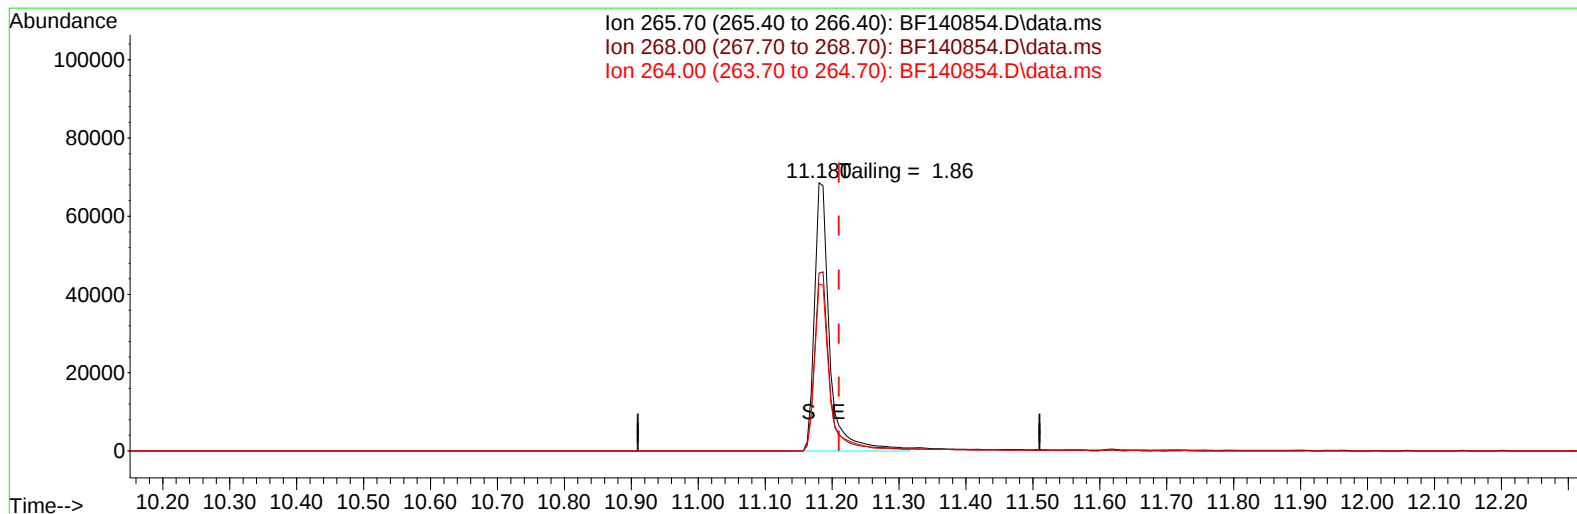

TIC: BF140854.D\data.ms

(70) Pentachlorophenol (C)




11.180min (-0.030) 3894.75 ng m

response 108541

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	67.10	66.31
264.00	62.30	62.20
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121624\
Data File : BF140854.D
Acq On : 16 Dec 2024 11:21
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Dec 16 12:02:25 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Nov 21 15:23:48 2024
Response via : Initial Calibration

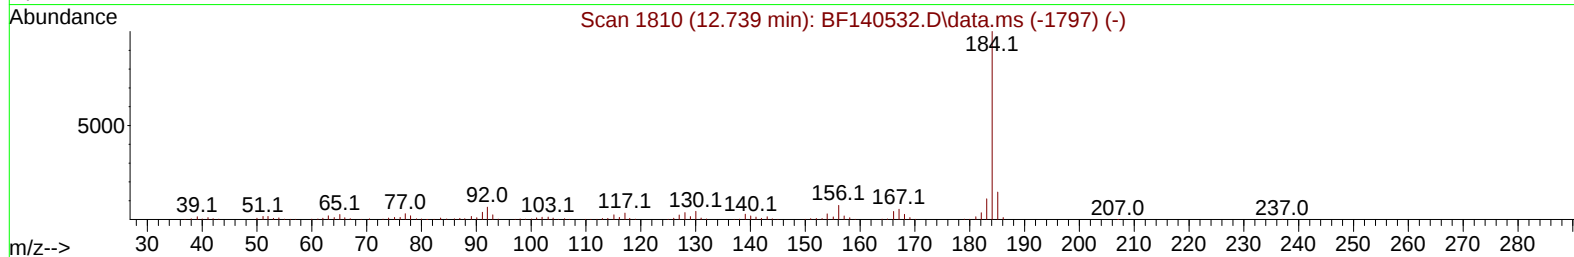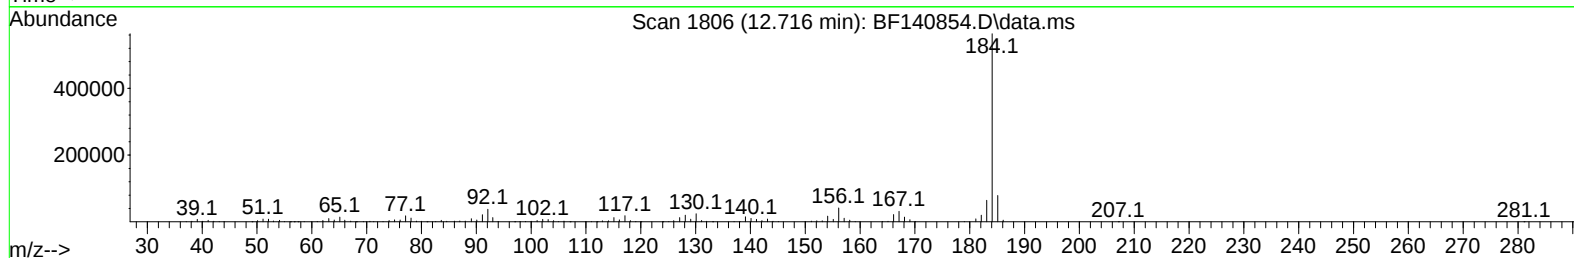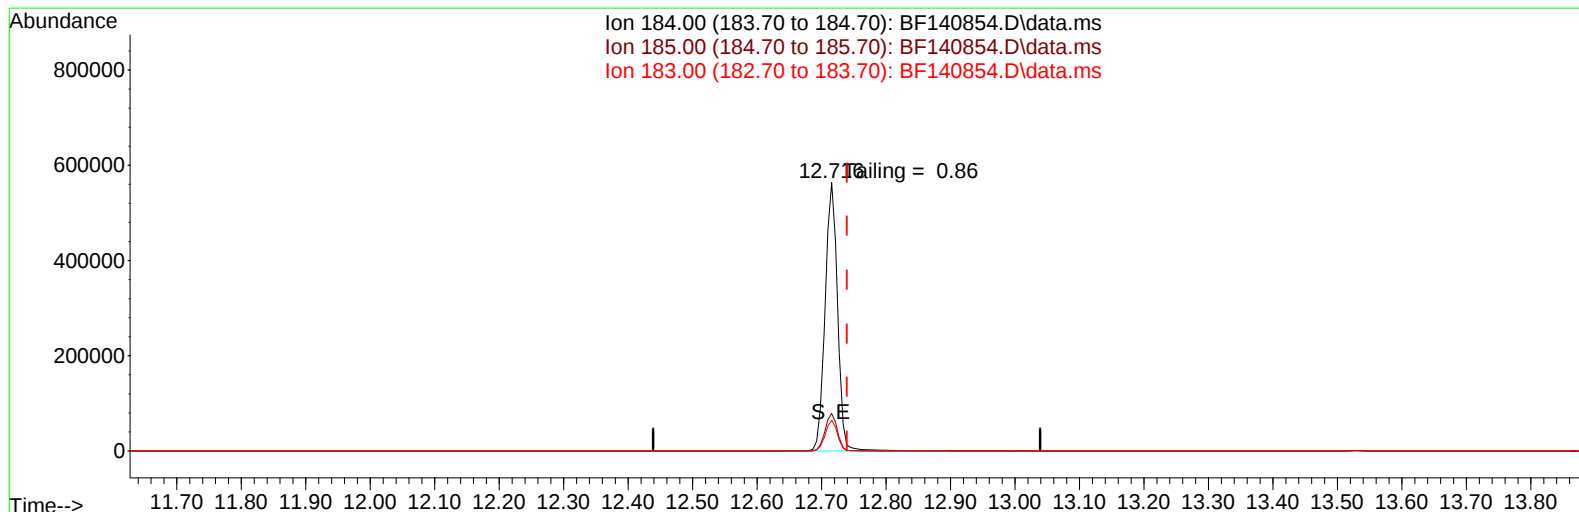

TIC: BF140854.D\data.ms

(77) Benzidine**12.716min (-0.023) 4792.75 ng****response 759160**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.01
183.00	11.00	11.44
0.00	0.00	0.00