

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121624\
 Data File : BF140864.D
 Acq On : 16 Dec 2024 17:08
 Operator : RC/JU
 Sample : PB165543BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB165543BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF140864.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.240	20	25	38	rVB	29228	53714	1.35%	0.260%
2	5.498	573	579	604	rBV	1799607	2470367	61.97%	11.964%
3	6.493	742	748	770	rBV	1777168	2551389	64.00%	12.356%
4	6.845	803	808	816	rBV	377785	471581	11.83%	2.284%
5	7.410	898	904	920	rBV	1279859	1833429	45.99%	8.879%
6	8.128	1020	1026	1040	rBV	461318	634638	15.92%	3.074%
7	9.198	1201	1208	1213	rBV	2498688	3493276	87.63%	16.918%
8	9.881	1317	1324	1338	rVB	611050	793031	19.89%	3.841%
9	10.675	1453	1459	1483	rBV	1705220	2294036	57.55%	11.110%
10	11.369	1572	1577	1589	rBV	612514	796199	19.97%	3.856%
11	12.957	1841	1847	1852	rBV	2950575	3986395	100.00%	19.306%
12	14.021	2023	2028	2043	rVB	510517	679334	17.04%	3.290%
13	15.504	2274	2280	2291	rBV	338457	548818	13.77%	2.658%
14	17.027	2532	2539	2544	rBV6	15728	42298	1.06%	0.205%




Sum of corrected areas: 20648505

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121624\
Data File : BF140864.D
Acq On : 16 Dec 2024 17:08
Operator : RC/JU
Sample : PB165543BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165543BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

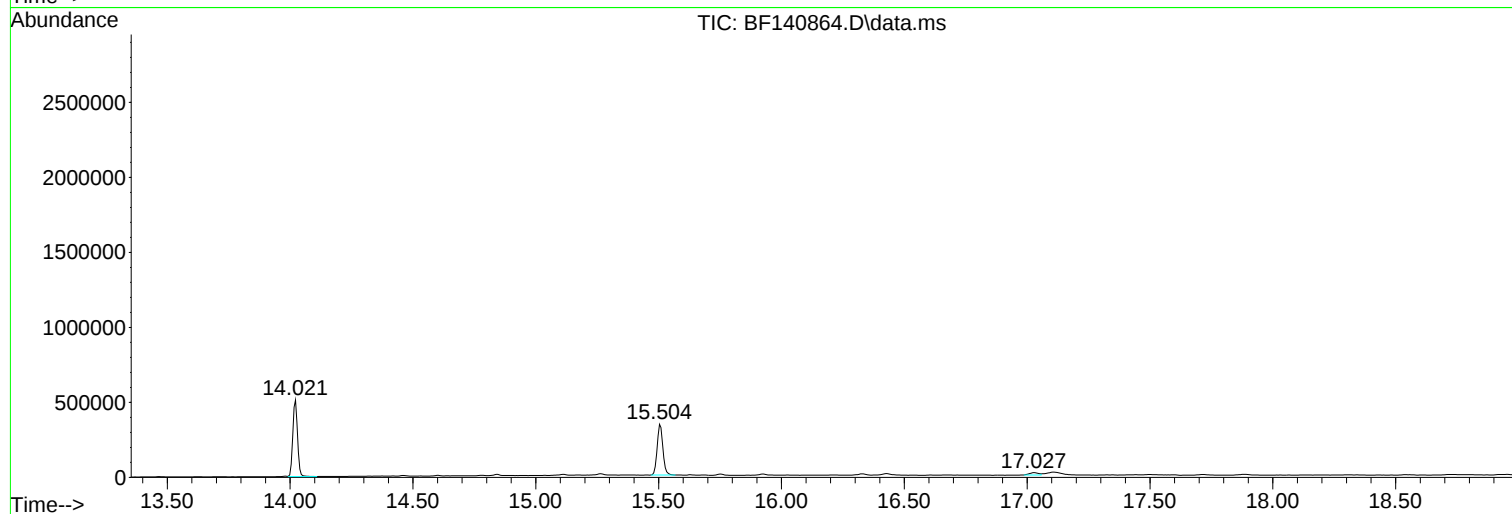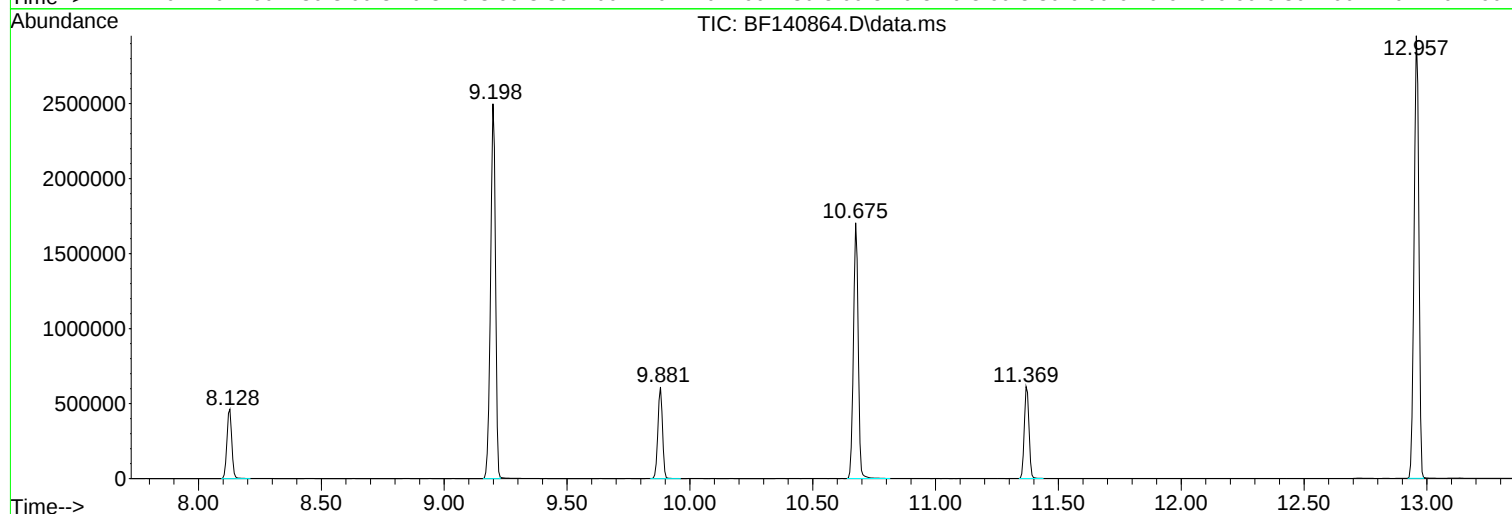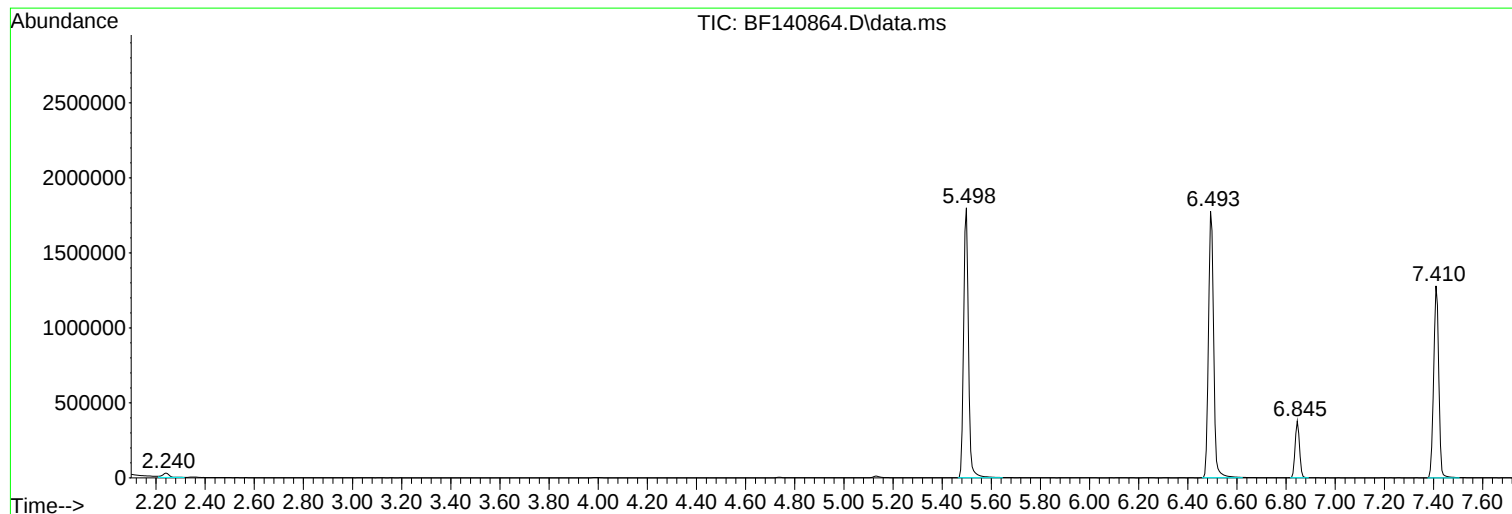

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121624\
Data File : BF140864.D
Acq On : 16 Dec 2024 17:08
Operator : RC/JU
Sample : PB165543BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165543BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.240	2.28 ng	53714	1,4-Dichlorobenzene-d4	6.845

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	83
2			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	40
3			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	38
4			Pentane, 3-methoxy-	102	C6H14O	036839-67-5	23
5			Acetamide, N-ethyl-	87	C4H9NO	000625-50-3	9

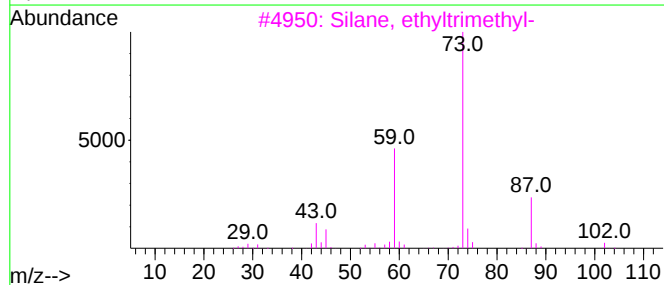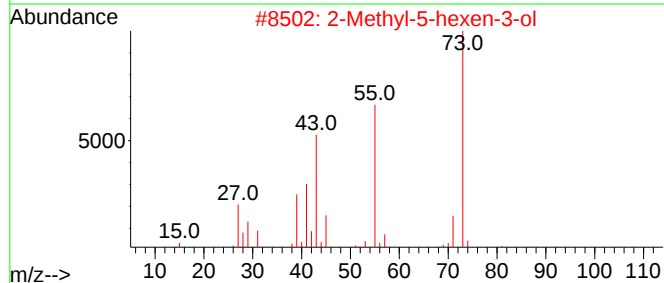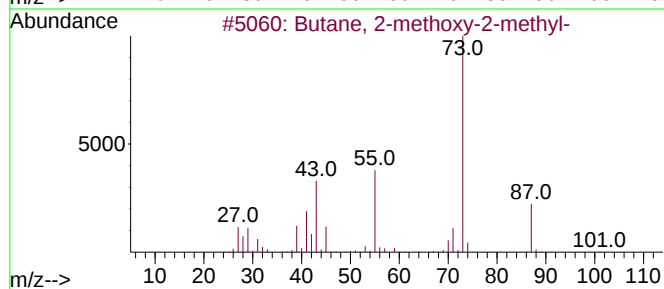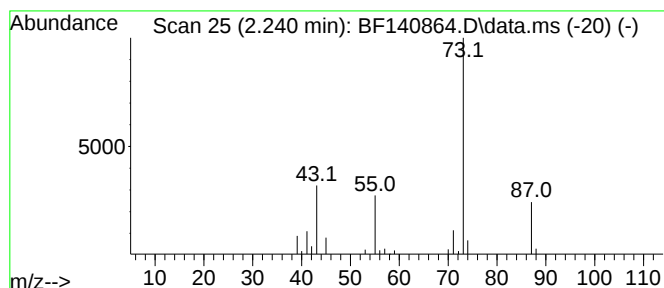

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF121624\
Data File : BF140864.D
Acq On : 16 Dec 2024 17:08
Operator : RC/JU
Sample : PB165543BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB165543BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF121624.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.240	2.3	ng	53714	1	6.845	471581	20.0