

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030122\
 Data File : BF127124.D
 Acq On : 01 Mar 2022 19:02
 Operator : CG\JU
 Sample : N1689-10
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DUP022222

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF127124.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.510	544	548	551	rBV	1310444	1181309	37.40%	7.174%
2	6.510	715	718	725	rBV	843262	768491	24.33%	4.667%
3	6.887	779	782	786	rBV	678593	555913	17.60%	3.376%
4	7.457	873	879	882	rBV	1899027	1848763	58.53%	11.228%
5	8.069	980	983	991	rBV	69115	67891	2.15%	0.412%
6	8.175	997	1001	1004	rBV	847229	753428	23.85%	4.576%
7	9.251	1178	1184	1187	rBV	3742753	3158804	100.00%	19.184%
8	9.733	1262	1266	1275	rBV3	30921	56808	1.80%	0.345%
9	9.933	1296	1300	1303	rVB	945565	817333	25.87%	4.964%
10	10.328	1365	1367	1369	rBV	43893	36522	1.16%	0.222%
11	10.722	1430	1434	1437	rBV	2435770	2178264	68.96%	13.229%
12	11.369	1540	1544	1548	rVB	78214	67489	2.14%	0.410%
13	11.422	1549	1553	1556	rBV	1071737	827753	26.20%	5.027%
14	11.580	1577	1580	1586	rVB	60037	63656	2.02%	0.387%
15	11.974	1644	1647	1650	rVB	69542	53147	1.68%	0.323%
16	13.010	1819	1823	1826	rBV	3322798	2954287	93.53%	17.942%
17	13.916	1970	1977	1978	rBV3	67091	103426	3.27%	0.628%
18	14.068	1999	2003	2006	rVB	535490	476590	15.09%	2.894%
19	15.557	2251	2256	2263	rBV	377876	496023	15.70%	3.012%




Sum of corrected areas: 16465897

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030122\
Data File : BF127124.D
Acq On : 01 Mar 2022 19:02
Operator : CG\JU
Sample : N1689-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP022222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

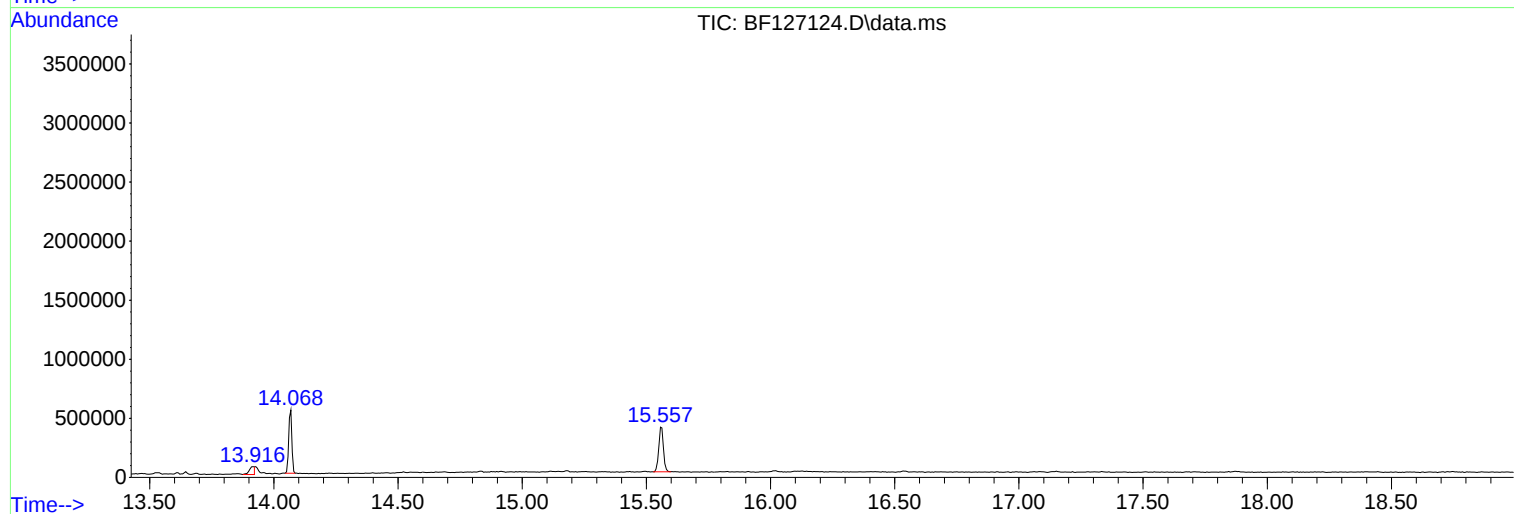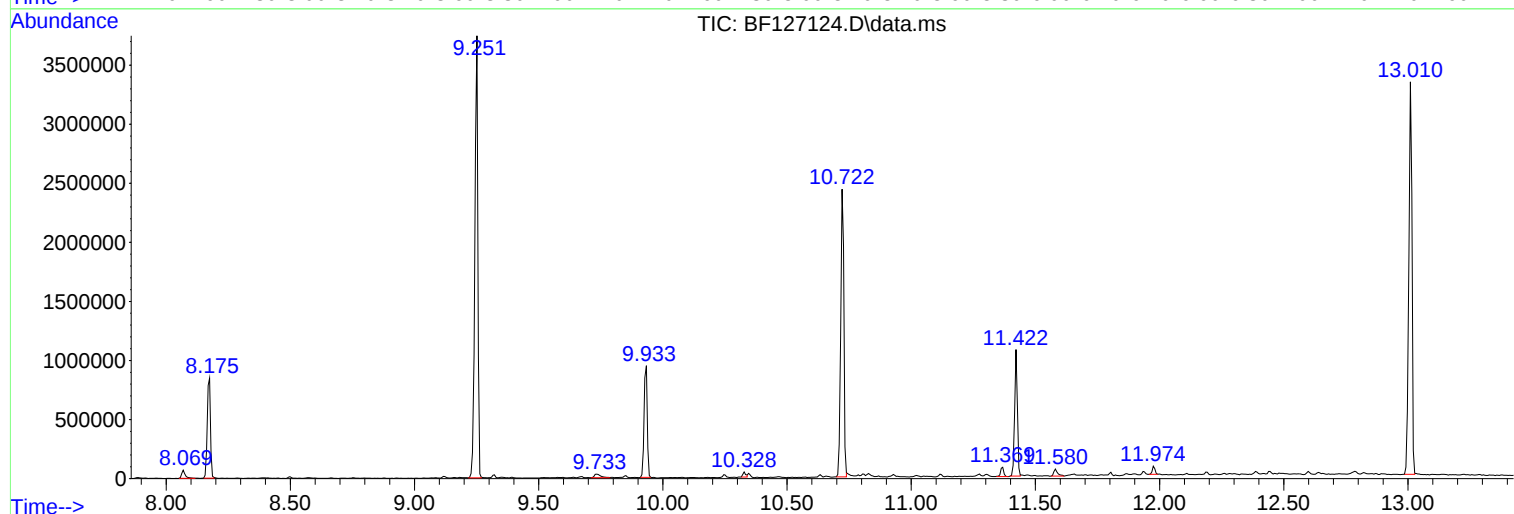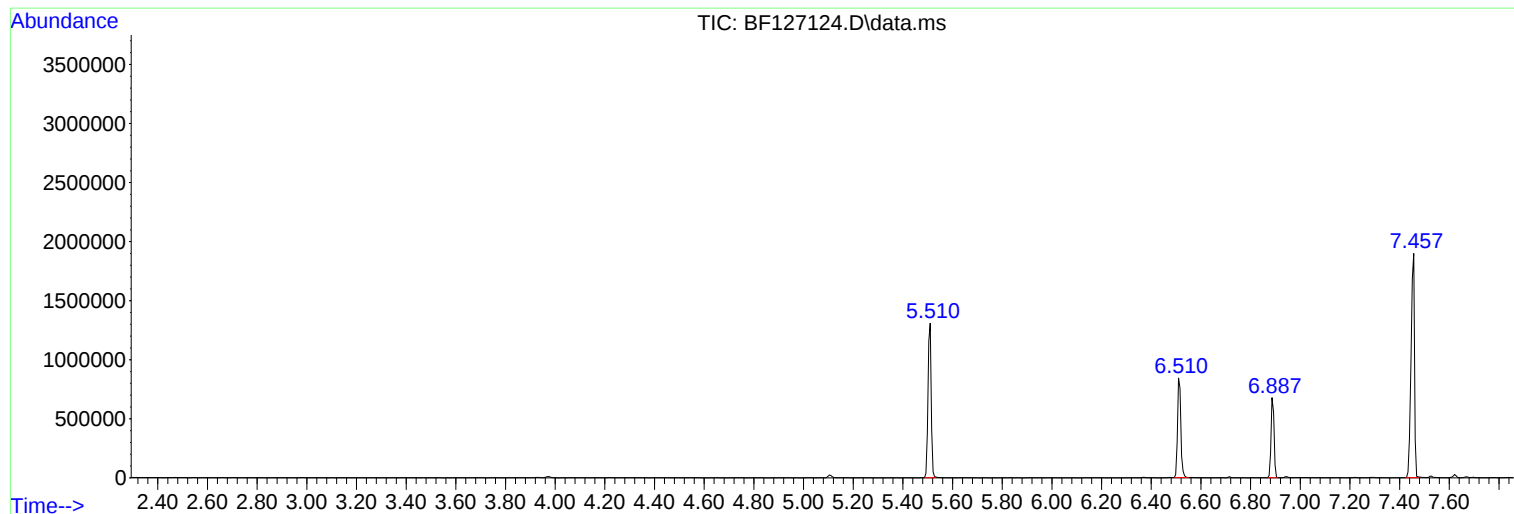

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030122\
Data File : BF127124.D
Acq On : 01 Mar 2022 19:02
Operator : CG\JU
Sample : N1689-10
Misc :
ALS Vial : 12 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
DUP022222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Pentafluoropropionic acid, ... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.	
13.916	4.34 ng	103426	Chrysene-d12	14.069	
Hit# of 5	Tentative ID	MW	MolForm	CAS#	Qual
1	Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	95
2	Trifluoroacetic acid, pentadecyl...	324	C17H31F3O2	959010-23-2	95
3	Trifluoroacetoxy hexadecane	338	C18H33F3O2	006222-03-3	95
4	Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
5	Heptafluorobutyric acid, n-tetra...	410	C18H29F7O2	007365-36-8	94

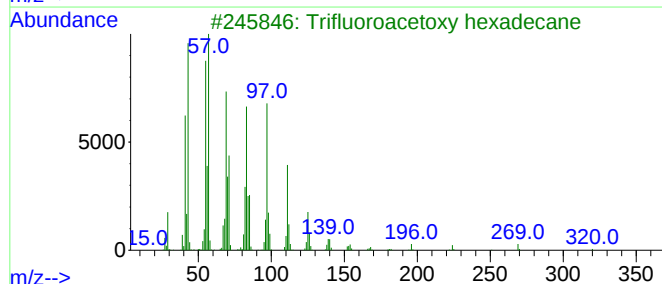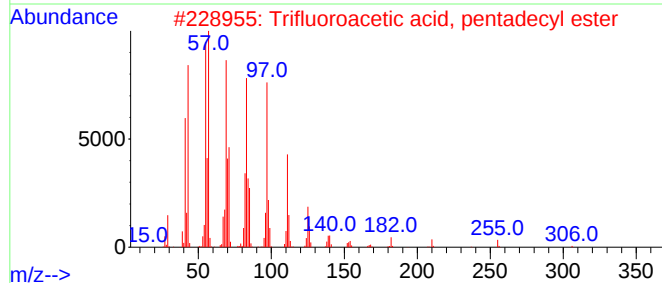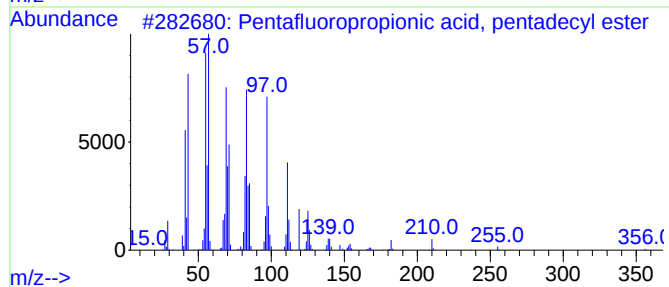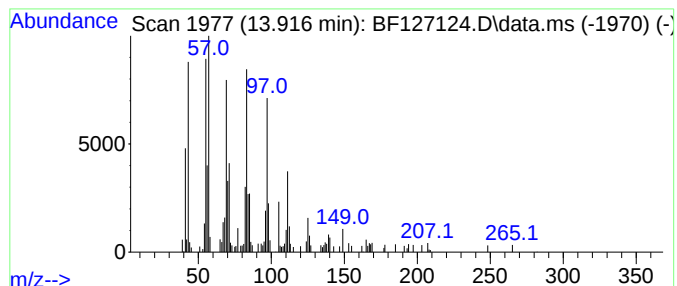

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030122\
Data File : BF127124.D
Acq On : 01 Mar 2022 19:02
Operator : CG\JU
Sample : N1689-10
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DUP022222

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Pentafluoroprop...	13.916	4.3	ng	103426	5	14.069	476590	20.0