


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030122\
 Data File : BF127113.D
 Acq On : 01 Mar 2022 13:38
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Mar 01 23:57:09 2022

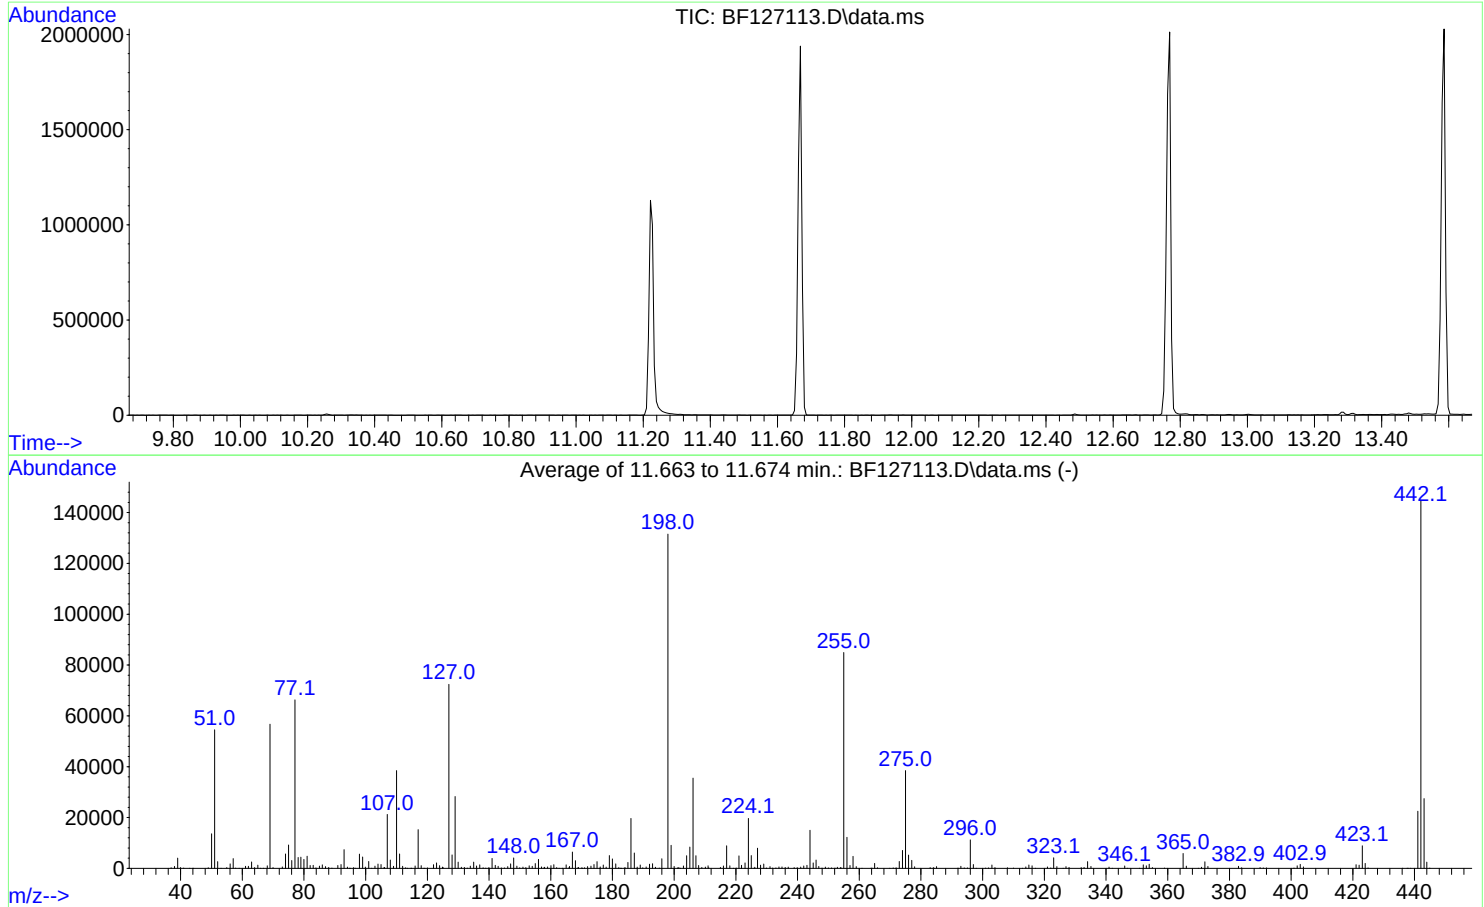




AutoFind: Scans 1594, 1595, 1596; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	54530	PASS
68	69	0.00	2	1.8	1023	PASS
69	198	0.00	100	43.1	56749	PASS
70	69	0.00	2	0.6	346	PASS
127	198	10	80	55.0	72400	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	131523	PASS
199	198	5	9	6.9	9042	PASS
275	198	10	60	29.3	38485	PASS
365	198	1	100	4.4	5847	PASS
441	198	0.01	100	17.1	22460	PASS
442	442	50	100	100.0	144731	PASS
443	442	15	24	19.0	27477	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030122\
Data File : BF127113.D
Acq On : 01 Mar 2022 13:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 02 03:51:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 01 23:57:09 2022
Response via : Initial Calibration

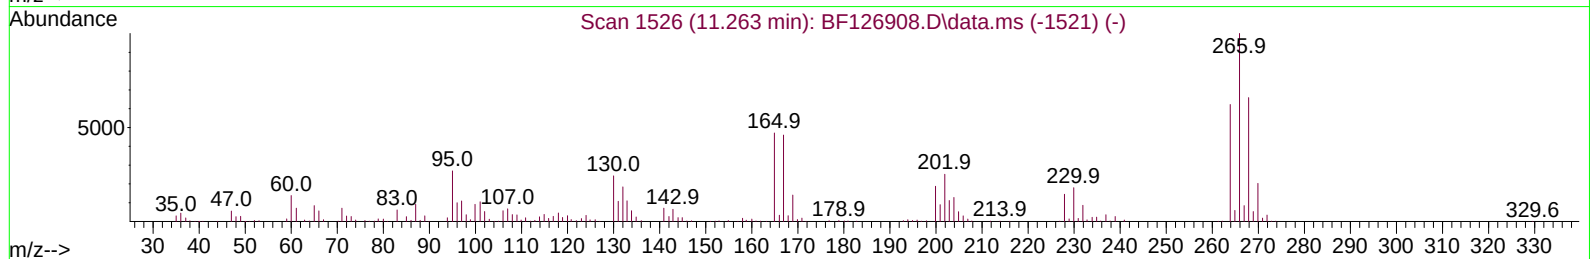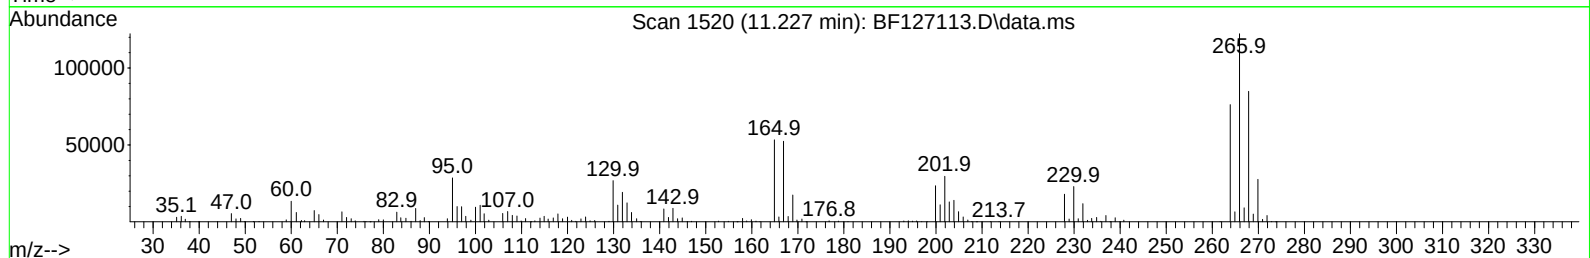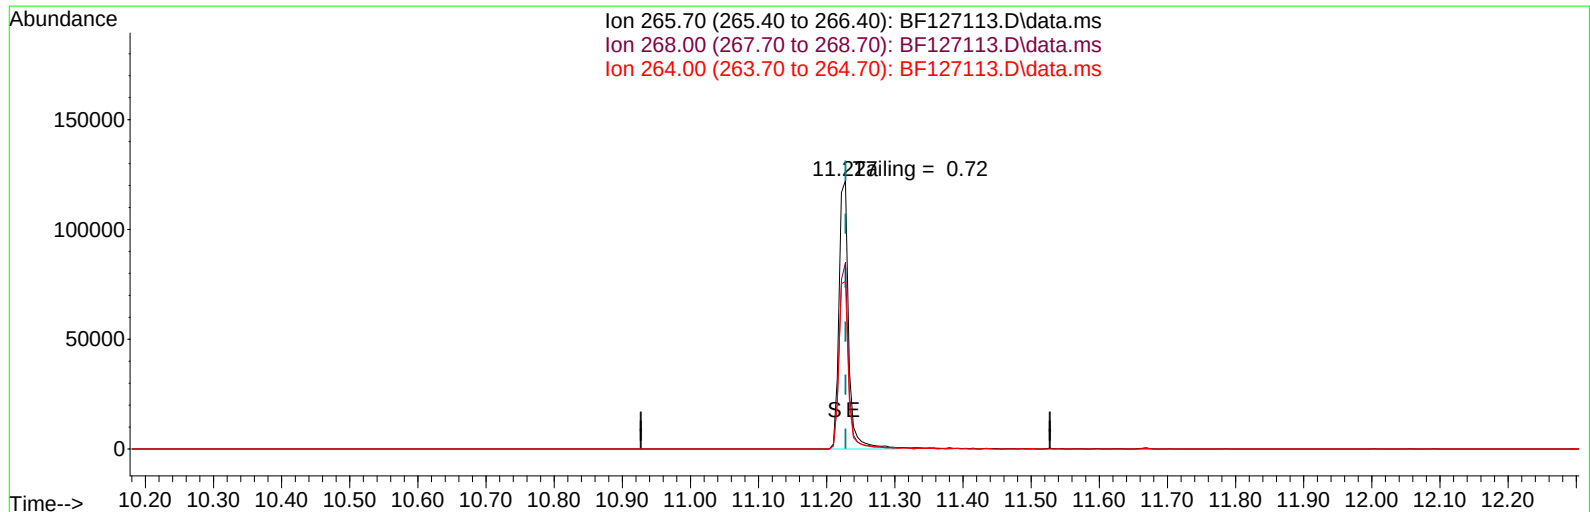

TIC: BF127113.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.000) 29584.98 ng




response 120049

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.40	69.44
264.00	63.00	62.34
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF030122\
Data File : BF127113.D
Acq On : 01 Mar 2022 13:38
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Mar 02 03:51:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF021622.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 01 23:57:09 2022
Response via : Initial Calibration

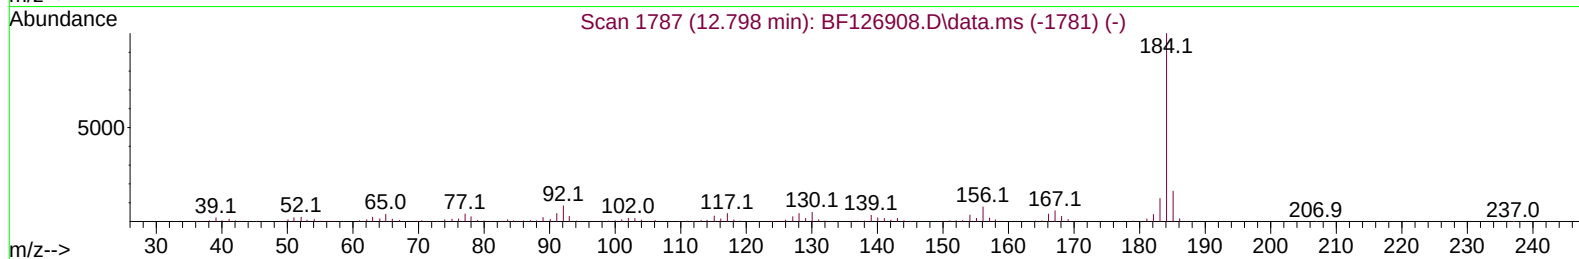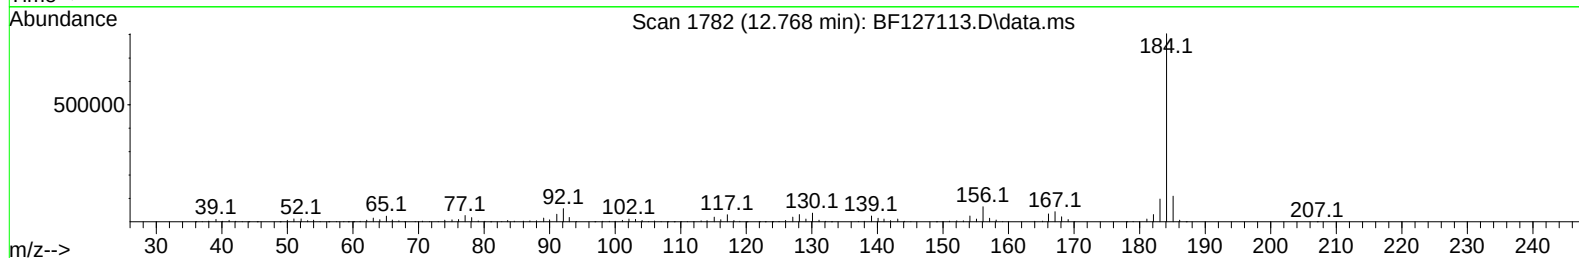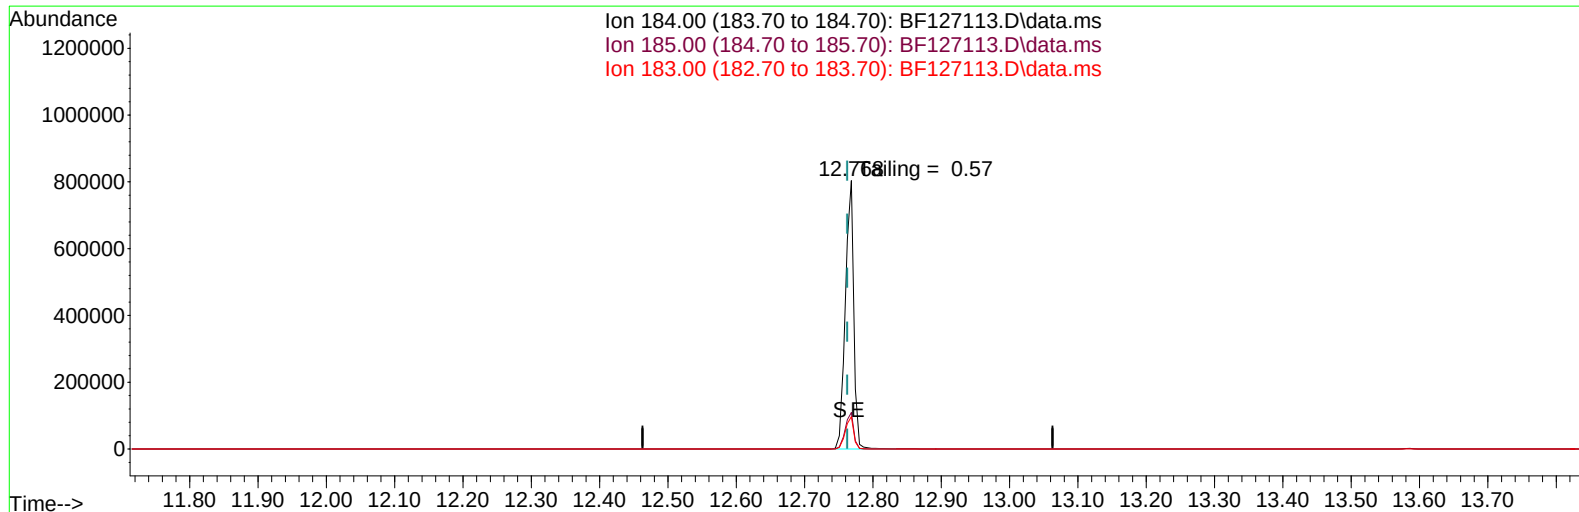

TIC: BF127113.D\data.ms

(77) Benzidine

12.768min (+ 0.006) 427463.52 ng

response 685380

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.80	13.63
183.00	10.20	12.07
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/1/2022	BNA_F	<u>BF127113.D</u>
Compound Name	Response	Retention Time
DDT	316652	13.586
DDD	4196	13.286
DDE	505	12.951
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4701	321353	1.46

Instrument :
BNA_F
ClientSampleId :
DFTPP