


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF060519\
 Data File : BF114806.D
 Acq On : 5 Jun 2019 8:29
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF060419.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jun 04 16:57:15 2019

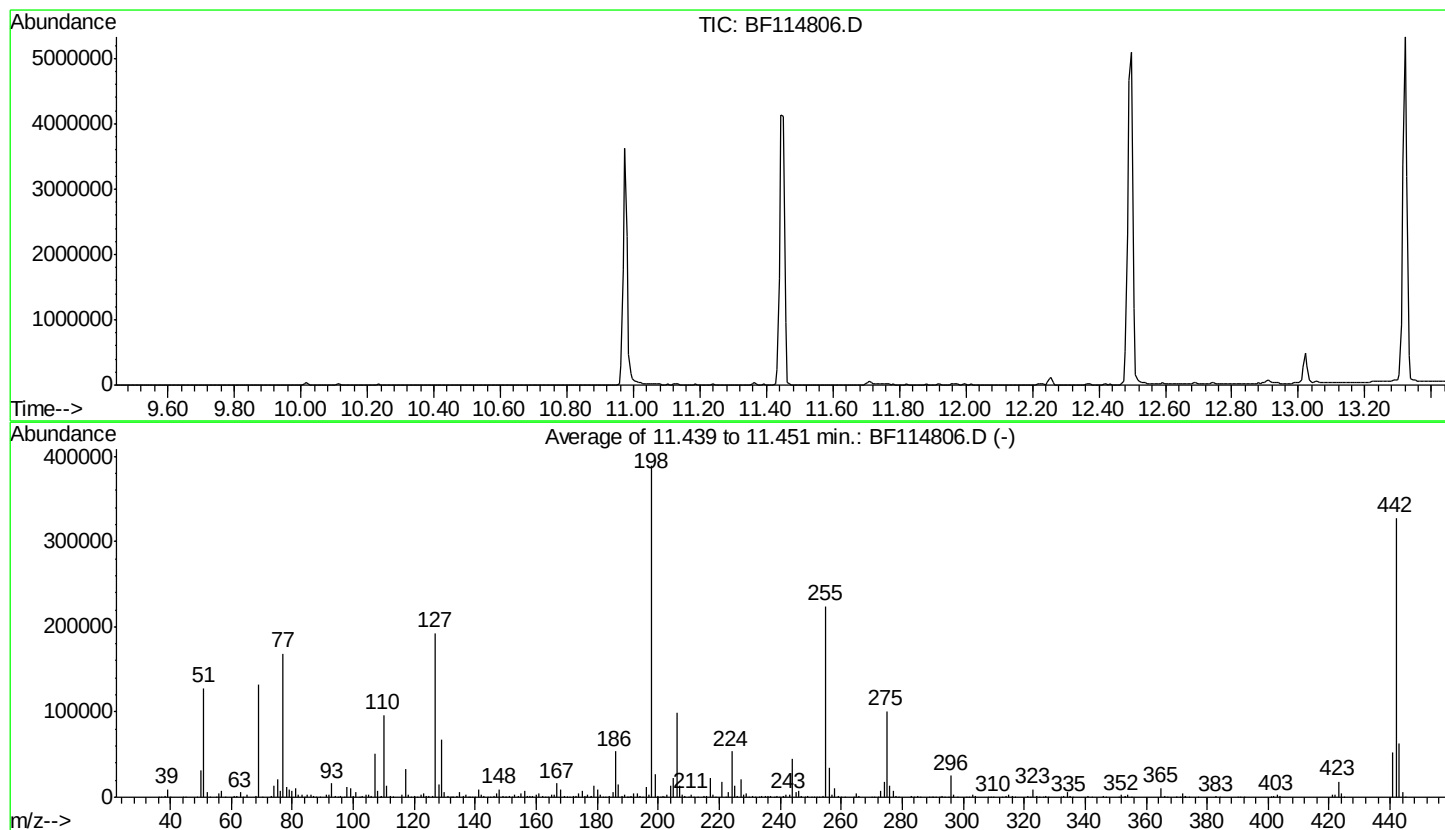

AutoFind: Scans 1590, 1591, 1592; Background Corrected with Scan 1585

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	128314	PASS
68	69	0.00	2	1.7	2258	PASS
69	198	0.00	100	33.8	131488	PASS
70	69	0.00	2	0.6	783	PASS
127	198	10	80	49.5	192442	PASS
197	198	0.00	2	0.6	2371	PASS
198	198	100	100	100.0	388970	PASS
199	198	5	9	6.8	26578	PASS
275	198	10	60	26.1	101357	PASS
365	198	1	100	2.9	11281	PASS
441	198	0.01	100	13.4	52127	PASS
442	198	50	100	84.2	327650	PASS
443	442	15	24	19.1	62429	PASS